
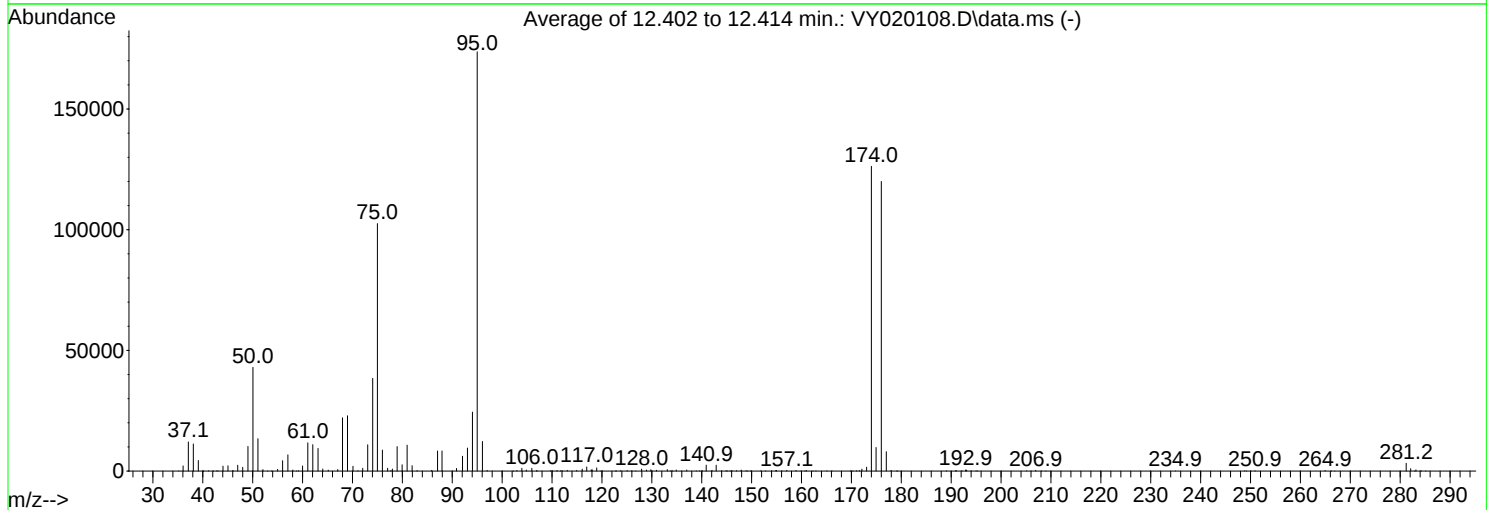


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110124\
Data File : VY020108.D
Acq On : 01 Nov 2024 08:26
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Title : SW846 8260
Last Update : Thu Oct 31 15:23:13 2024

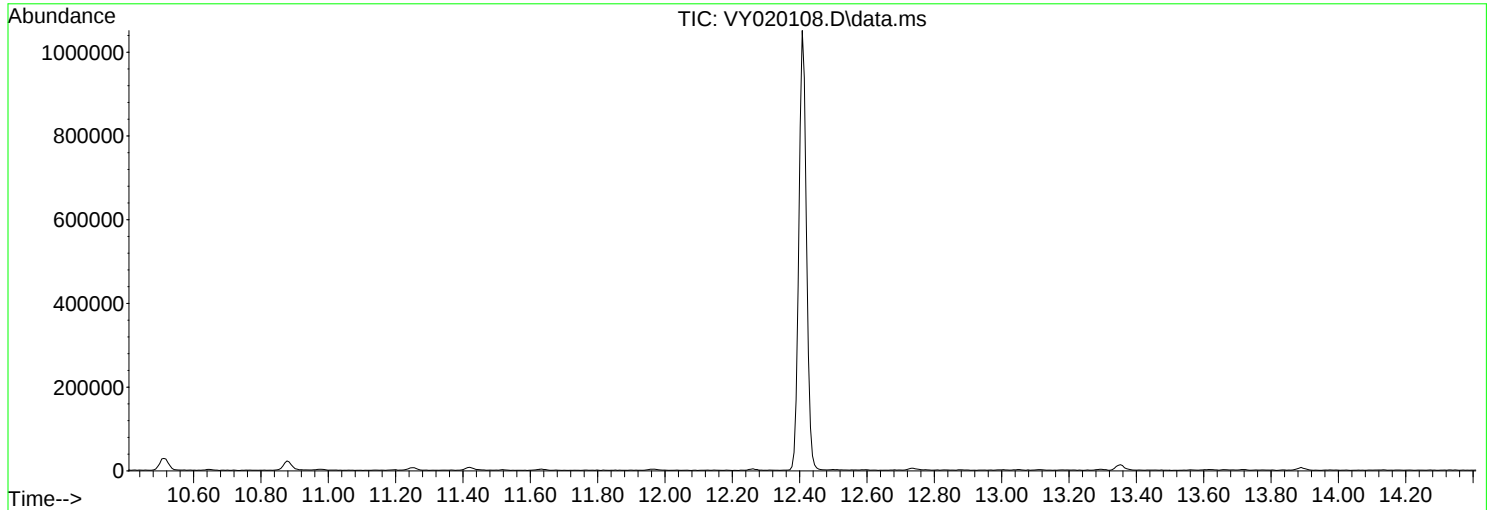

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	42973	PASS
75	95	30	60	59.0	102539	PASS
95	95	100	100	100.0	173739	PASS
96	95	5	9	7.1	12286	PASS
173	174	0.00	2	1.3	1619	PASS
174	95	50	100	72.7	126267	PASS
175	174	5	9	7.8	9797	PASS
176	174	95	101	95.0	119995	PASS
177	176	5	9	6.7	8034	PASS