

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110422\
 Data File : VY011319.D
 Acq On : 04 Nov 2022 23:34
 Operator : KP/MD
 Sample : N5436-10
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 250FERRYBLVD-TFS-10

Quant Time: Nov 07 01:57:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 01 11:56:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.79
34) 1,4-Difluorobenzene	0.000	114	0	0.000	ug/l	-8.69
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.42
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/l	
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount	50.000	Range	54 - 147	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0	0.000	ug/l	
Spiked Amount	50.000	Range	49 - 140	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	25 - 144	Recovery	=	0.000%#


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110422\
Data File : VY011319.D
Acq On : 04 Nov 2022 23:34
Operator : KP/MD
Sample : N5436-10
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-10

Quant Time: Nov 07 01:57:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 01 11:56:18 2022
Response via : Initial Calibration

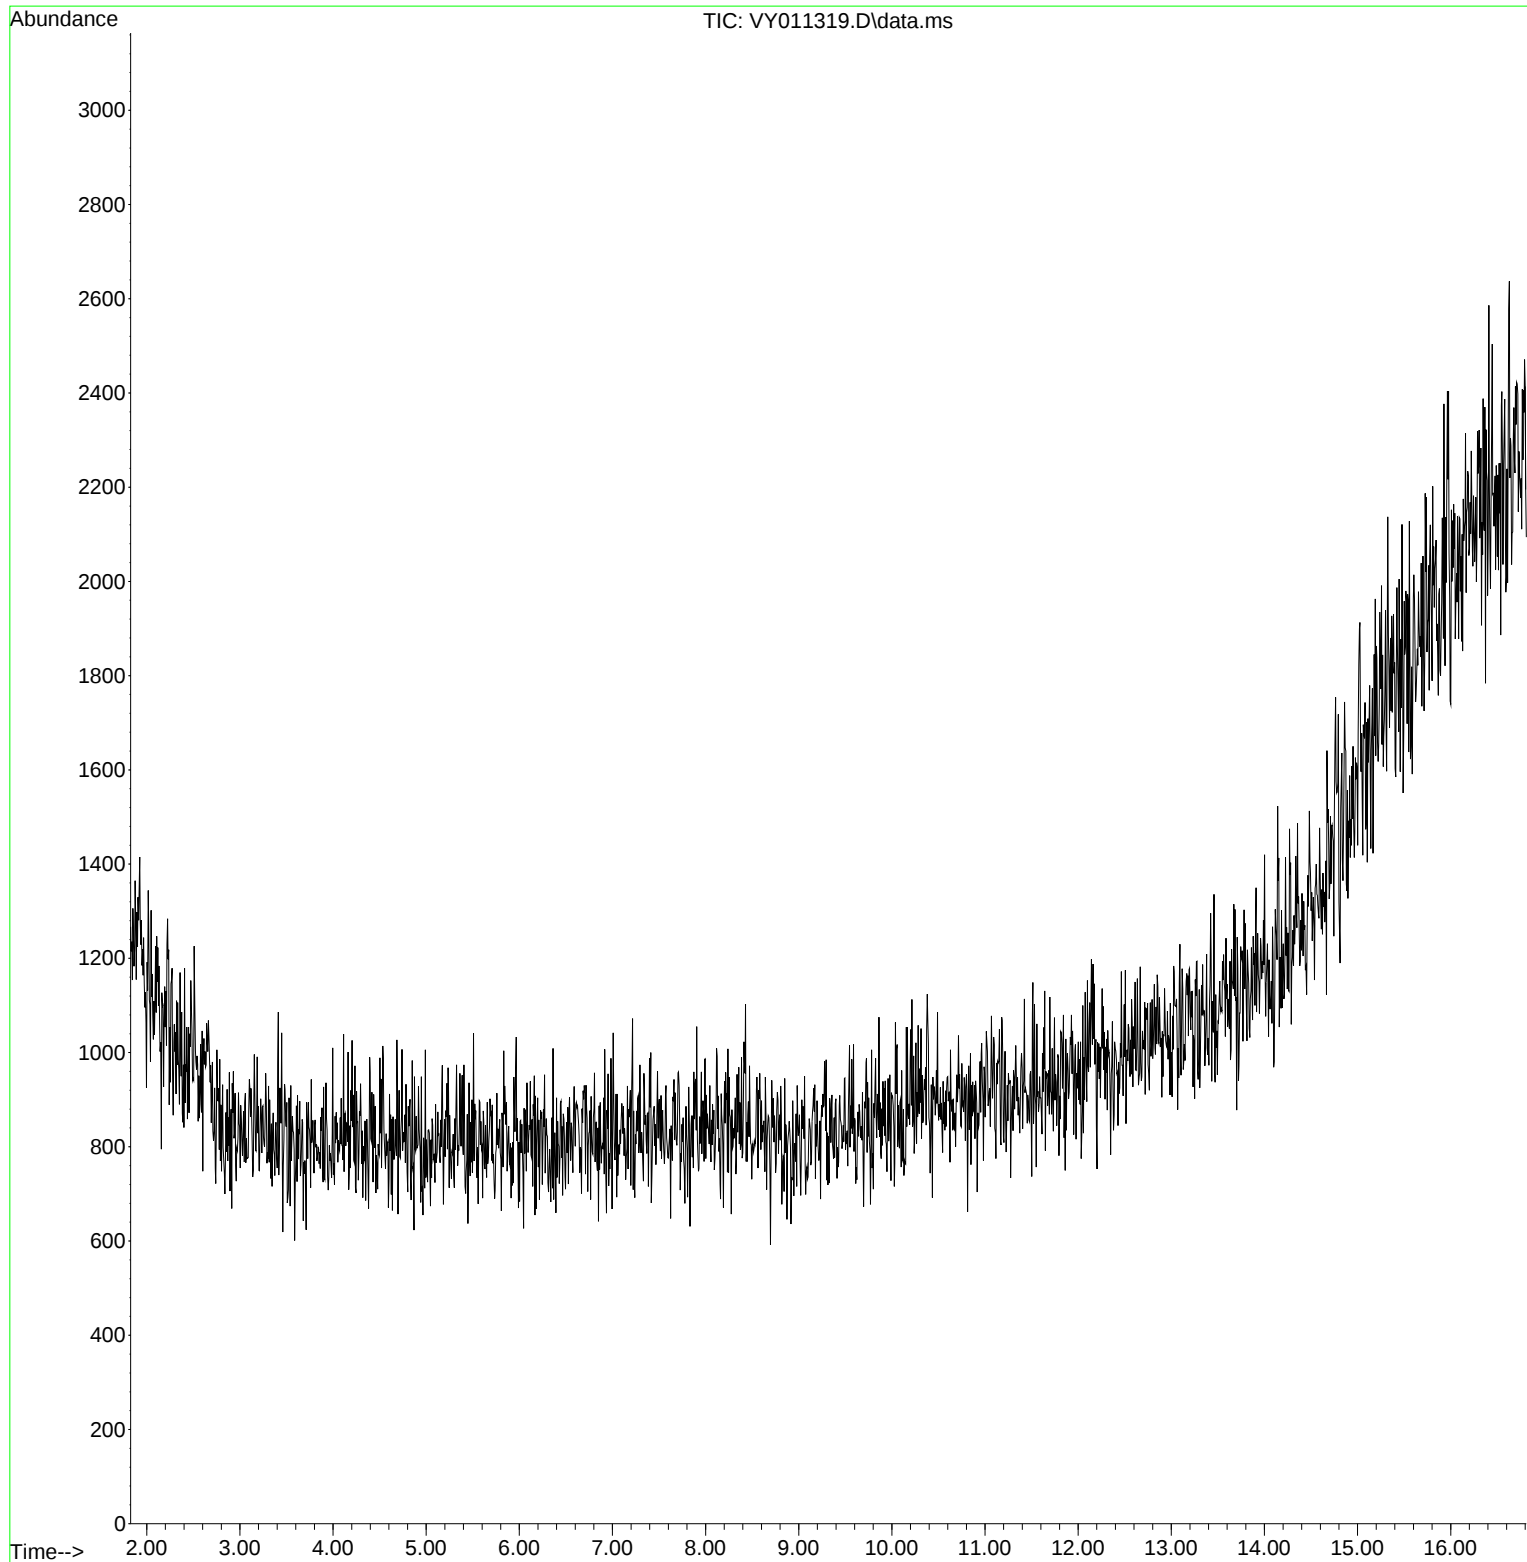


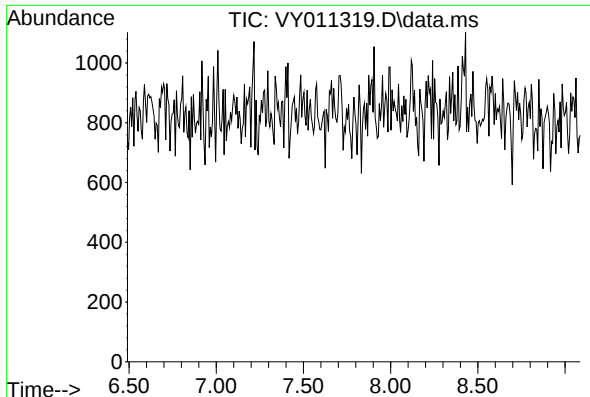


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.79 min

Lab File: VY011319.D
Acq: 04 Nov 2022 23:34

Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-10


Tgt Ion: 168
Sig Exp Ratio
168 100
99 58.6

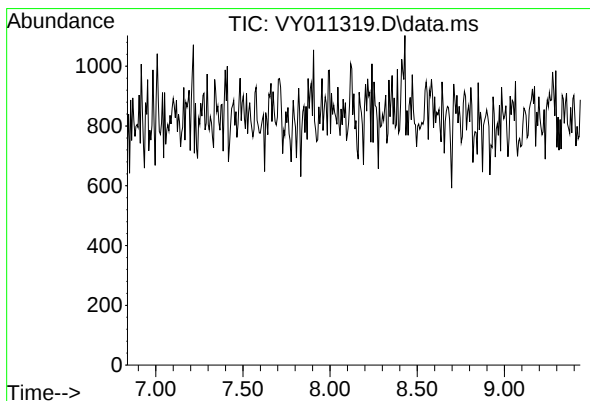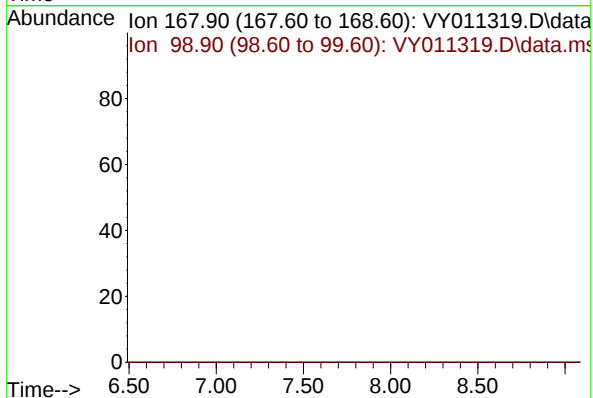


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.14 min

Lab File: VY011319.D
Acq: 04 Nov 2022 23:34

Tgt Ion: 65
Sig Exp Ratio
65 100
67 49.7

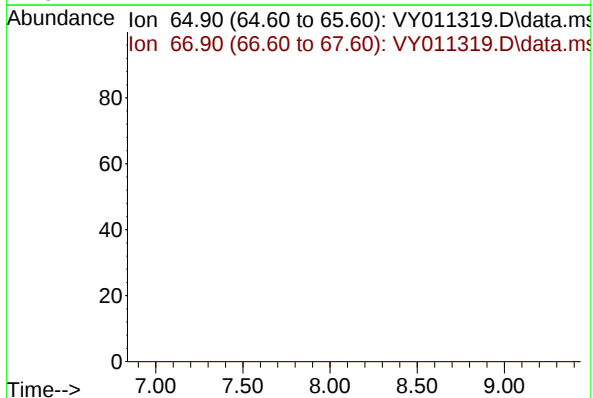


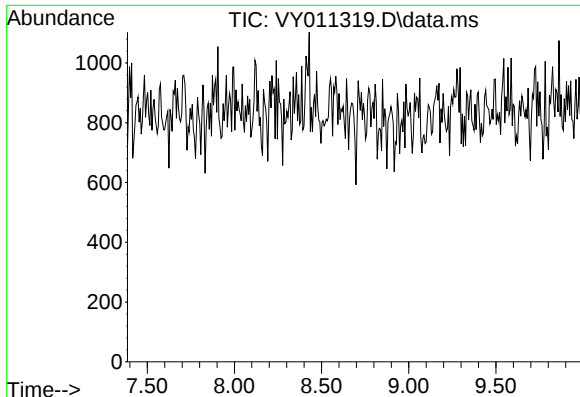


#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.69 min
 Lab File: VY011319.D
 Acq: 04 Nov 2022 23:34

Instrument :
 MSVOA_Y
 ClientSampleId :
 250FERRYBLVD-TFS-10

Tgt Ion: 114


Sig	Exp Ratio
114	100
63	21.6
88	15.9

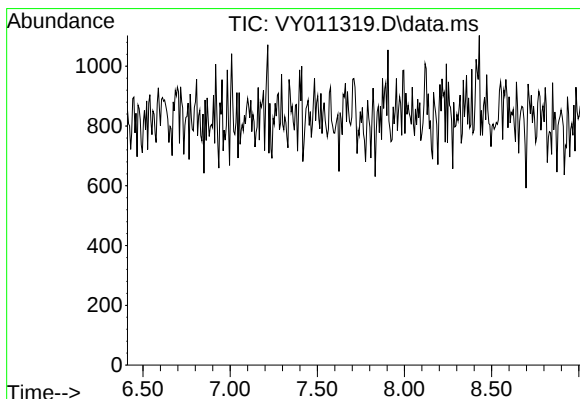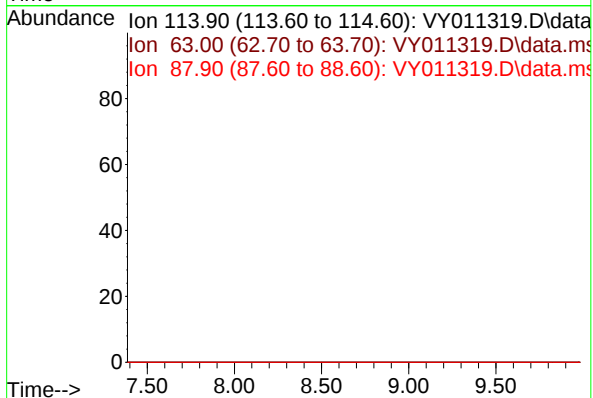


#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.71 min
 Lab File: VY011319.D
 Acq: 04 Nov 2022 23:34

Tgt Ion: 113

Sig	Exp Ratio
113	100
111	103.3
192	22.0

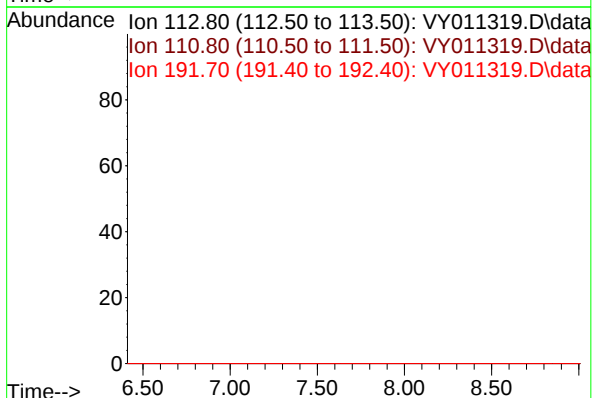


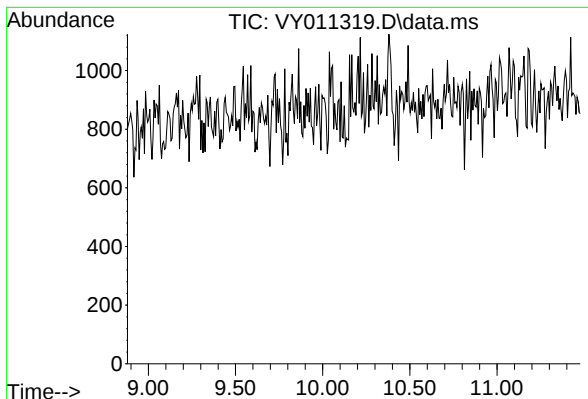


#50
 Toluene-d8
 Concen: 0.000 ug/l
 Expected RT: 10.18 min

Lab File: VY011319.D
 Acq: 04 Nov 2022 23:34

Tgt Ion: 98
 Sig Exp Ratio
 98 100
 100 62.7


Instrument :
 MSVOA_Y
 ClientSampleId :
 250FERRYBLVD-TFS-10

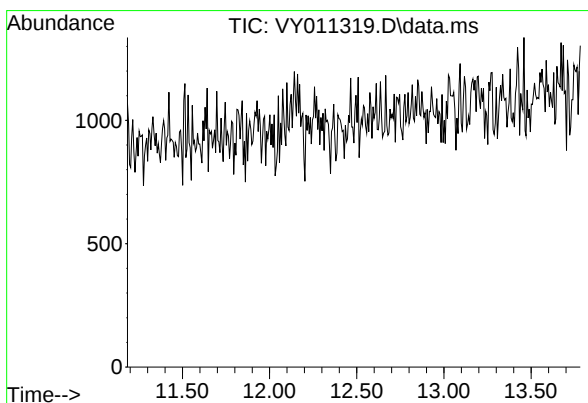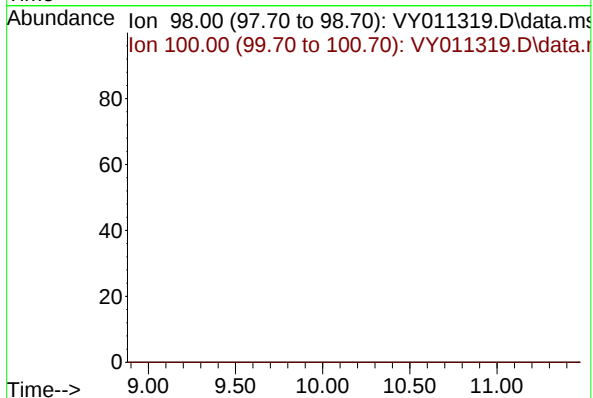


#62
 4-Bromofluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 12.48 min

Lab File: VY011319.D
 Acq: 04 Nov 2022 23:34

Tgt Ion: 95
 Sig Exp Ratio
 95 100
 174 88.5
 176 87.9

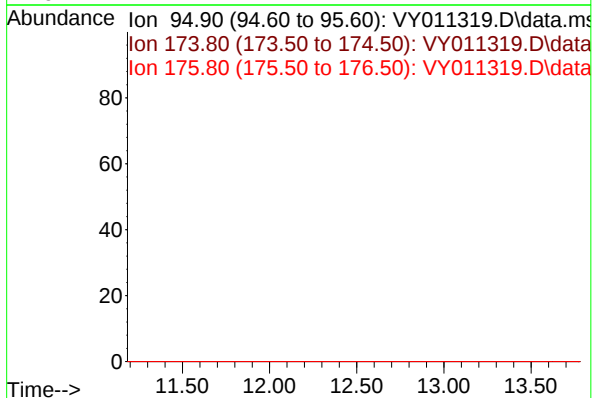


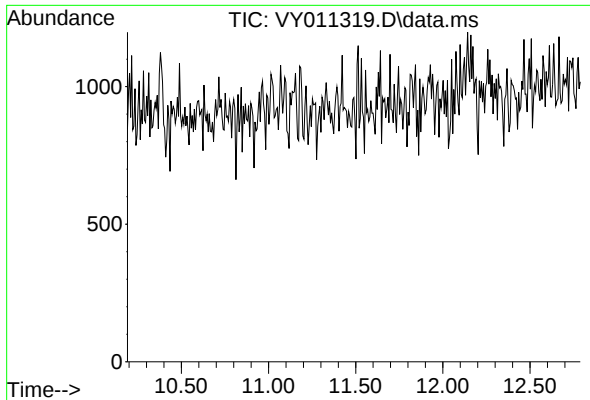


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.49 min

Lab File: VY011319.D
Acq: 04 Nov 2022 23:34

Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-10

Tgt Ion: 117
Sig Exp Ratio
117 100
82 53.7
119 31.7

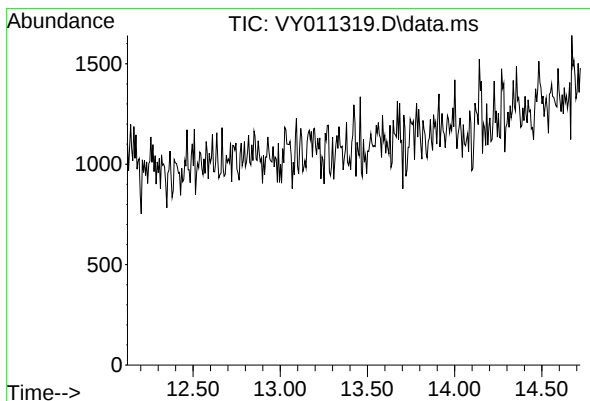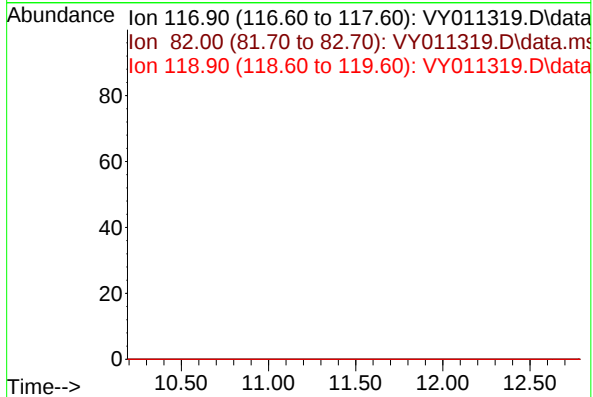

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.42 min

Lab File: VY011319.D
Acq: 04 Nov 2022 23:34

Tgt Ion: 152
Sig Exp Ratio
152 100
115 56.5
150 173.8

