
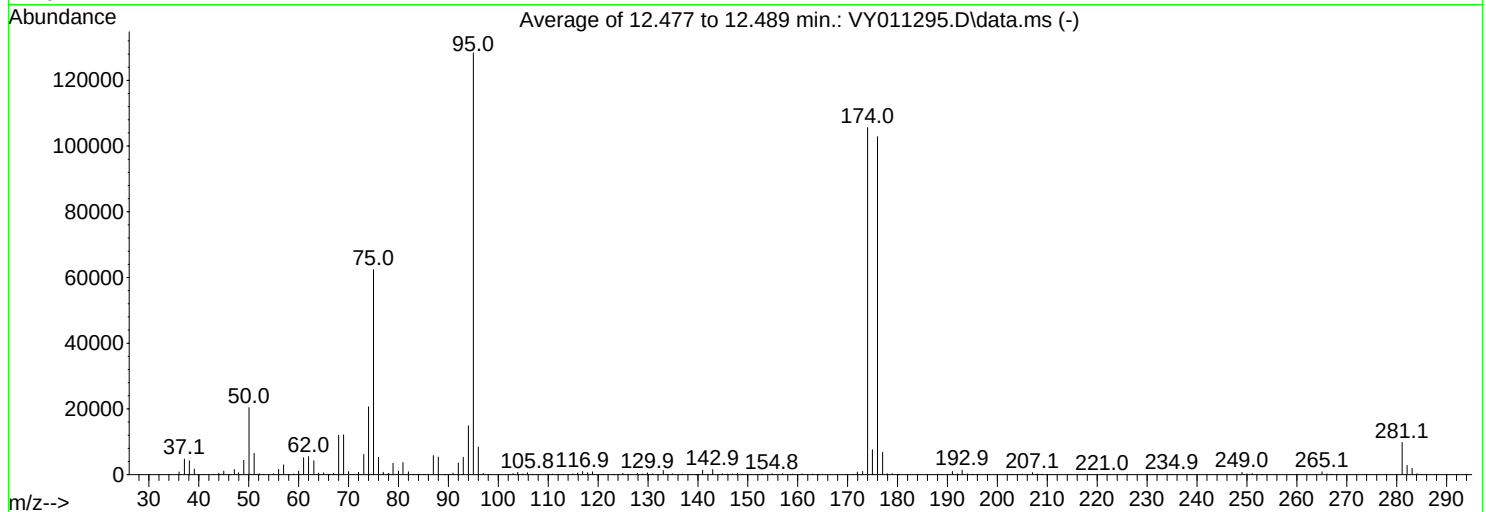


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110422\
 Data File : VY011295.D
 Acq On : 04 Nov 2022 13:15
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Title : SW846 8260
 Last Update : Tue Nov 01 11:56:18 2022

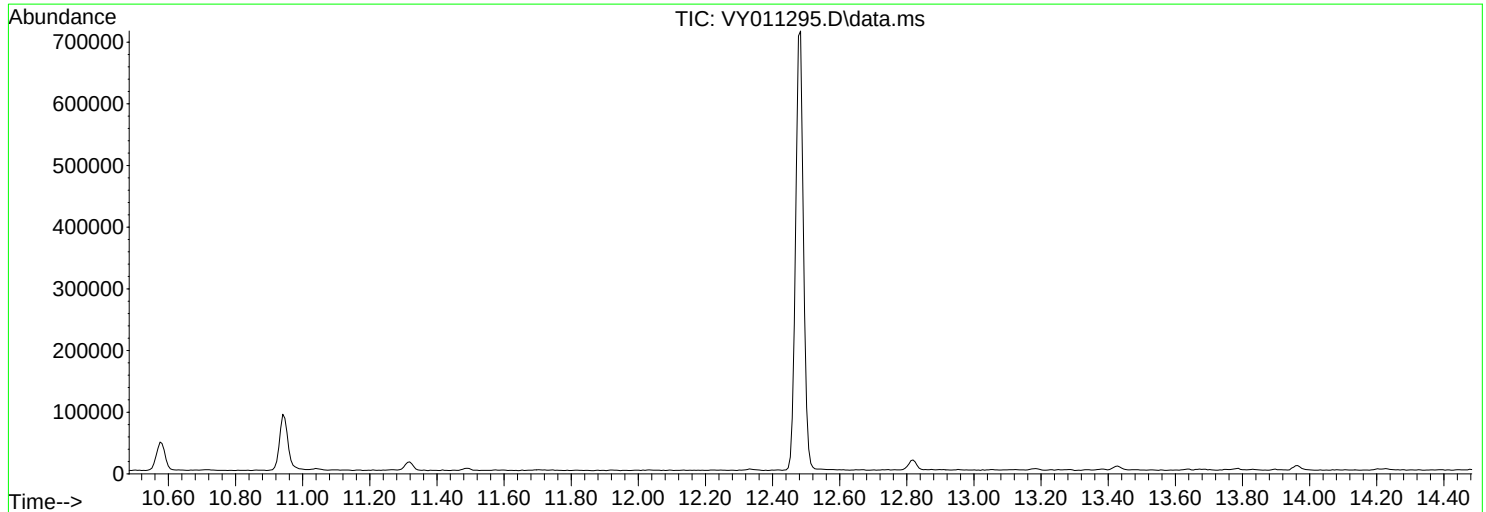

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	20386	PASS
75	95	30	60	48.6	62397	PASS
95	95	100	100	100.0	128376	PASS
96	95	5	9	6.6	8428	PASS
173	174	0.00	2	0.9	978	PASS
174	95	50	100	82.3	105648	PASS
175	174	5	9	7.2	7605	PASS
176	174	95	101	97.4	102856	PASS
177	176	5	9	6.6	6786	PASS