
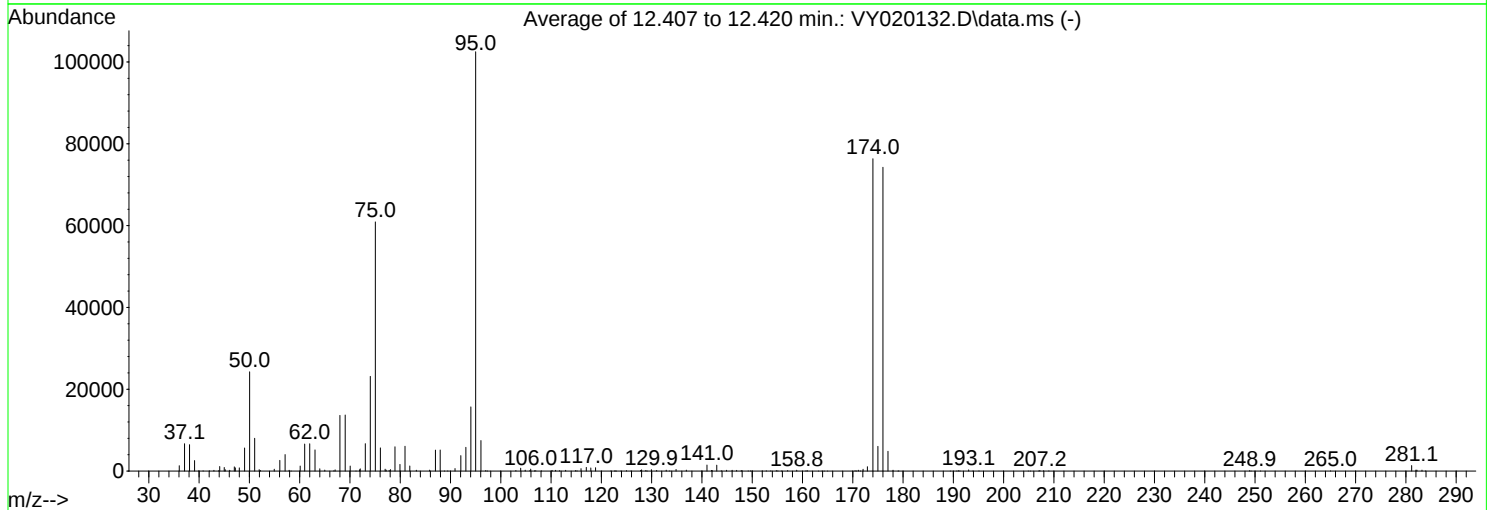


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110424\
Data File : VY020132.D
Acq On : 04 Nov 2024 08:51
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y103024S.M
Title : SW846 8260
Last Update : Thu Oct 31 15:23:13 2024

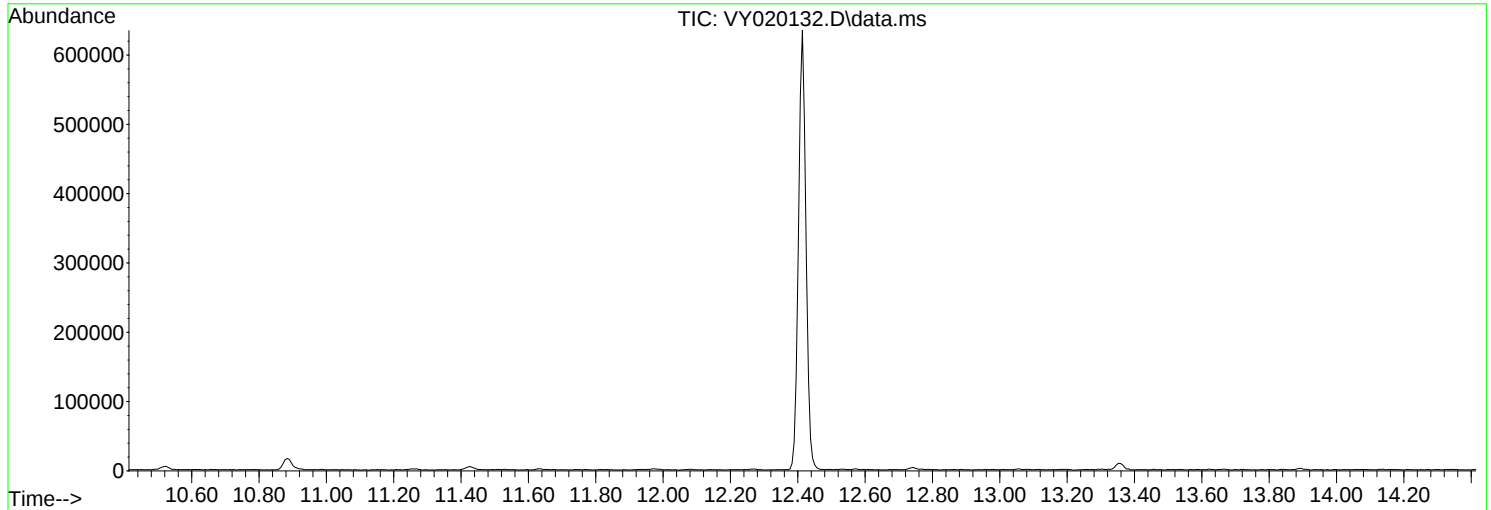

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	24264	PASS
75	95	30	60	59.4	60915	PASS
95	95	100	100	100.0	102507	PASS
96	95	5	9	7.3	7466	PASS
173	174	0.00	2	1.4	1070	PASS
174	95	50	100	74.5	76349	PASS
175	174	5	9	7.9	6044	PASS
176	174	95	101	97.3	74261	PASS
177	176	5	9	6.5	4839	PASS