

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110521\
 Data File : VY006666.D
 Acq On : 05 Nov 2021 19:04
 Operator : SY/MD
 Sample : M4477-11
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 T5-B2-NW

Quant Time: Nov 06 20:42:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
 Quant Title : SW846 8260
 QLast Update : Sat Oct 23 06:59:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	36347	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	55047	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	46633	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	15389	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	21090	47.152	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.300%
35) Dibromofluoromethane	7.728	113	16728	54.521	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.040%
50) Toluene-d8	10.185	98	67435	51.848	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.700%
62) 4-Bromofluorobenzene	12.483	95	17353	39.607	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	79.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110521\
Data File : VY006666.D
Acq On : 05 Nov 2021 19:04
Operator : SY/MD
Sample : M4477-11
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
T5-B2-NW

Quant Time: Nov 06 20:42:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y102221S.M
Quant Title : SW846 8260
QLast Update : Sat Oct 23 06:59:04 2021
Response via : Initial Calibration




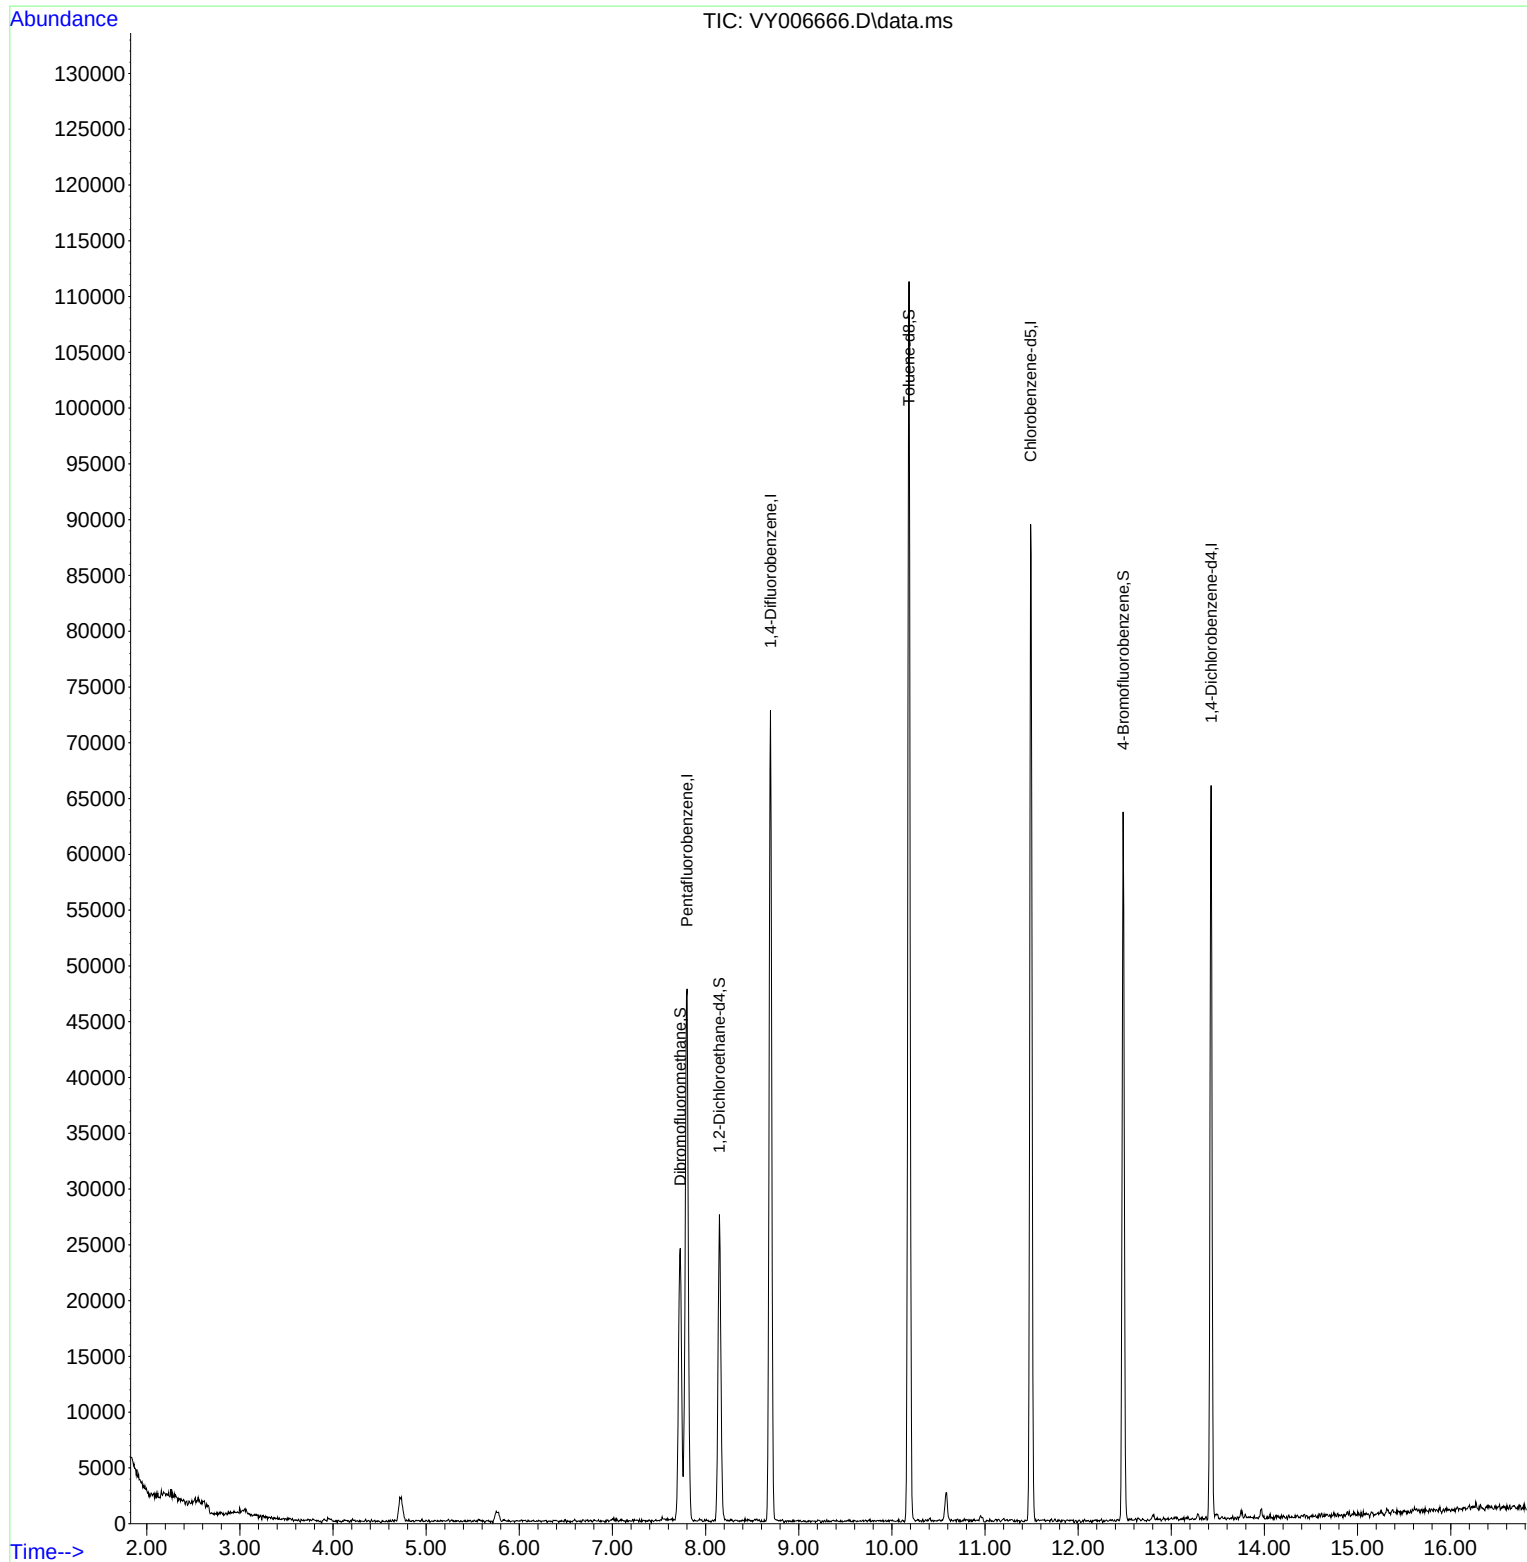


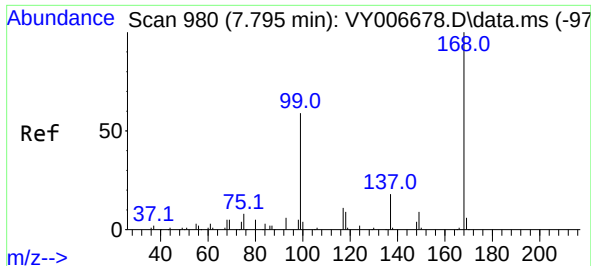

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04




Instrument :
MSVOA_Y
ClientSampleId :
T5-B2-NW


Tgt Ion:168 Resp: 36347
Ion Ratio Lower Upper
168 100
99 54.3 44.8 67.2

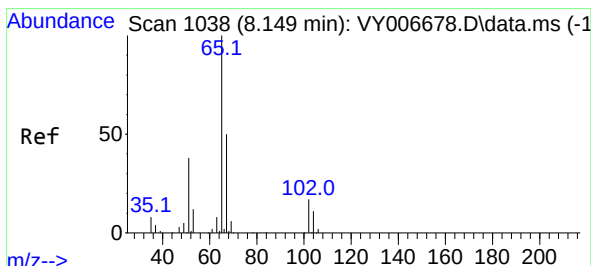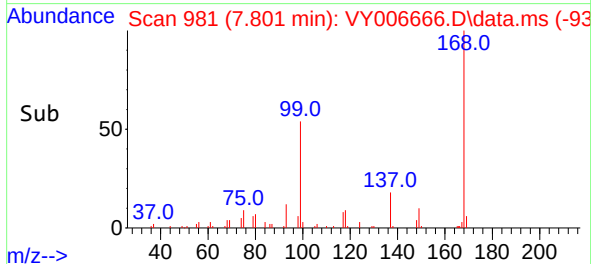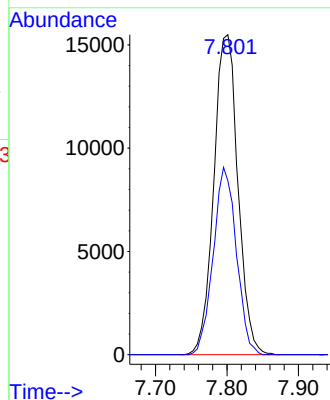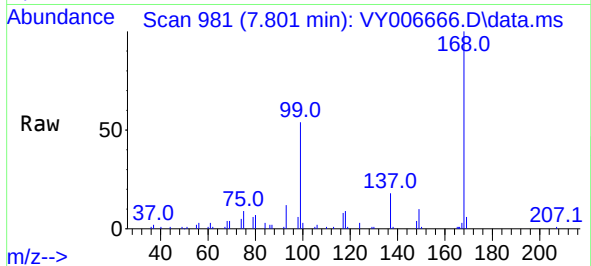

#33
1,2-Dichloroethane-d4
Concen: 47.152 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04

Tgt Ion: 65 Resp: 21090
Ion Ratio Lower Upper
65 100
67 52.3 0.0 98.2

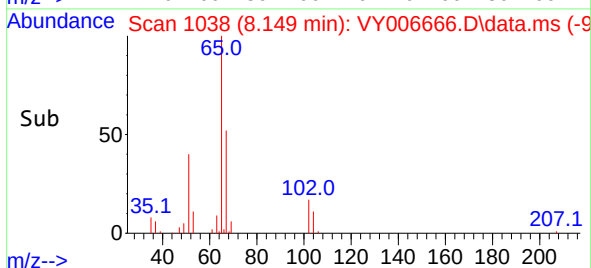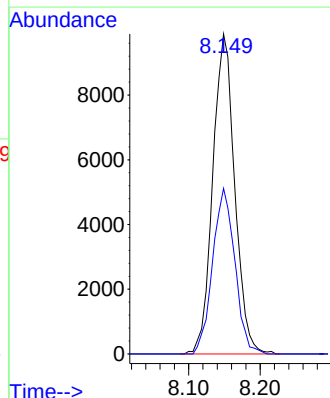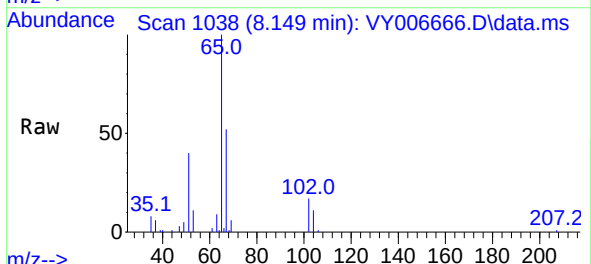

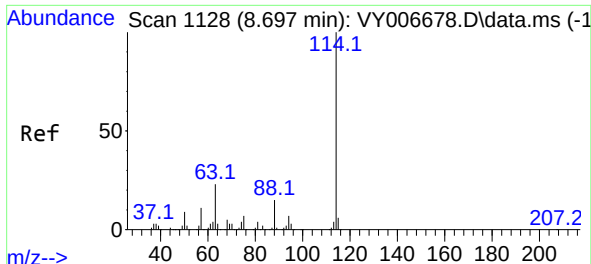

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.697 min Scan# 1128

Delta R.T. 0.000 min

Lab File: VY006666.D

Acq: 05 Nov 2021 19:04

Instrument :

MSVOA_Y

ClientSampleId :

T5-B2-NW





Tgt Ion:114 Resp: 55047

Ion Ratio Lower Upper

114 100

63 23.3 0.0 45.0

88 15.5 0.0 30.6

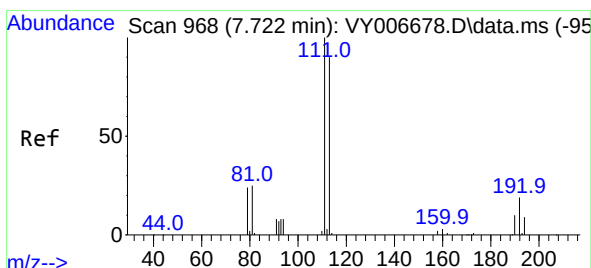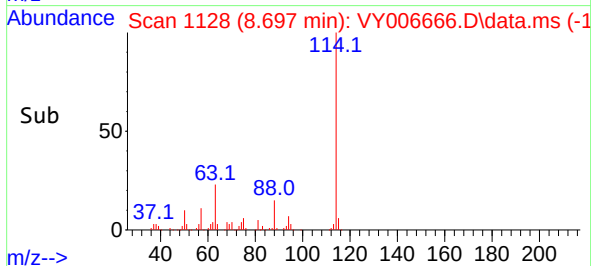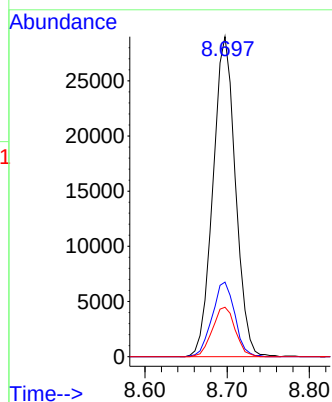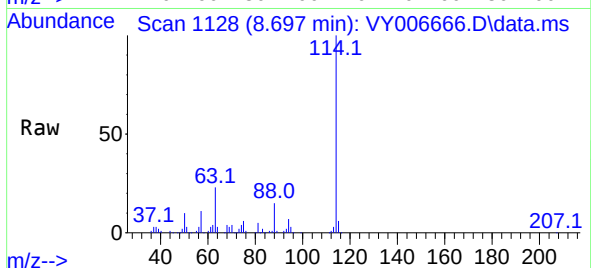

#35

Dibromofluoromethane

Concen: 54.521 ug/l

RT: 7.728 min Scan# 969

Delta R.T. 0.006 min

Lab File: VY006666.D

Acq: 05 Nov 2021 19:04




Tgt Ion:113 Resp: 16728


Ion Ratio Lower Upper

113 100

111 101.9 82.3 123.5

192 20.7 17.4 26.2


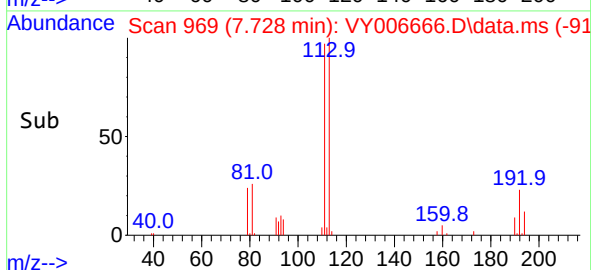
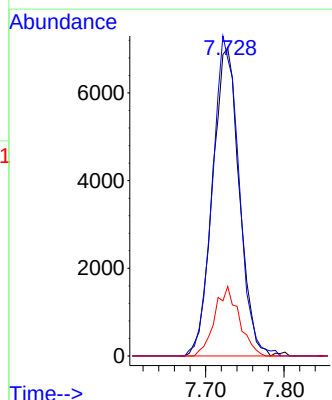
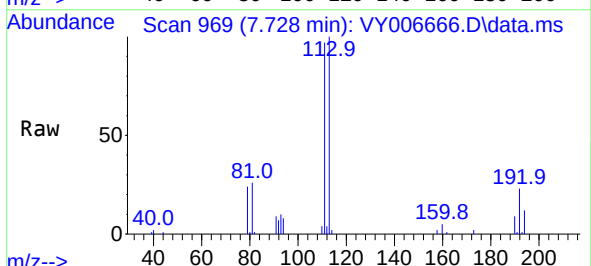


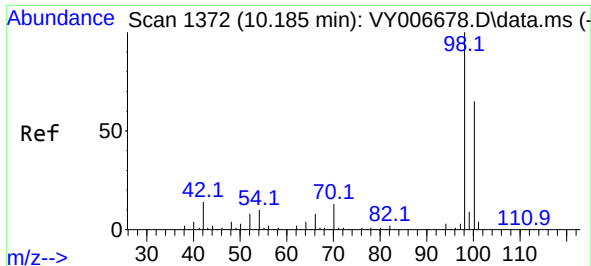

#50
Toluene-d8
Concen: 51.848 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04




Instrument :
MSVOA_Y
ClientSampleId :
T5-B2-NW


Tgt Ion: 98 Resp: 67435
Ion Ratio Lower Upper
98 100
100 64.0 50.9 76.3

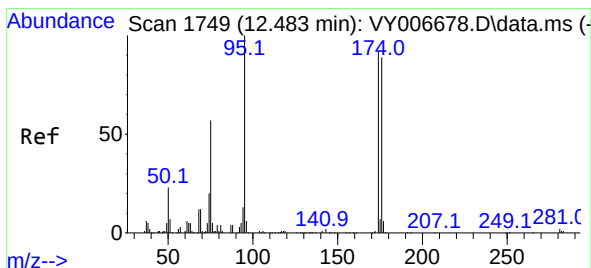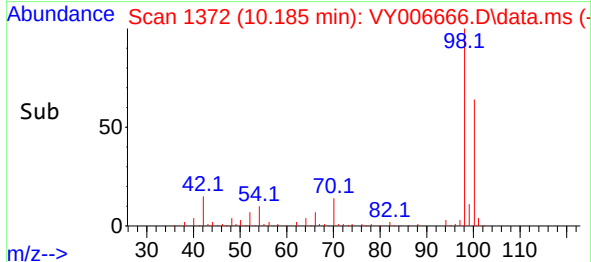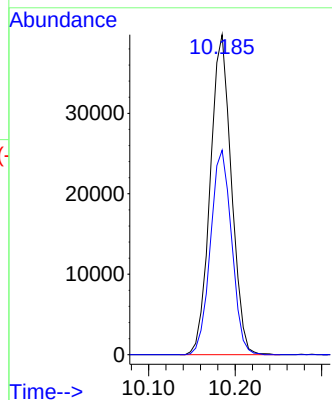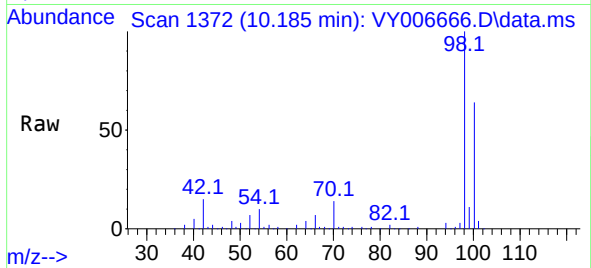

#62
4-Bromofluorobenzene
Concen: 39.607 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04

Tgt Ion: 95 Resp: 17353
Ion Ratio Lower Upper
95 100
174 94.2 0.0 177.0
176 89.9 0.0 169.4


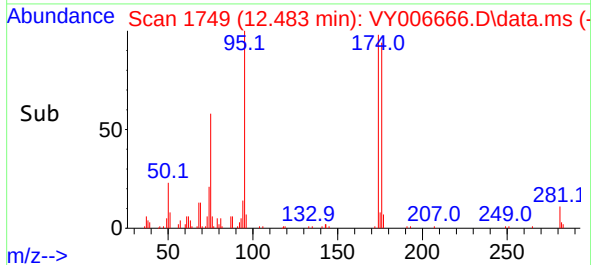
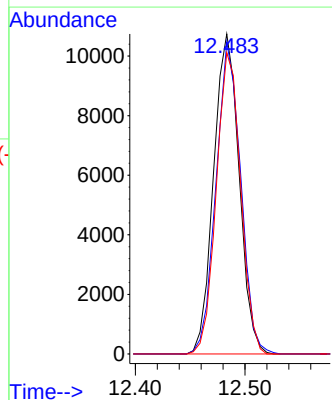
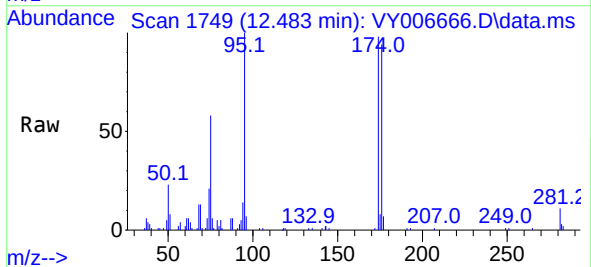


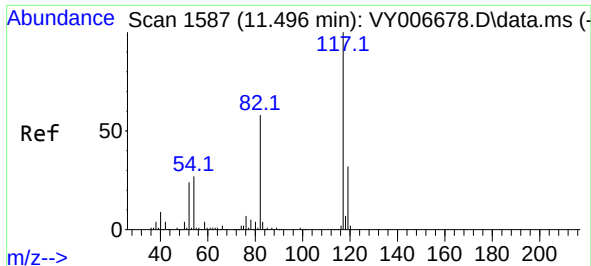

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04

Instrument :
MSVOA_Y
ClientSampleId :
T5-B2-NW

Tgt Ion:	117	Resp:	46633
Ion	Ratio	Lower	Upper
117	100		
82	56.5	45.7	68.5
119	31.0	25.5	38.3

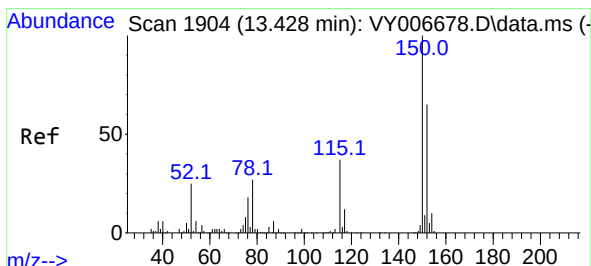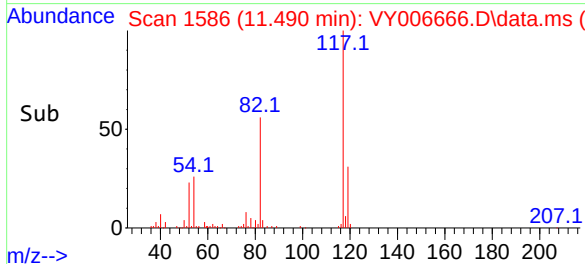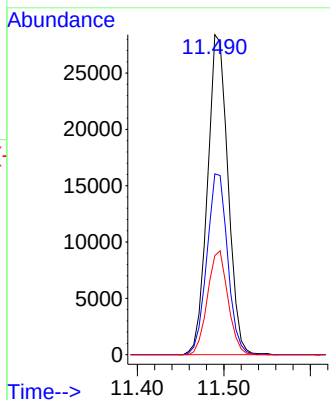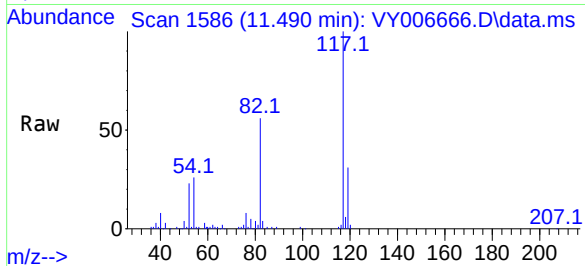

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY006666.D
Acq: 05 Nov 2021 19:04

Tgt Ion:	152	Resp:	15389
Ion	Ratio	Lower	Upper
152	100		
115	57.1	28.5	85.5
150	159.6	0.0	348.2

