
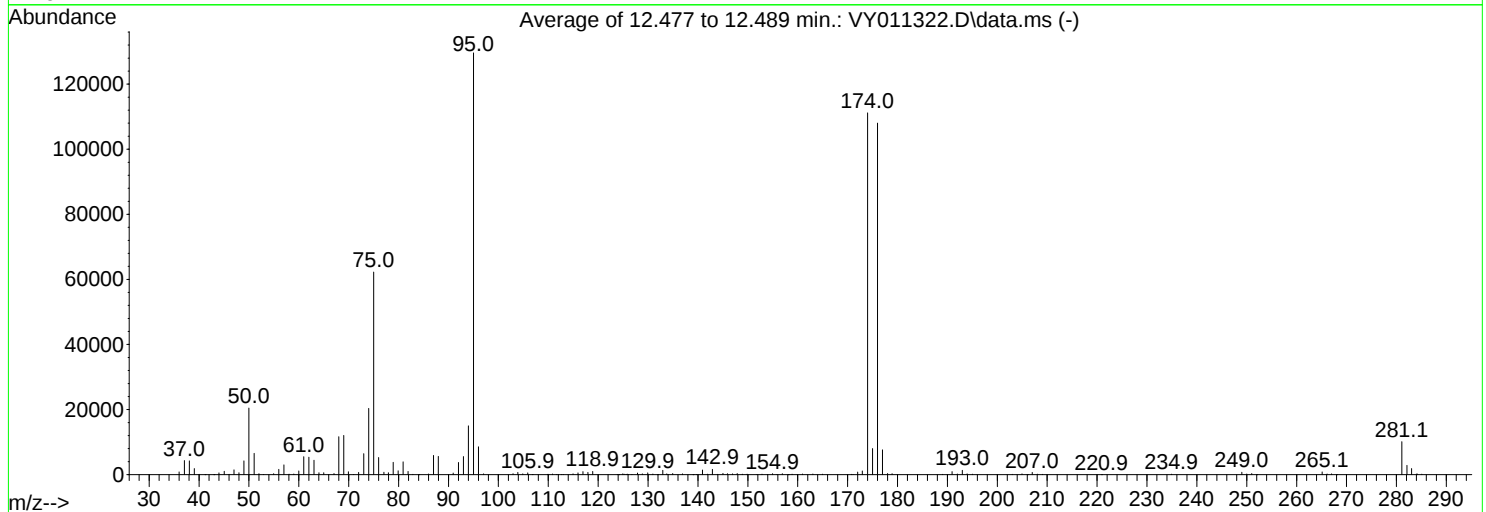


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110722\
Data File : VY011322.D
Acq On : 07 Nov 2022 09:10
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Title : SW846 8260
Last Update : Tue Nov 01 11:56:18 2022

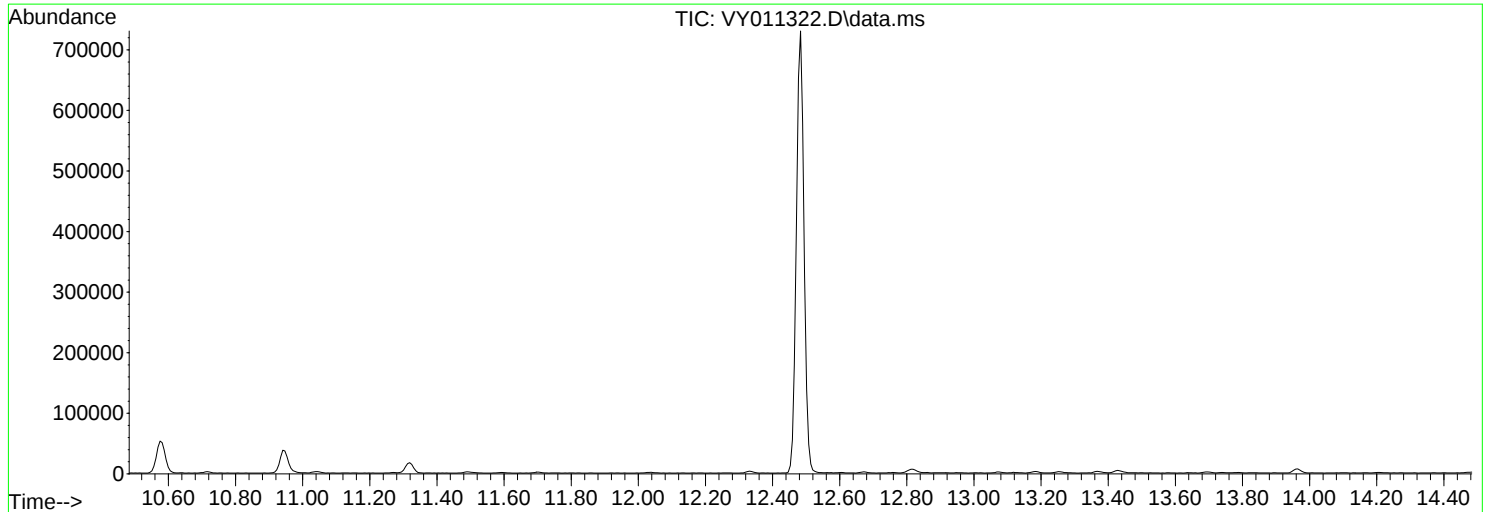

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	20437	PASS
75	95	30	60	48.0	62243	PASS
95	95	100	100	100.0	129616	PASS
96	95	5	9	6.6	8545	PASS
173	174	0.00	2	1.0	1133	PASS
174	95	50	100	85.8	111176	PASS
175	174	5	9	7.2	8006	PASS
176	174	95	101	97.2	108040	PASS
177	176	5	9	7.1	7633	PASS