

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110822\
 Data File : VY011375.D
 Acq On : 08 Nov 2022 20:13
 Operator : KP/MD
 Sample : N5436-06RE
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 250FERRYBLVD-TFS-06RE

Quant Time: Nov 09 03:35:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 01 11:56:18 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	202002	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	330591	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	274291	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	108260	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	127084	58.824	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	117.640%
35) Dibromofluoromethane	7.716	113	136784	64.398	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	128.800%
50) Toluene-d8	10.179	98	409893	49.704	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.400%
62) 4-Bromofluorobenzene	12.477	95	131276	45.853	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	91.700%
Target Compounds						
20) Methylene Chloride	4.716	84	37170	9.904	ug/l	Qvalue # 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY110822\
Data File : VY011375.D
Acq On : 08 Nov 2022 20:13
Operator : KP/MD
Sample : N5436-06RE
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-06RE

Quant Time: Nov 09 03:35:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y110122S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 01 11:56:18 2022
Response via : Initial Calibration




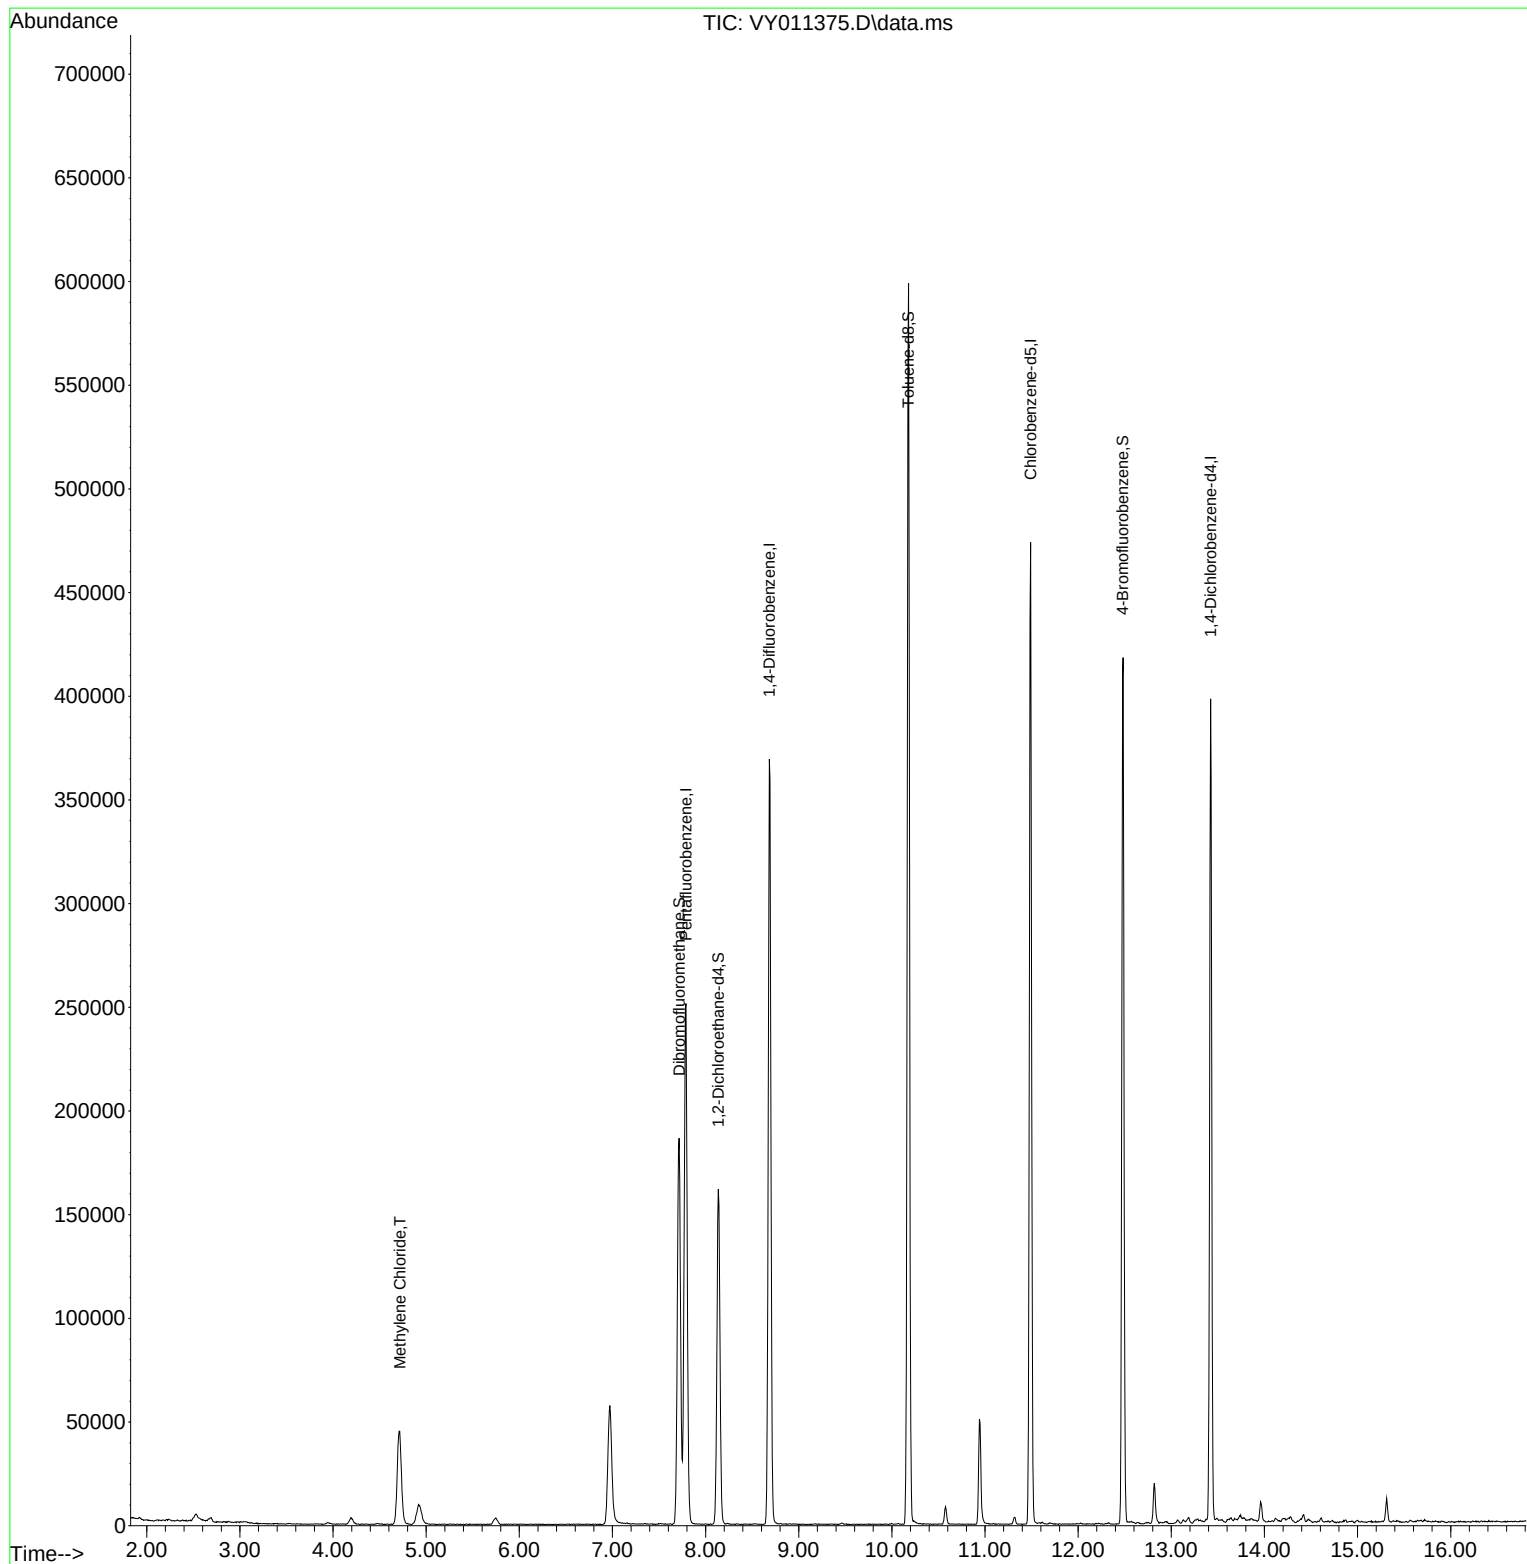


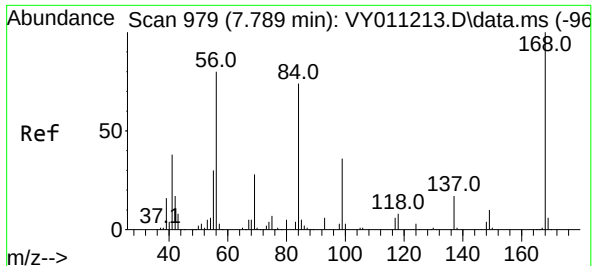

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13




Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-06RE


Tgt Ion:168 Resp: 202002
Ion Ratio Lower Upper
168 100
99 51.8 46.9 70.3

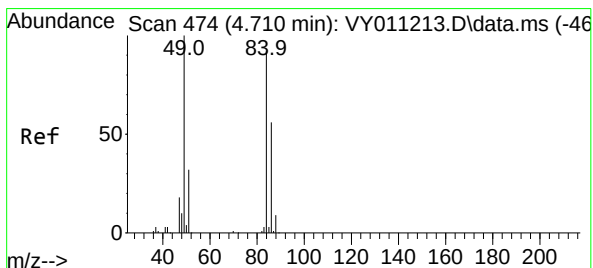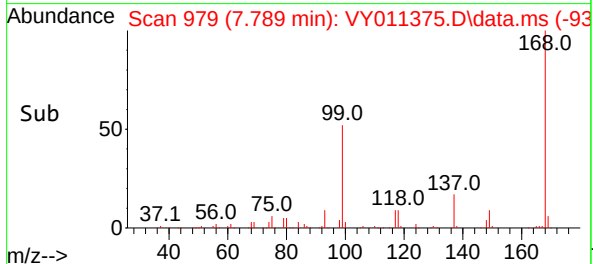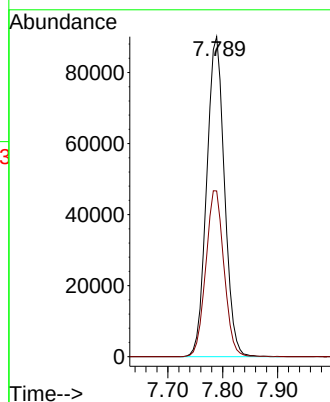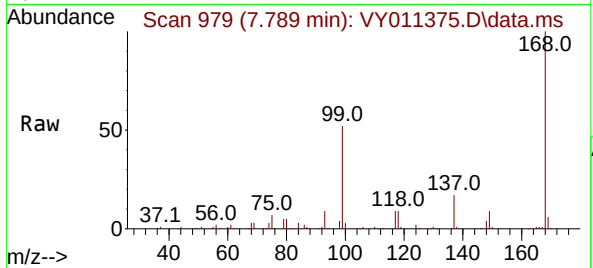

#20
Methylene Chloride
Concen: 9.904 ug/l
RT: 4.716 min Scan# 475
Delta R.T. 0.006 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13

Tgt Ion: 84 Resp: 37170
Ion Ratio Lower Upper
84 100
49 105.4 114.4 171.6#
51 34.3 35.3 52.9#
86 63.0 53.7 80.5

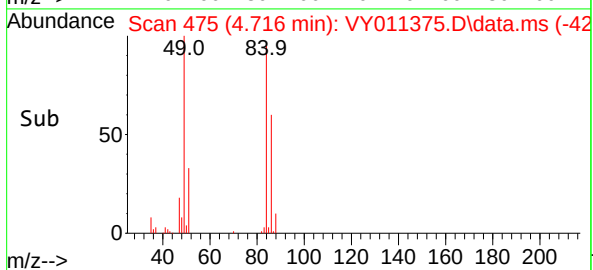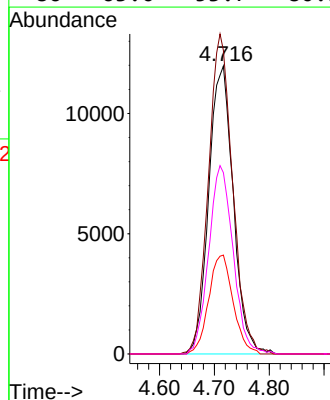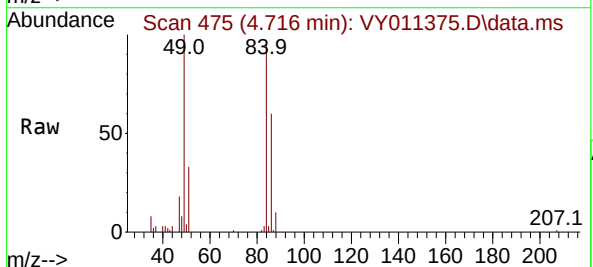

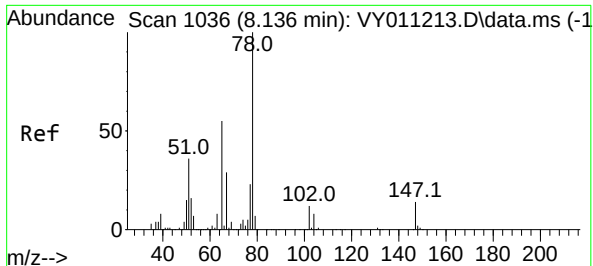

#33

1,2-Dichloroethane-d4

Concen: 58.824 ug/l

RT: 8.136 min Scan# 1103

Delta R.T. 0.000 min

Lab File: VY011375.D

Acq: 08 Nov 2022 20:13

Instrument :

MSVOA_Y

ClientSampleId :





250FERRYBLVD-TFS-06RE

Tgt Ion: 65 Resp: 127084

Ion Ratio Lower Upper

65 100

67 54.3 0.0 99.4

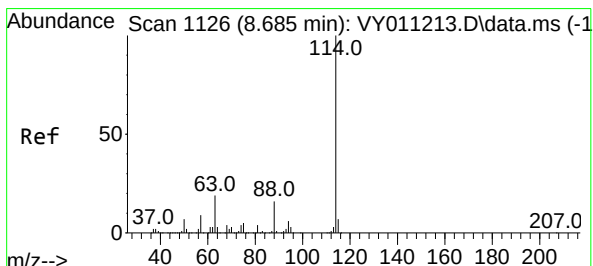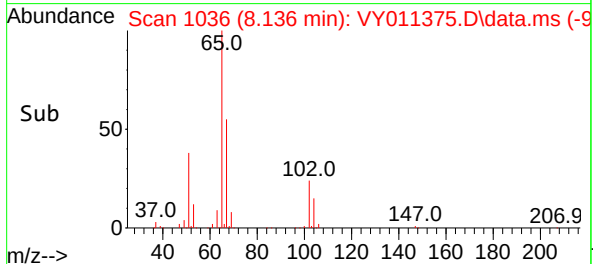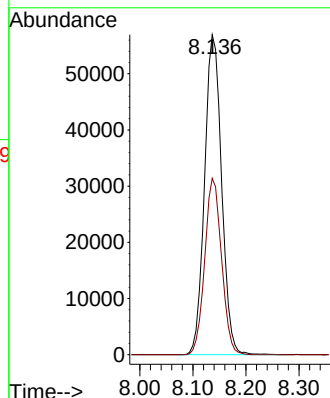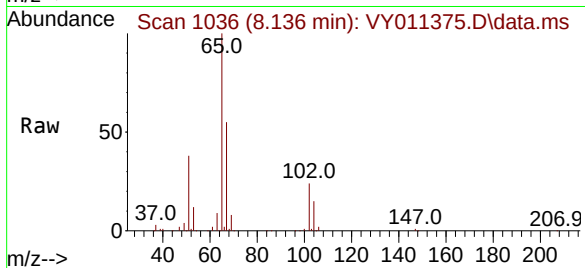

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY011375.D

Acq: 08 Nov 2022 20:13




Tgt Ion: 114 Resp: 330591


Ion Ratio Lower Upper

114 100

63 18.5 0.0 43.2

88 15.2 0.0 31.8


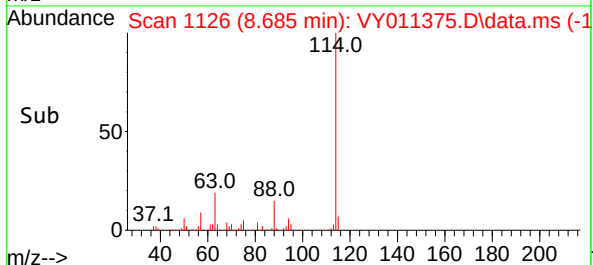
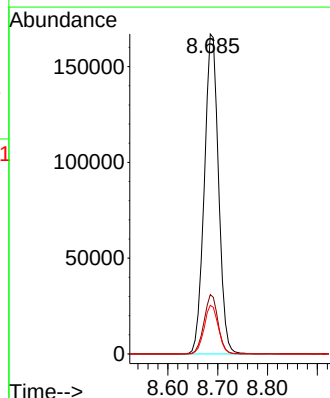
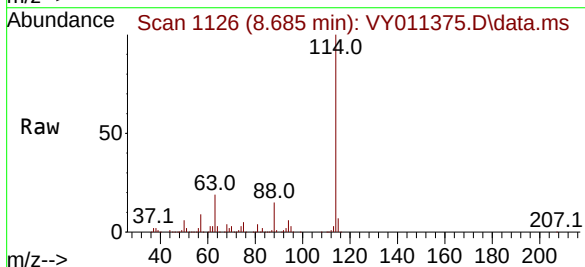


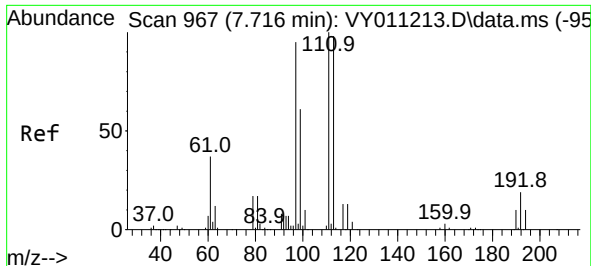

#35
Dibromofluoromethane
Concen: 64.398 ug/l
RT: 7.716 min Scan# 90
Delta R.T. 0.006 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13




Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-06RE


Tgt Ion:113 Resp: 136784
Ion Ratio Lower Upper
113 100
111 102.3 82.6 124.0
192 20.7 17.6 26.4

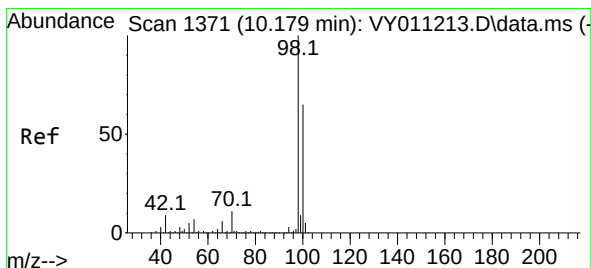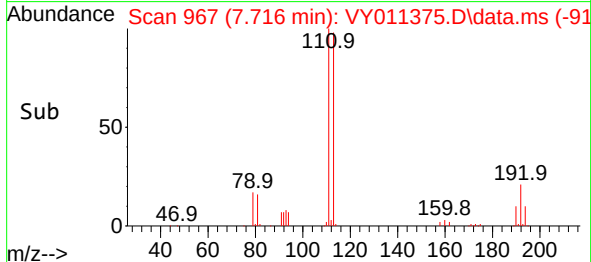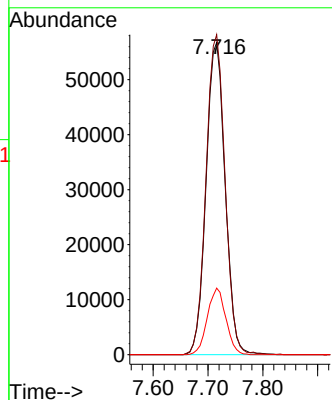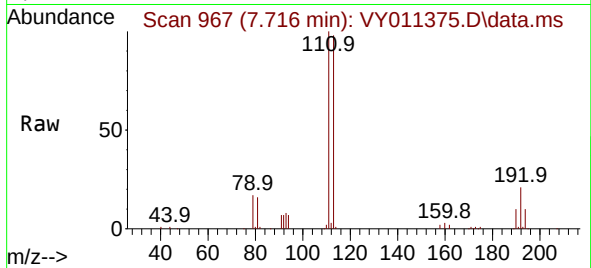

#50
Toluene-d8
Concen: 49.704 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13

Tgt Ion: 98 Resp: 409893
Ion Ratio Lower Upper
98 100
100 64.7 50.2 75.2


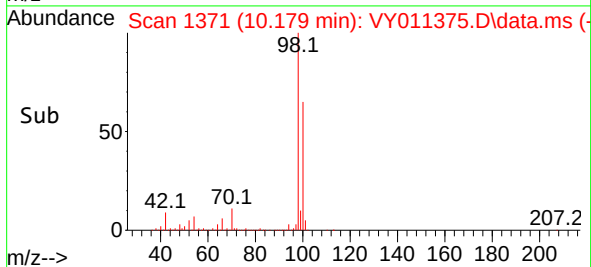
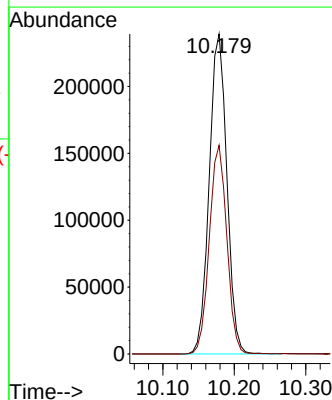
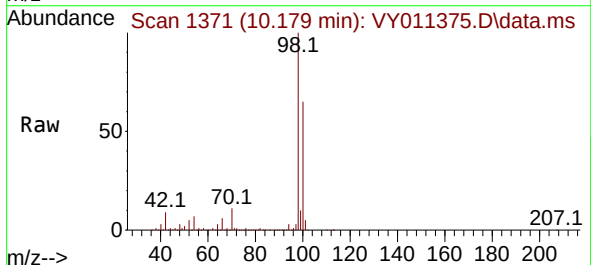


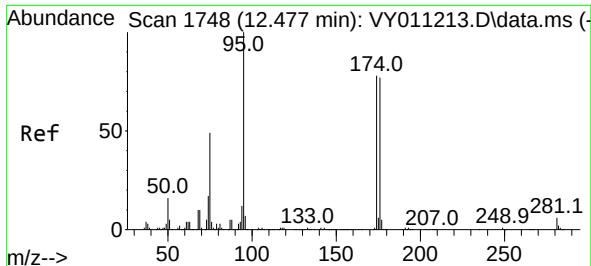

#62
4-Bromofluorobenzene
Concen: 45.853 ug/l
RT: 12.477 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13




Instrument :
MSVOA_Y
ClientSampleId :
250FERRYBLVD-TFS-06RE


Tgt Ion: 95 Resp: 131276
Ion Ratio Lower Upper
95 100
174 87.1 0.0 177.0
176 84.2 0.0 175.8

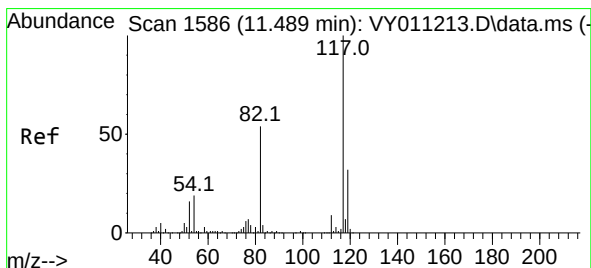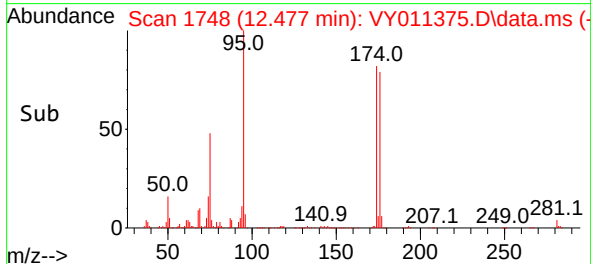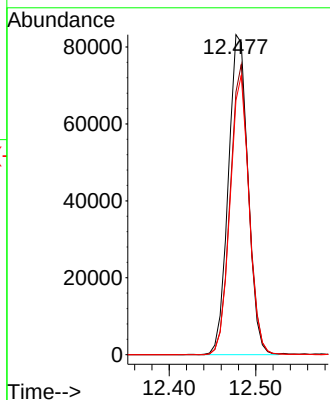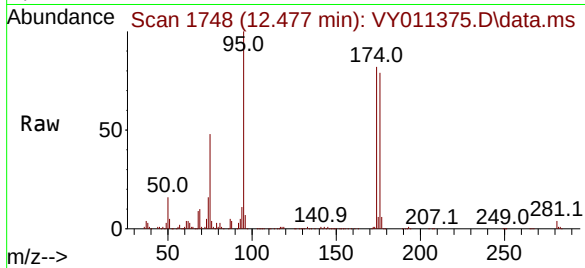

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.001 min
Lab File: VY011375.D
Acq: 08 Nov 2022 20:13

Tgt Ion: 117 Resp: 274291
Ion Ratio Lower Upper
117 100
82 52.1 43.0 64.4
119 32.6 25.4 38.0

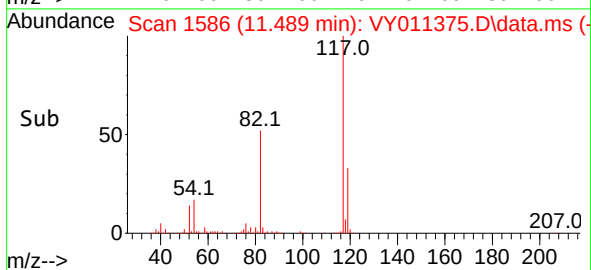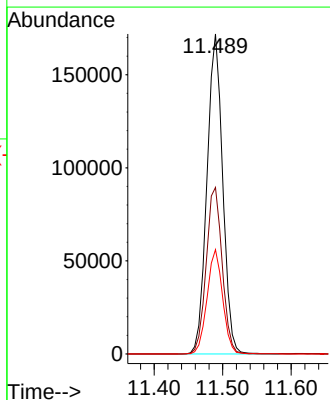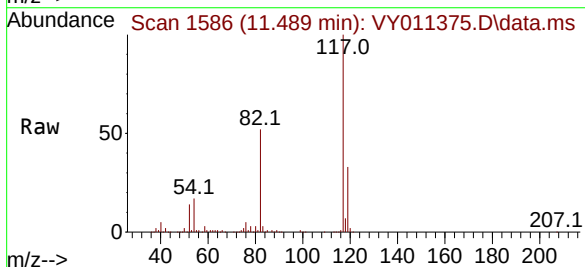

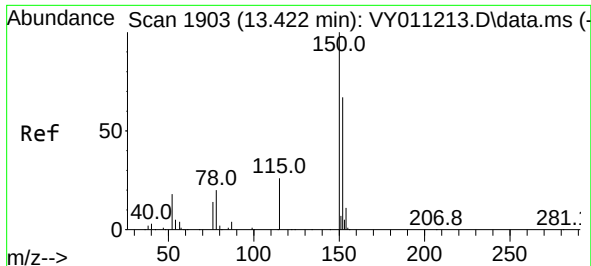

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY011375.D


Acq: 08 Nov 2022 20:13

Instrument :

MSVOA_Y

ClientSampleId :

250FERRYBLVD-TFS-06RE

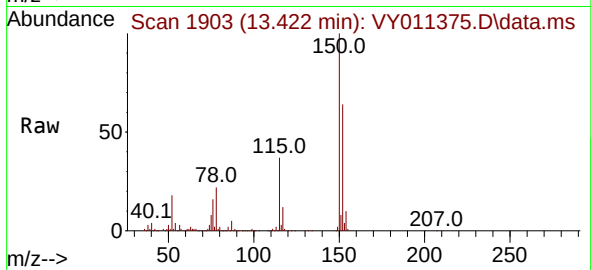

Tgt Ion:152 Resp: 108260

Ion Ratio Lower Upper

152 100

115 57.1 28.2 84.7

150 156.1 0.0 347.6

