
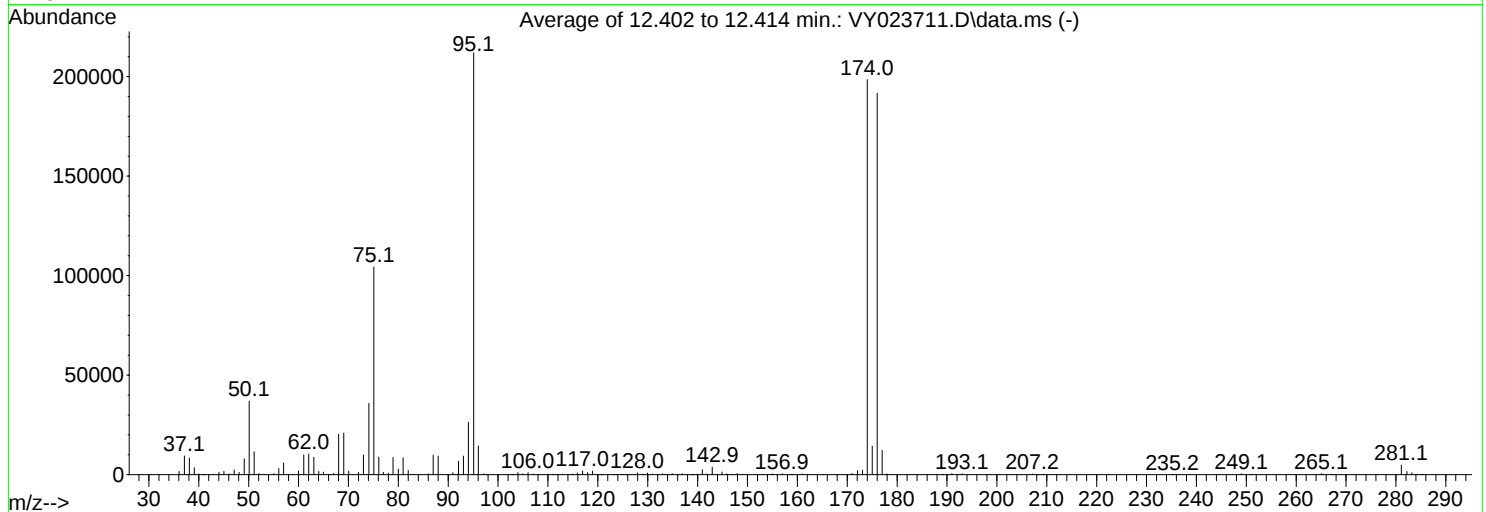


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111025\
Data File : VY023711.D
Acq On : 10 Nov 2025 08:08
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Title : SW846 8260
Last Update : Wed Oct 08 05:12:50 2025

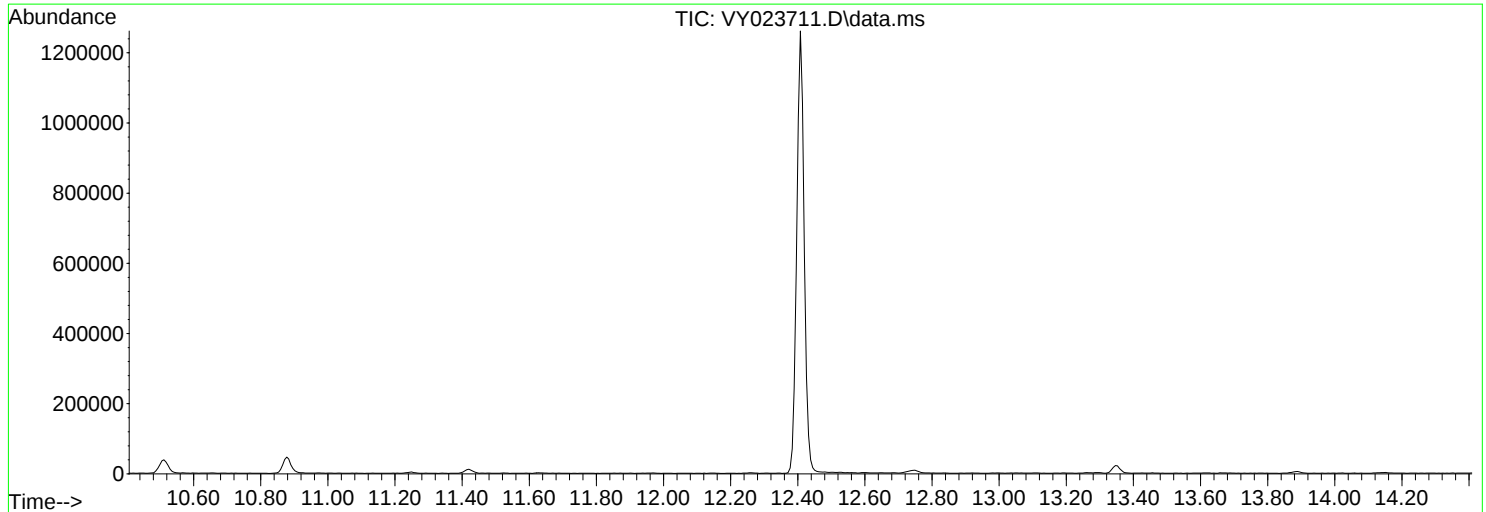

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	36909	PASS
75	95	30	60	49.3	104405	PASS
95	95	100	100	100.0	211947	PASS
96	95	5	9	6.8	14382	PASS
173	174	0.00	2	1.1	2257	PASS
174	95	50	100	93.7	198528	PASS
175	174	5	9	7.2	14283	PASS
176	174	95	101	96.6	191680	PASS
177	176	5	9	6.4	12194	PASS