

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111125\
 Data File : VY023730.D
 Acq On : 11 Nov 2025 11:03
 Operator : SY/MD
 Sample : VY1111SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1111SBL01

Quant Time: Nov 12 03:32:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 08 05:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.713	168	807177	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.622	114	1372130	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	1134523	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	441999	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.067	65	373536	55.341	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.680%
35) Dibromofluoromethane	7.640	113	430836	51.101	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.200%
50) Toluene-d8	10.109	98	1525090	48.573	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.140%
62) 4-Bromofluorobenzene	12.408	95	434745	41.939	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY111125\
Data File : VY023730.D
Acq On : 11 Nov 2025 11:03
Operator : SY/MD
Sample : VY1111SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1111SBL01

Quant Time: Nov 12 03:32:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y100725S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 08 05:12:50 2025
Response via : Initial Calibration




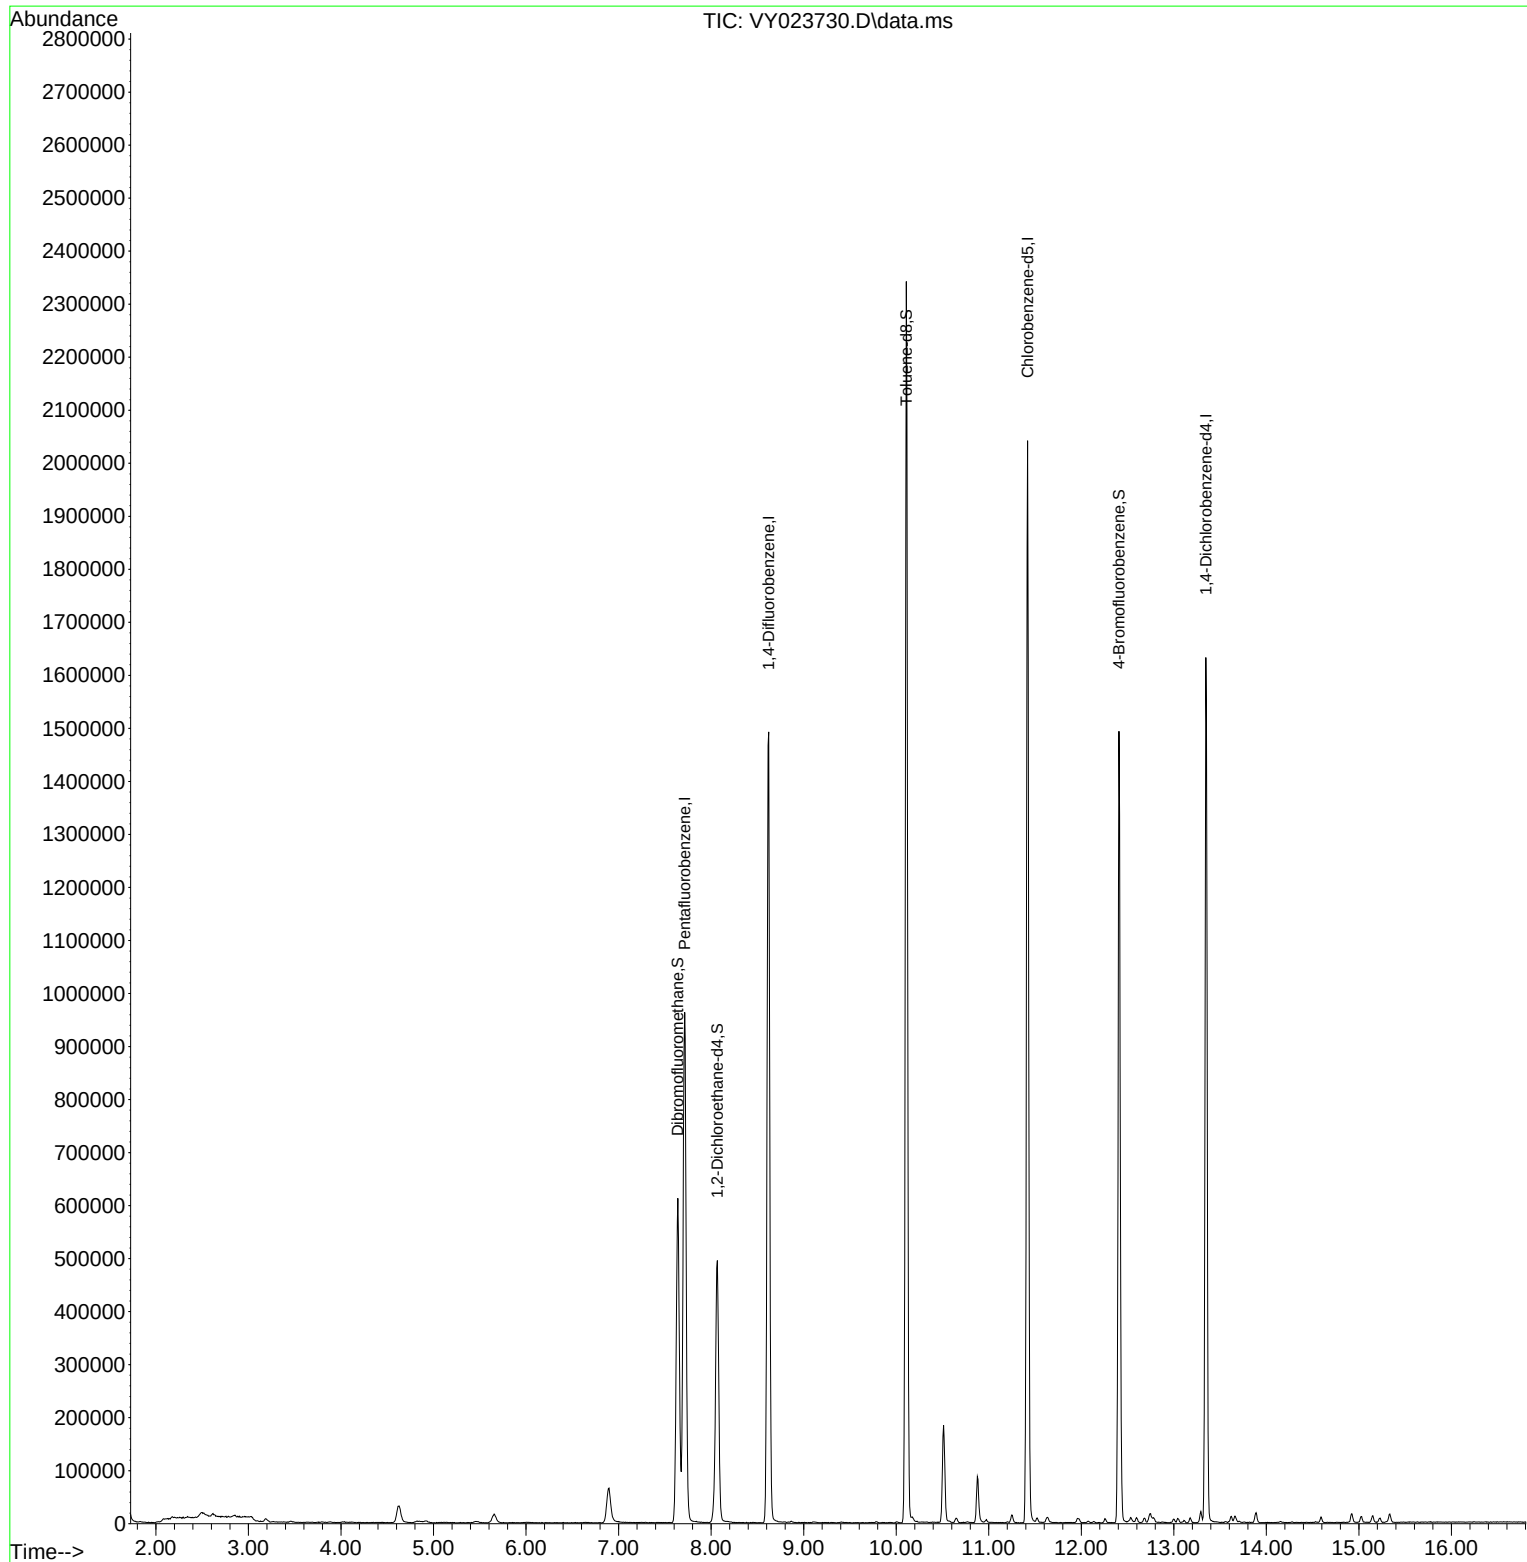


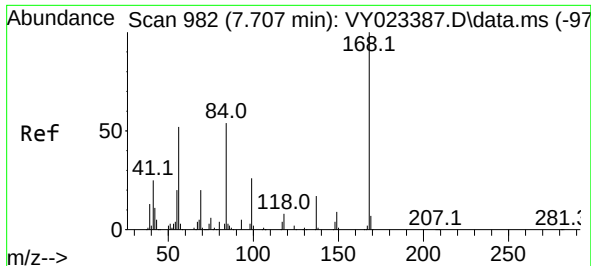

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.713 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03




Instrument :
MSVOA_Y
ClientSampleId :
VY1111SBL01


Tgt Ion:168 Resp: 807177
Ion Ratio Lower Upper
168 100
99 49.6 39.7 59.5

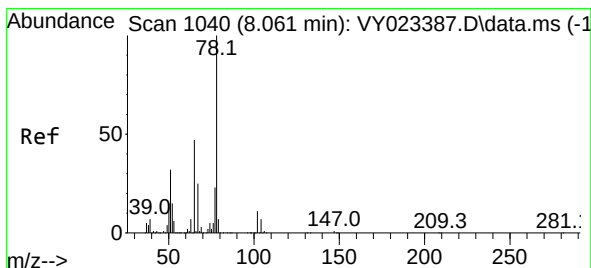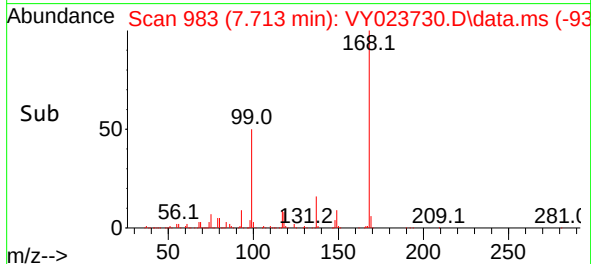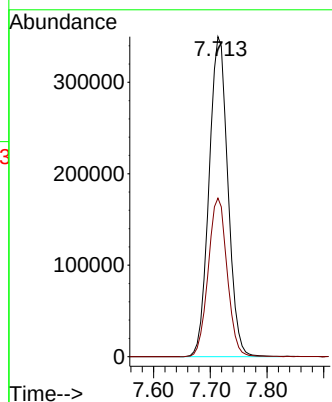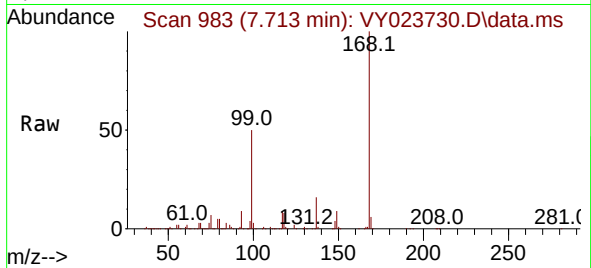

#33
1,2-Dichloroethane-d4
Concen: 55.341 ug/l
RT: 8.067 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03

Tgt Ion: 65 Resp: 373536
Ion Ratio Lower Upper
65 100
67 53.5 0.0 105.8


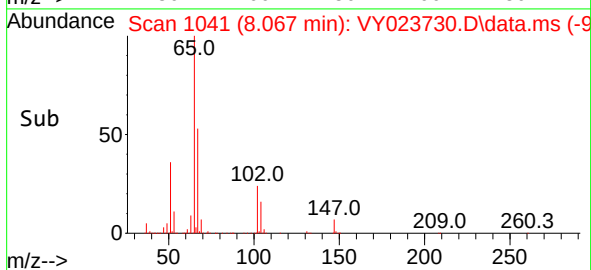
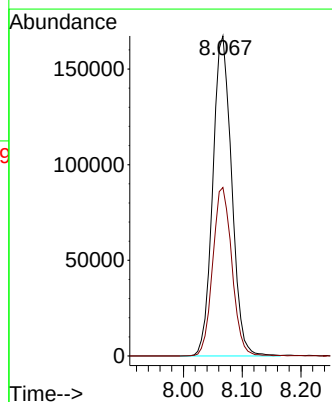
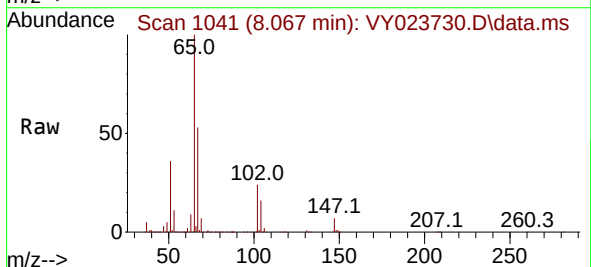


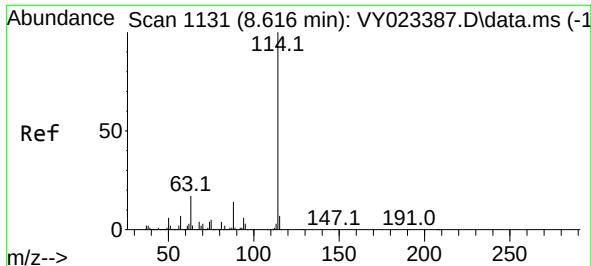

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.622 min Scan# 1132
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03




Instrument :
MSVOA_Y
ClientSampleId :
VY1111SBL01


Tgt Ion:114 Resp: 1372130
Ion Ratio Lower Upper
114 100
63 17.2 0.0 34.2
88 14.3 0.0 28.4

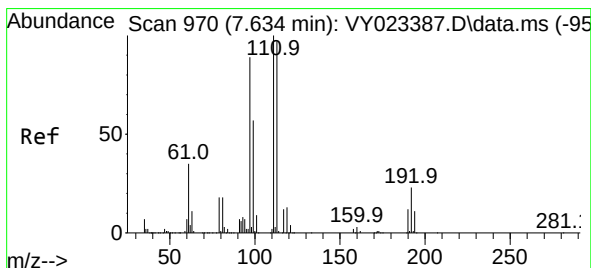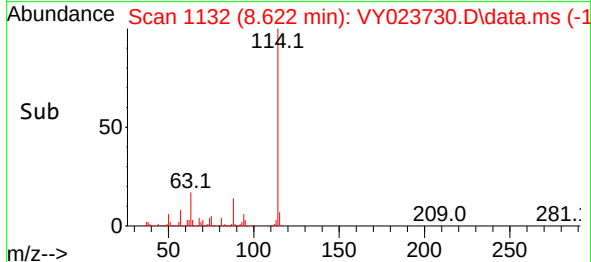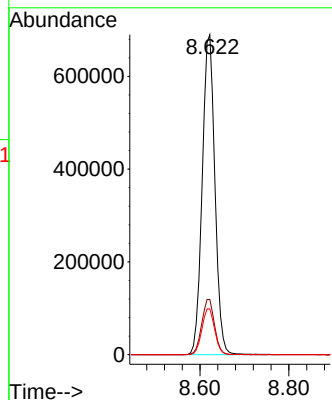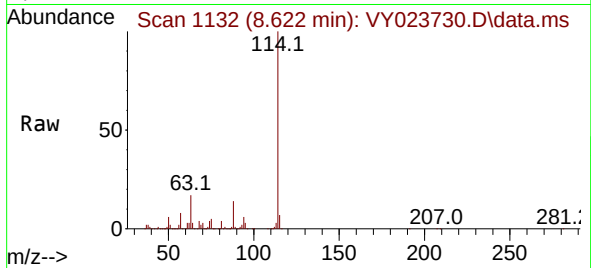

#35
Dibromofluoromethane
Concen: 51.101 ug/l
RT: 7.640 min Scan# 971
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03

Tgt Ion:113 Resp: 430836
Ion Ratio Lower Upper
113 100
111 102.1 81.8 122.6
192 21.8 18.0 27.0


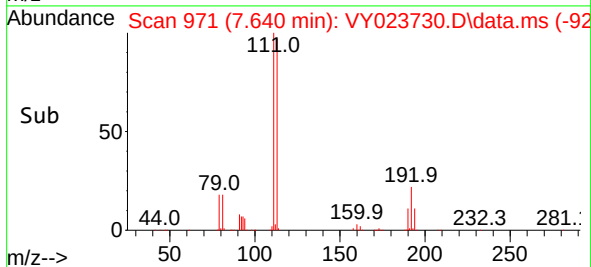
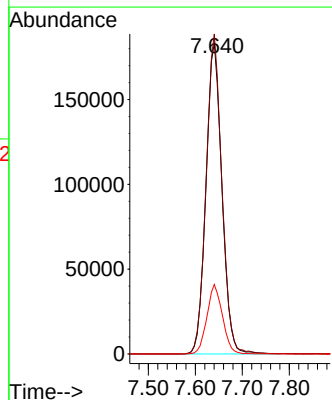
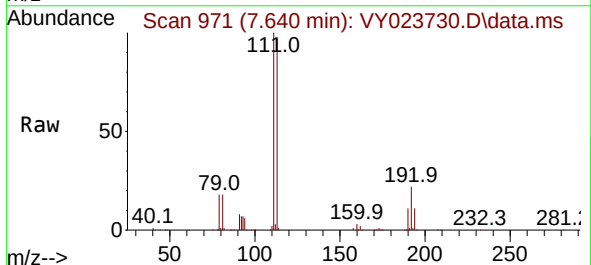


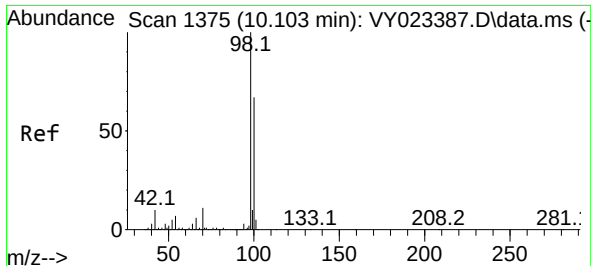

#50
Toluene-d8
Concen: 48.573 ug/l
RT: 10.109 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03




Instrument :
MSVOA_Y
ClientSampleId :
VY1111SBL01


Tgt Ion: 98 Resp: 1525090
Ion Ratio Lower Upper
98 100
100 65.3 53.0 79.4

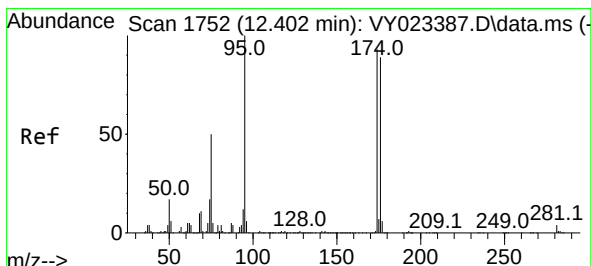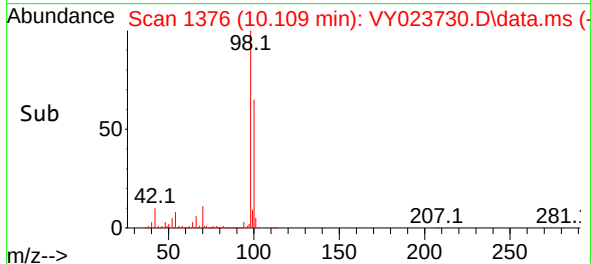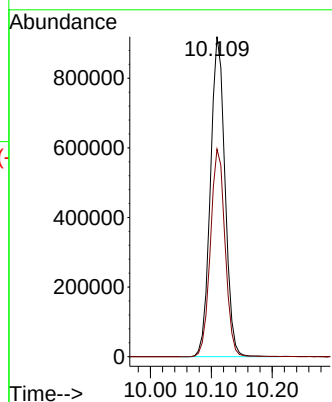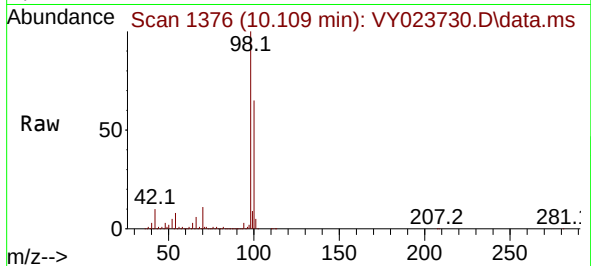

#62
4-Bromofluorobenzene
Concen: 41.939 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03

Tgt Ion: 95 Resp: 434745
Ion Ratio Lower Upper
95 100
174 93.7 0.0 192.8
176 90.5 0.0 187.6


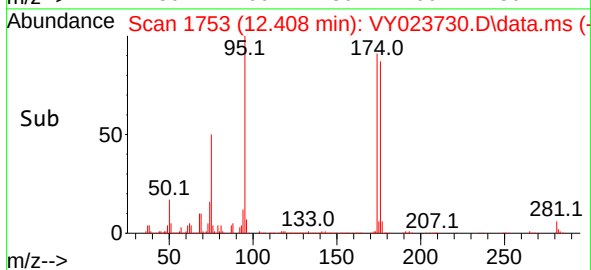
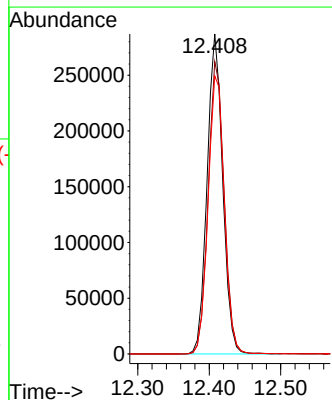
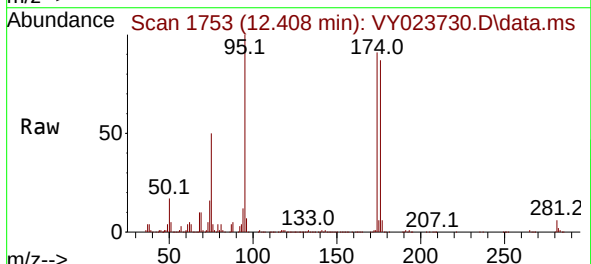


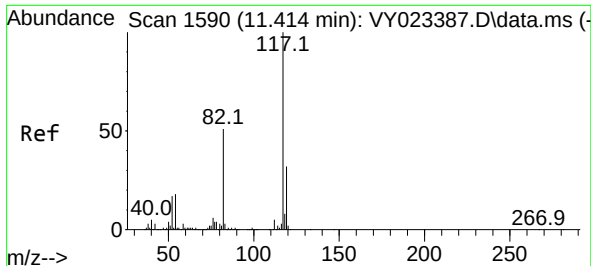

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.420 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03

Instrument :
MSVOA_Y
ClientSampleId :
VY1111SBL01

Tgt Ion:117 Resp: 1134523
Ion Ratio Lower Upper
117 100
82 50.9 41.0 61.4
119 32.2 25.6 38.4

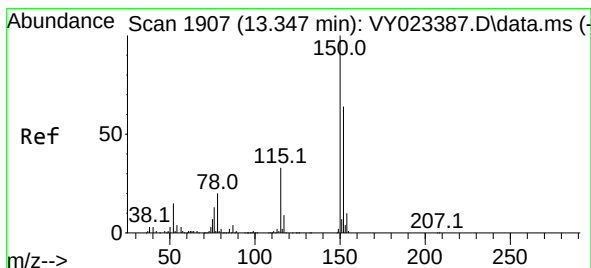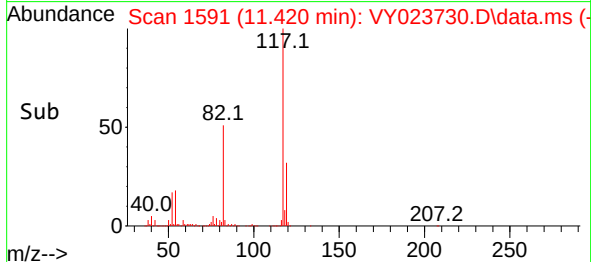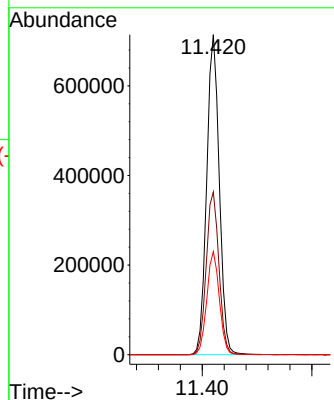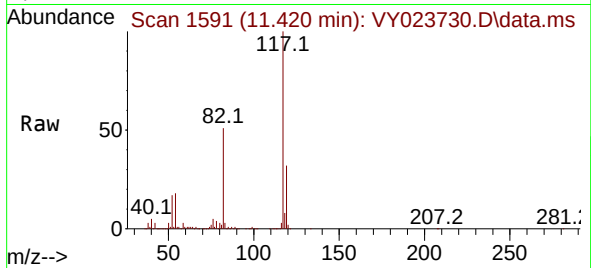

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.347 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY023730.D
Acq: 11 Nov 2025 11:03

Tgt Ion:152 Resp: 441999
Ion Ratio Lower Upper
152 100
115 55.5 27.1 81.2
150 156.3 0.0 347.4

