

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112024\
 Data File : VY020357.D
 Acq On : 20 Nov 2024 14:17
 Operator : SY/MD
 Sample : P4916-11
 Misc : 4.21g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-3-VOC

Quant Time: Nov 21 00:47:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 20 04:38:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	153605	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.616	114	298657	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	281091	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.347	152	110395	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	98639	55.894	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.780%
35) Dibromofluoromethane	7.634	113	94704	49.452	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.900%
50) Toluene-d8	10.103	98	366156	48.537	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	97.080%
62) 4-Bromofluorobenzene	12.402	95	126187	52.033	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	104.060%


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112024\
Data File : VY020357.D
Acq On : 20 Nov 2024 14:17
Operator : SY/MD
Sample : P4916-11
Misc : 4.21g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-3-VOC


Quant Time: Nov 21 00:47:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 20 04:38:24 2024
Response via : Initial Calibration

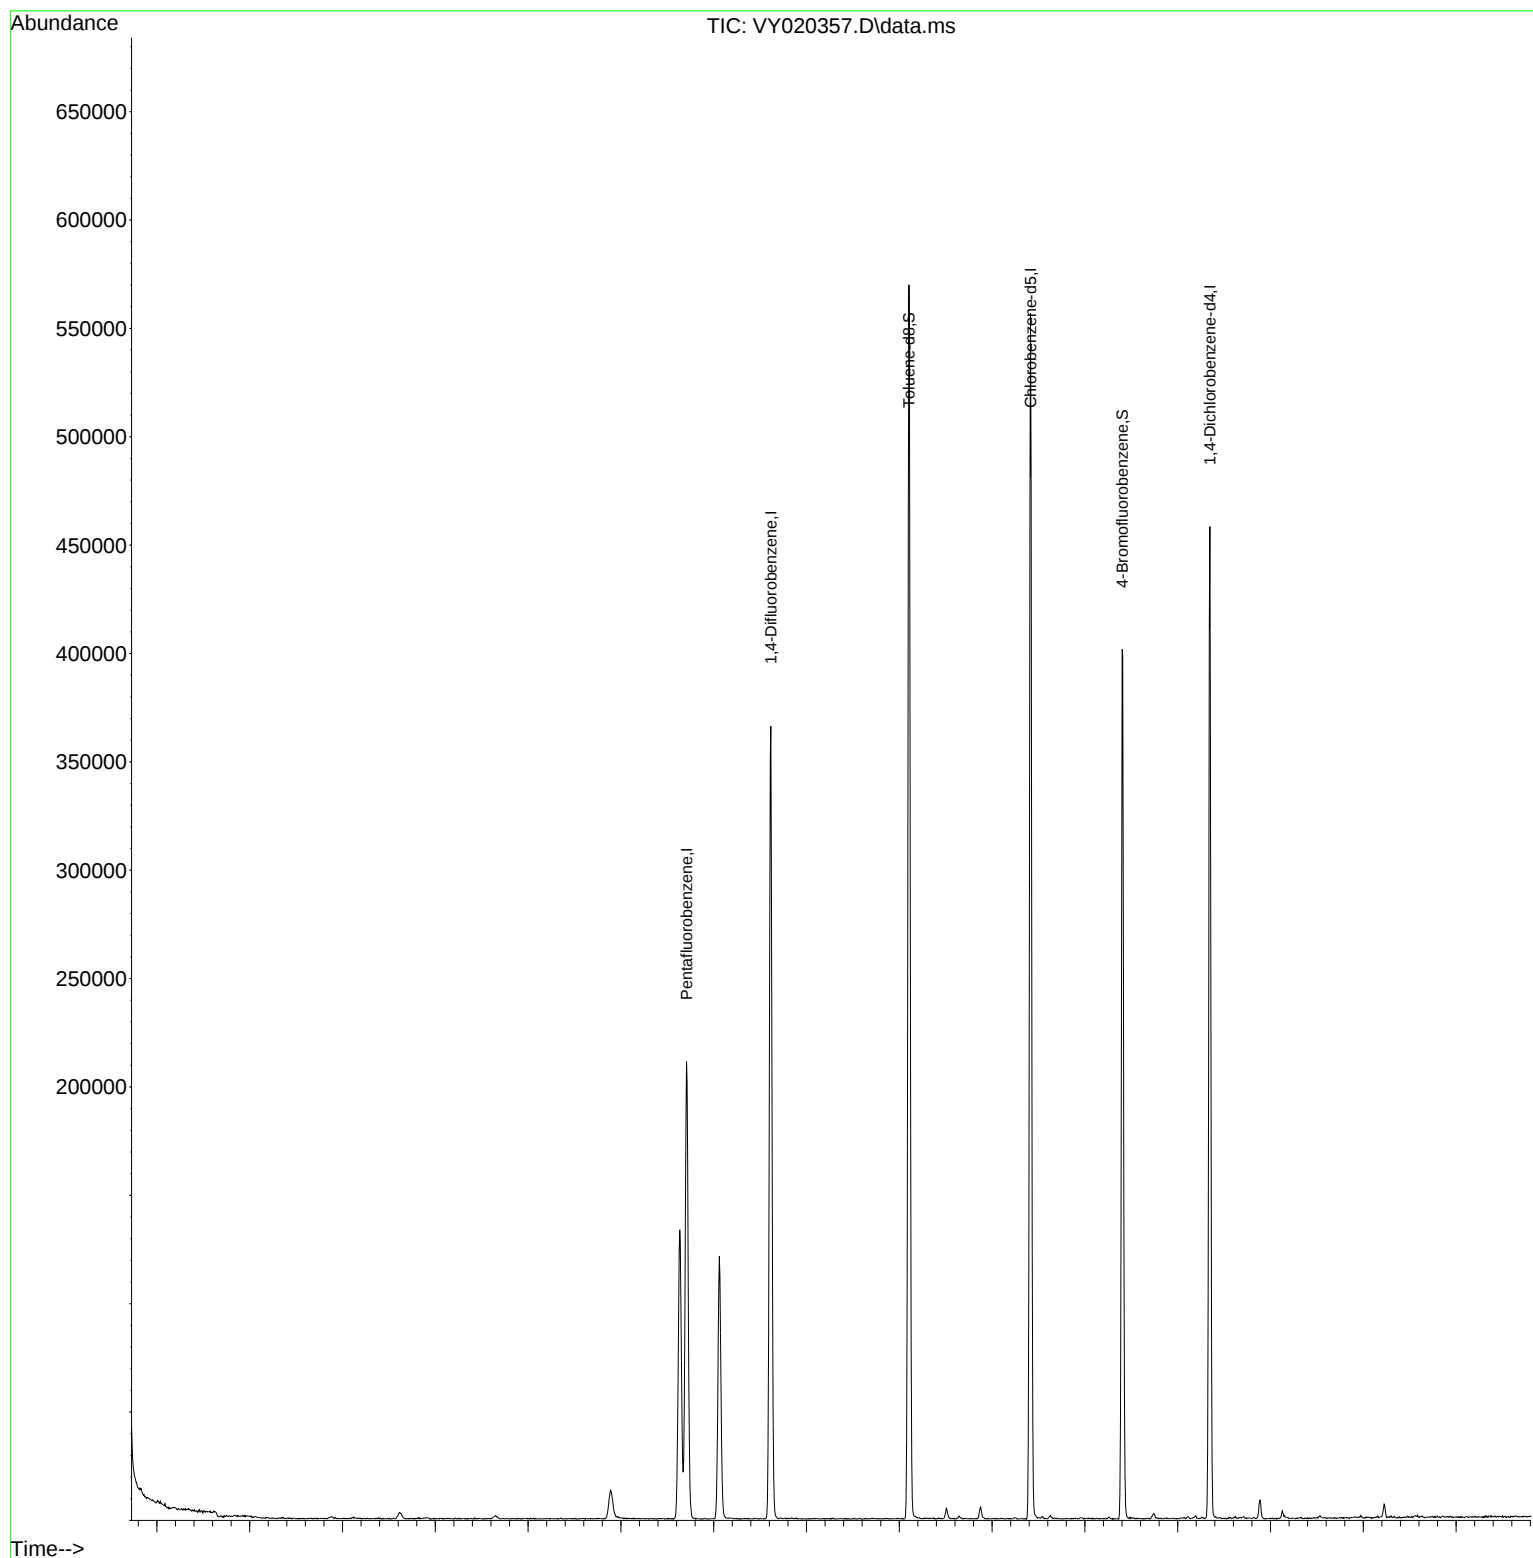



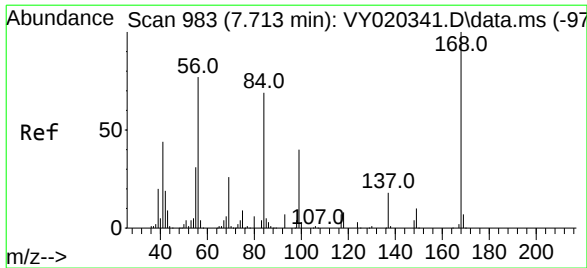


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 983
Delta R.T. -0.006 min
Lab File: VY020357.D
Acq: 20 Nov 2024 14:17

Instrument :
MSVOA_Y
ClientSampleId :
TP-3-VOC



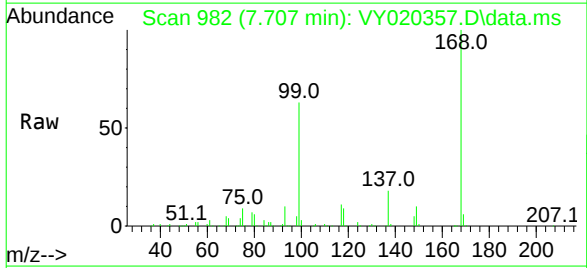



Tgt Ion:168 Resp: 153605
Ion Ratio Lower Upper
168 100
99 63.0 46.6 69.8

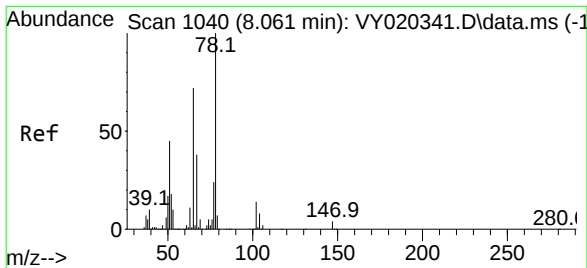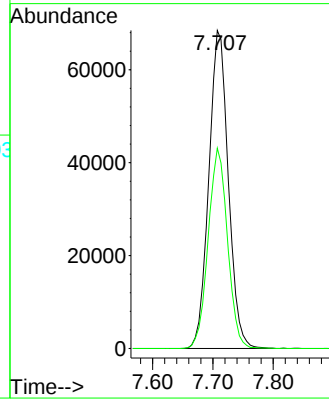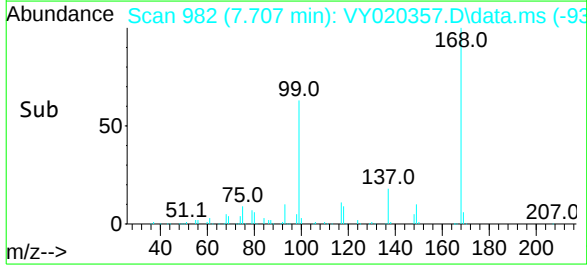

#33
1,2-Dichloroethane-d4
Concen: 55.894 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VY020357.D
Acq: 20 Nov 2024 14:17

Tgt Ion: 65 Resp: 98639
Ion Ratio Lower Upper
65 100
67 51.2 0.0 105.8


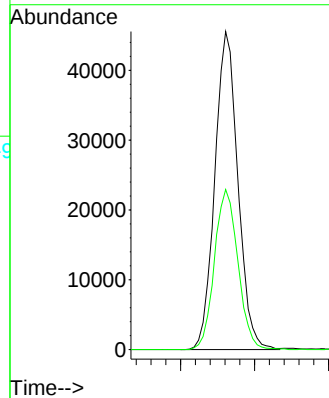
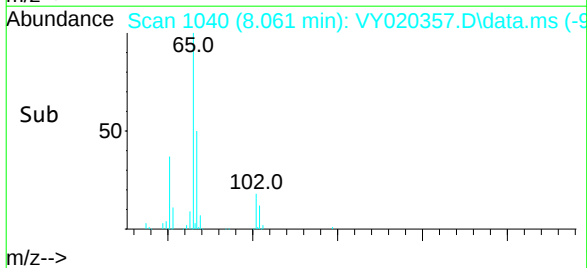
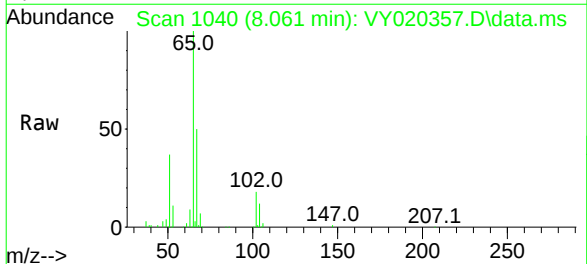


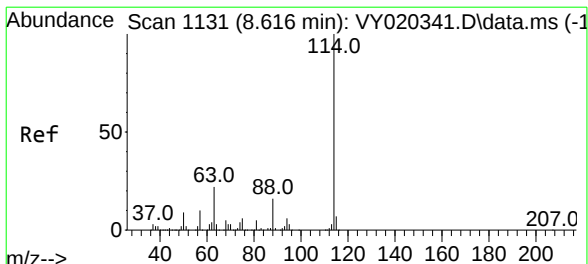

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.616 min Scan# 111
 Delta R.T. -0.000 min
 Lab File: VY020357.D
 Acq: 20 Nov 2024 14:17




Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-3-VOC


Tgt Ion:	114	Resp:	298657
Ion	Ratio	Lower	Upper
114	100		
63	21.4	0.0	44.8
88	16.8	0.0	32.0

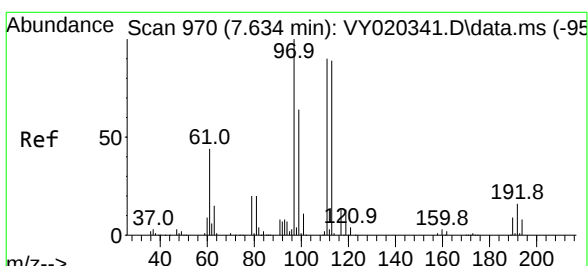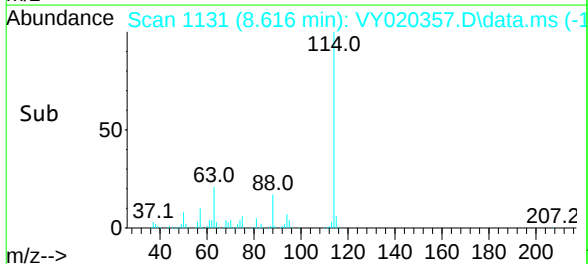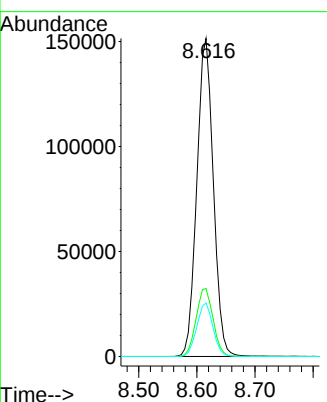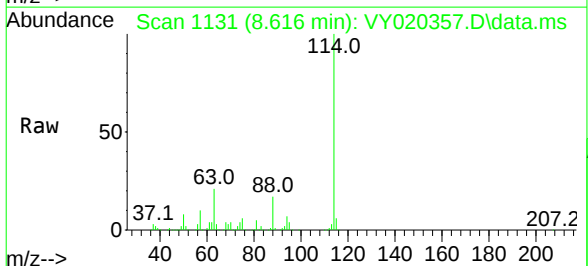

#35
 Dibromofluoromethane
 Concen: 49.452 ug/l
 RT: 7.634 min Scan# 970
 Delta R.T. -0.000 min
 Lab File: VY020357.D
 Acq: 20 Nov 2024 14:17

Tgt Ion:	113	Resp:	94704
Ion	Ratio	Lower	Upper
113	100		
111	103.4	81.4	122.0
192	18.9	15.1	22.7

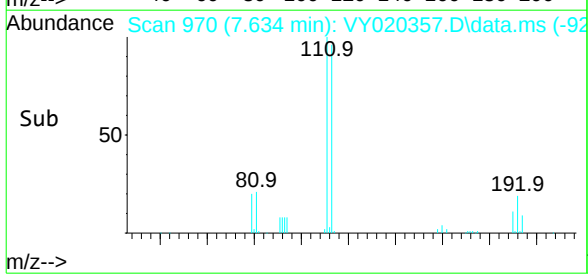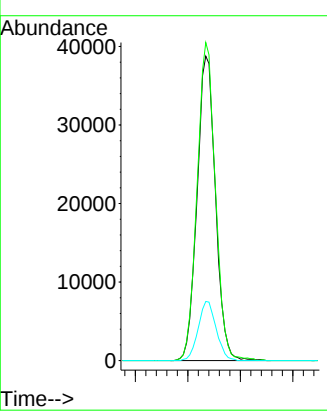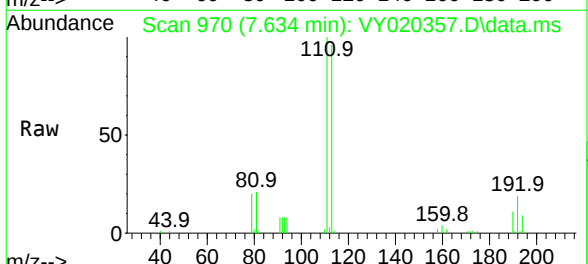

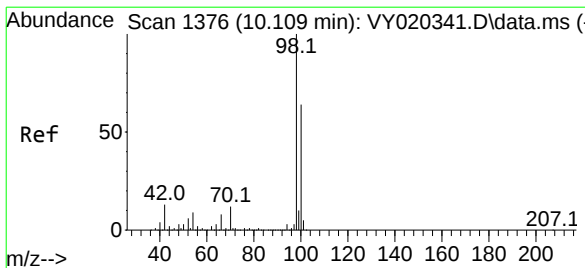

#50

Toluene-d8

Concen: 48.537 ug/l

RT: 10.103 min Scan# 1376

Delta R.T. -0.006 min

Lab File: VY020357.D

Acq: 20 Nov 2024 14:17

Instrument :

MSVOA_Y

ClientSampleId :





TP-3-VOC

Tgt Ion: 98 Resp: 366156

Ion Ratio Lower Upper

98 100

100 64.6 51.3 76.9

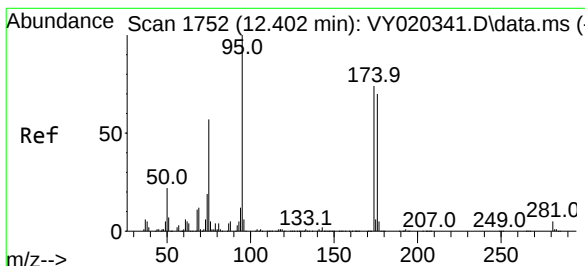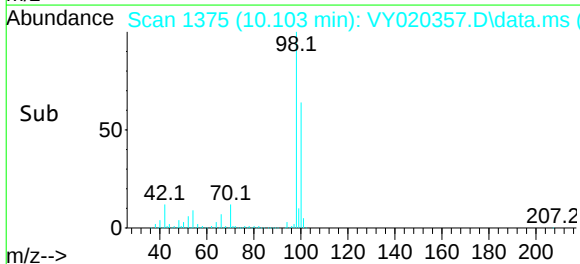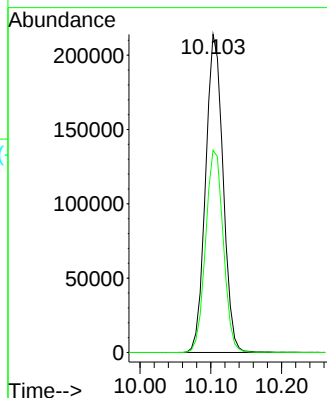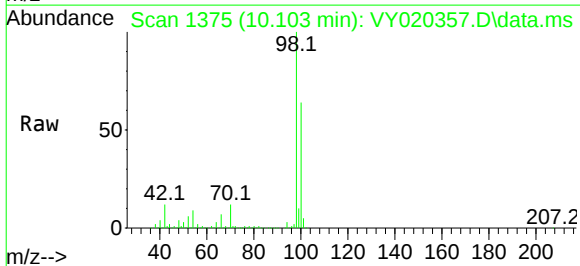

#62

4-Bromofluorobenzene

Concen: 52.033 ug/l

RT: 12.402 min Scan# 1752

Delta R.T. -0.000 min

Lab File: VY020357.D

Acq: 20 Nov 2024 14:17




Tgt Ion: 95 Resp: 126187


Ion Ratio Lower Upper

95 100

174 76.7 0.0 156.8

176 73.7 0.0 152.0

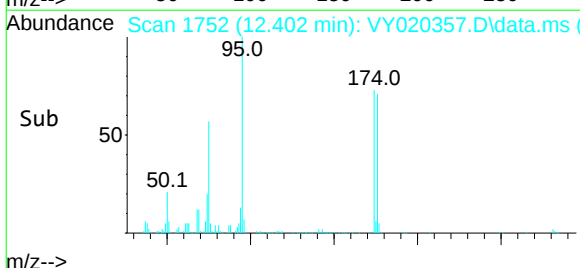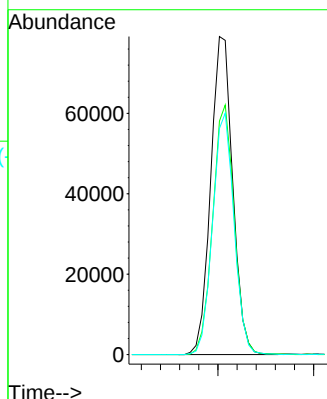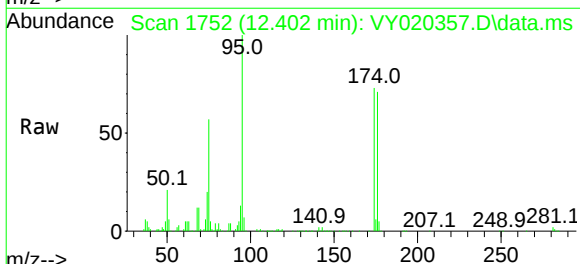

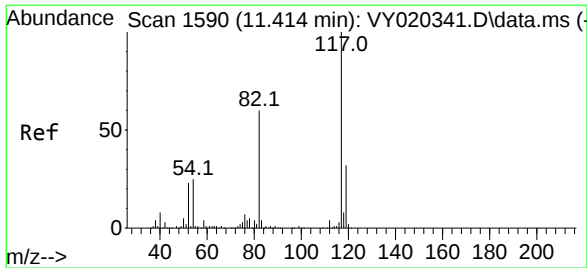

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.414 min Scan# 1590

Delta R.T. -0.000 min

Lab File: VY020357.D

Acq: 20 Nov 2024 14:17

Instrument :

MSVOA_Y

ClientSampleId :

TP-3-VOC





Tgt Ion:117 Resp: 281091

Ion Ratio Lower Upper

117 100

82 59.9 48.2 72.4

119 32.8 25.8 38.8

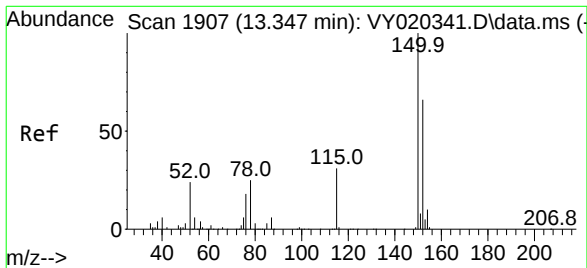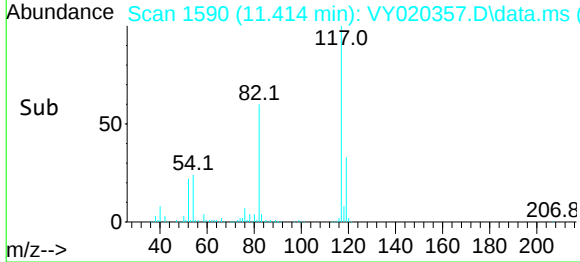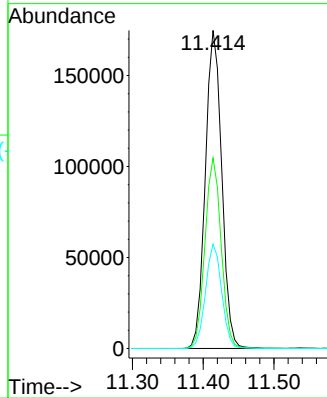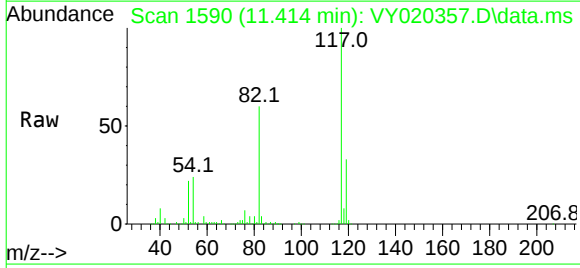

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.347 min Scan# 1907

Delta R.T. -0.000 min

Lab File: VY020357.D

Acq: 20 Nov 2024 14:17

Tgt Ion:152 Resp: 110395

Ion Ratio Lower Upper

152 100

115 60.6 30.0 90.0

150 158.5 0.0 348.2

