

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112224\
 Data File : VY020418.D
 Acq On : 22 Nov 2024 17:10
 Operator : SY/MD
 Sample : P4960-05
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SW3

Quant Time: Nov 23 00:03:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 20 04:38:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.71
34) 1,4-Difluorobenzene	8.622	114	204	50.000	ug/l	0.00
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.41
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.35

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.079	65	51	0.000	ug/l	0.02
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	7.628	113	21	16.054	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	32.100%#
50) Toluene-d8	10.109	98	79	15.331	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	30.660%#
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	29 - 146	Recovery	=	0.000%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112224\
Data File : VY020418.D
Acq On : 22 Nov 2024 17:10
Operator : SY/MD
Sample : P4960-05
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SW3

Quant Time: Nov 23 00:03:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Quant Title : SW846 8260
QLast Update : Wed Nov 20 04:38:24 2024
Response via : Initial Calibration


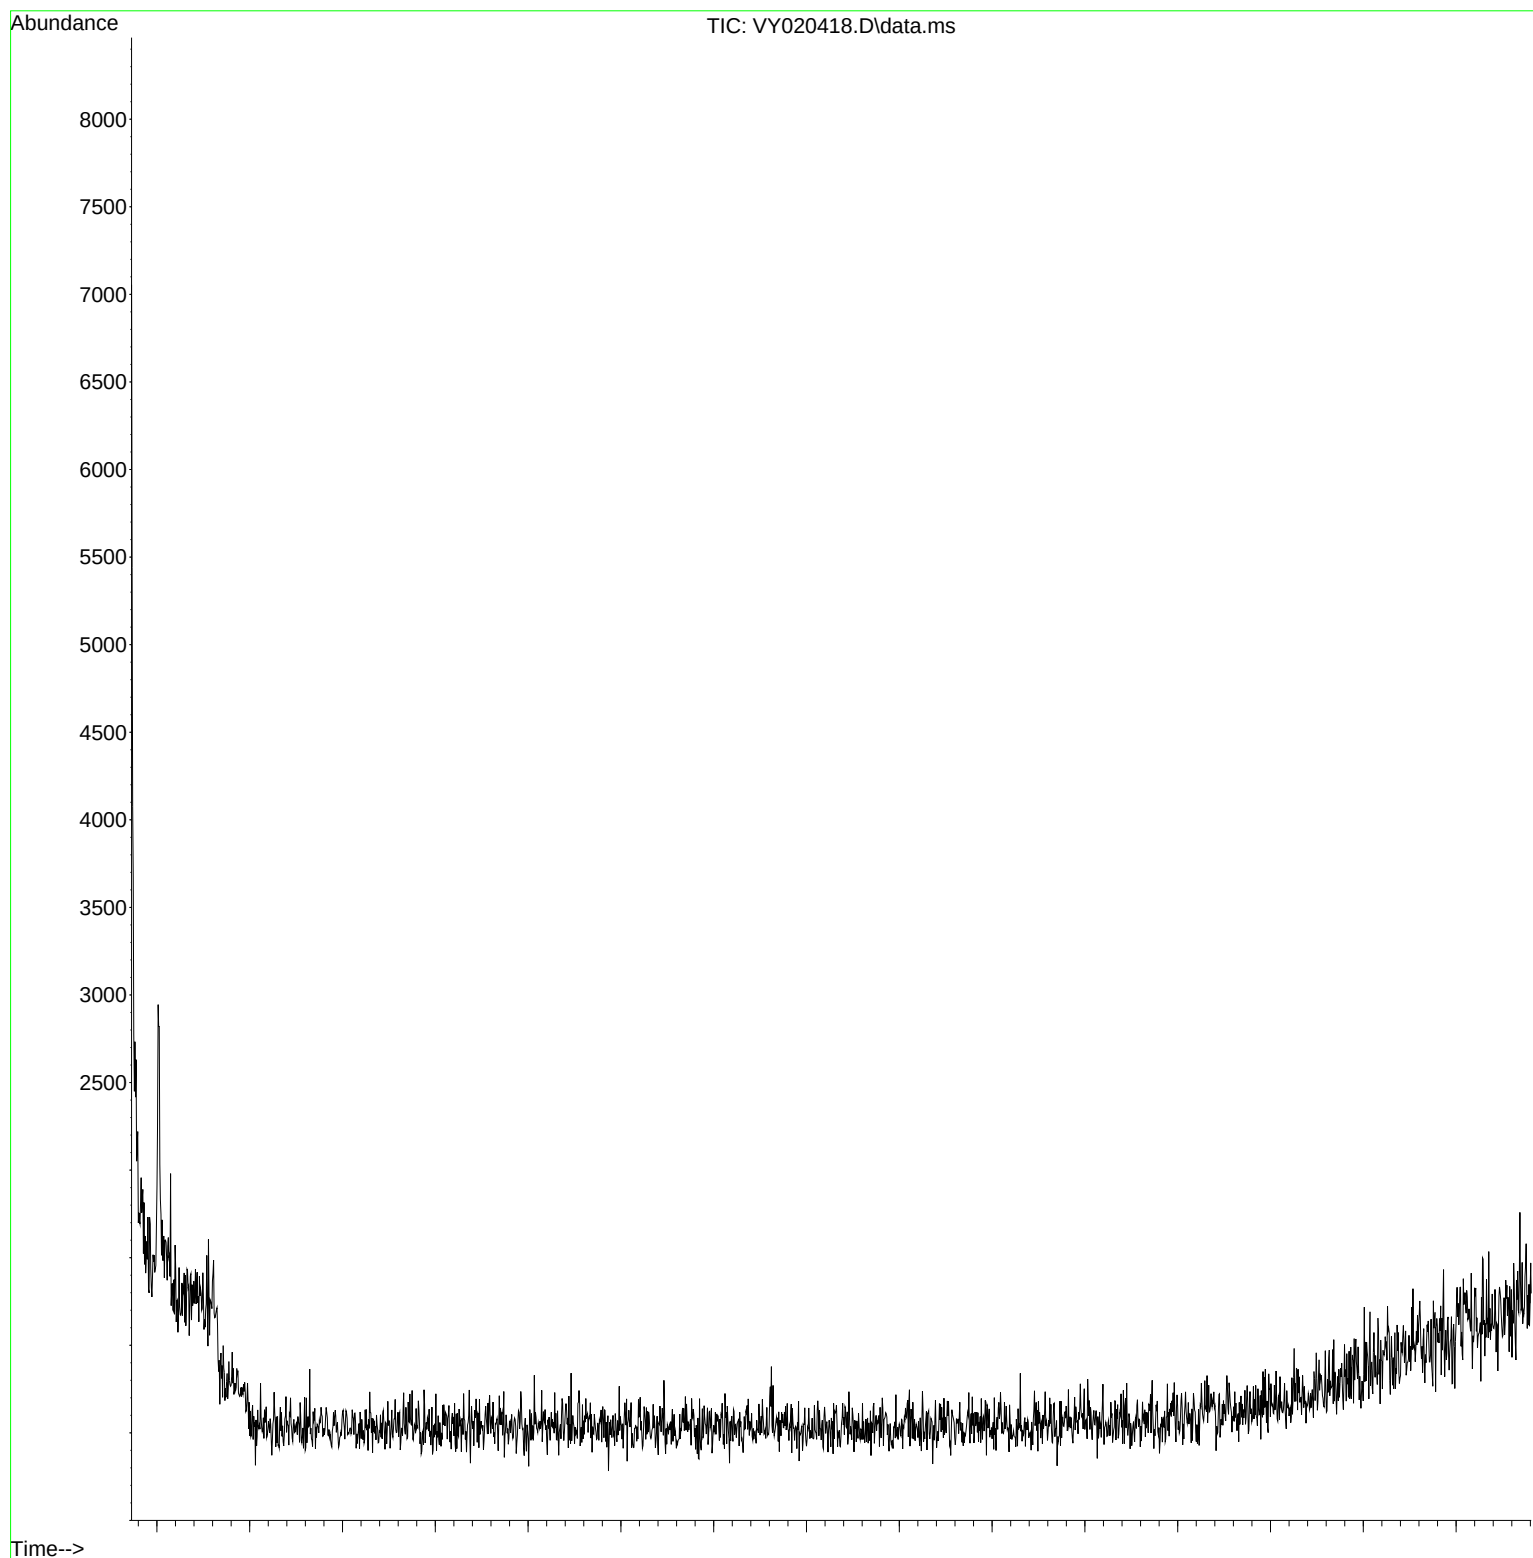


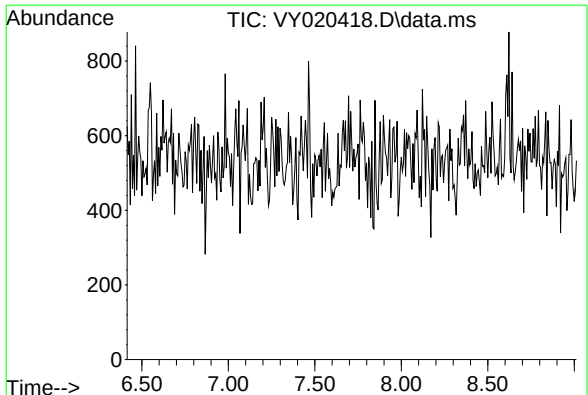

#1
 Pentafluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 7.71 min
 Lab File: VY020418.D
 Acq: 22 Nov 2024 17:10




Instrument :
 MSVOA_Y
 ClientSampleId :
 SW3


Tgt Ion: 168
 Sig Exp Ratio
 168 100
 99 58.2

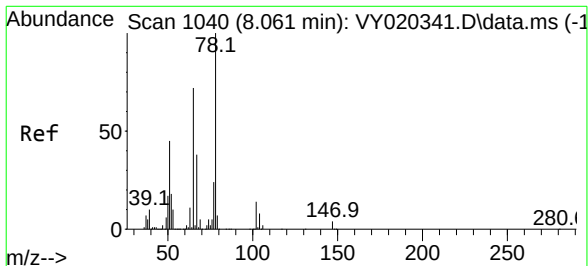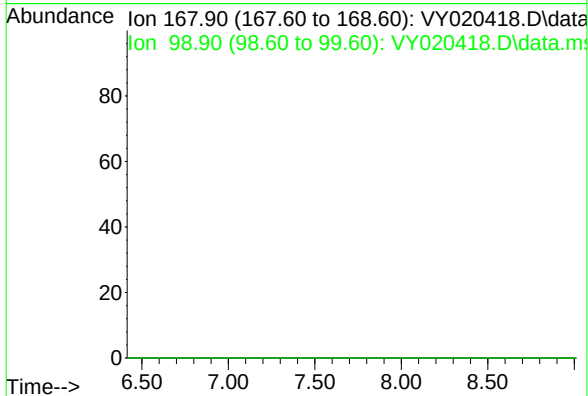

#33
 1,2-Dichloroethane-d4
 Concen: 0.000 ug/l
 RT: 8.079 min Scan# 1043
 Delta R.T. 0.018 min
 Lab File: VY020418.D
 Acq: 22 Nov 2024 17:10


Tgt Ion: 65 Resp: 51
 Ion Ratio Lower Upper
 65 100
 67 0.0 0.0 105.8

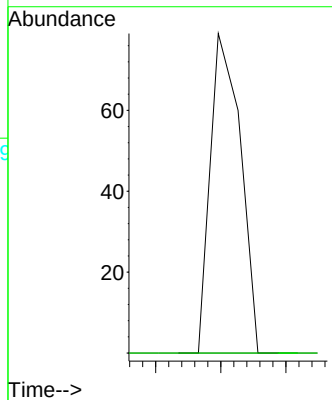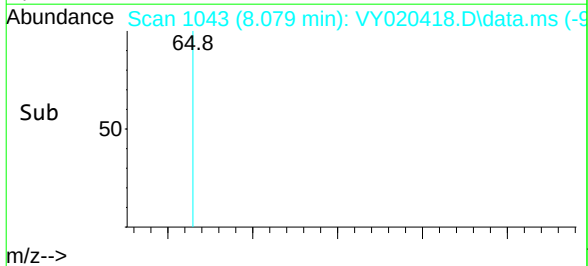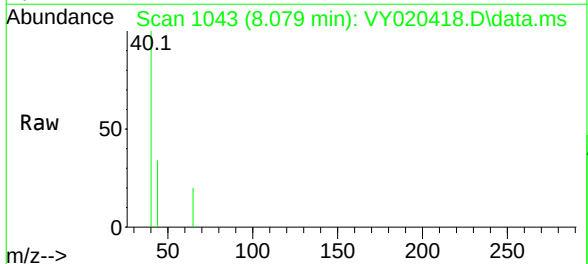



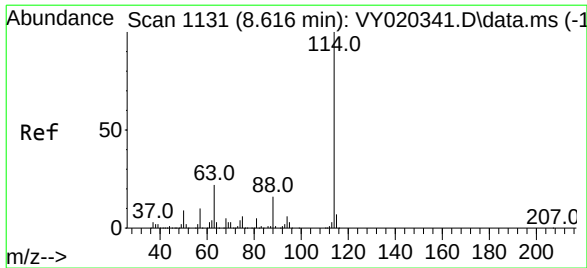


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.622 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY020418.D
Acq: 22 Nov 2024 17:10

Instrument :
MSVOA_Y
ClientSampleId :
SW3



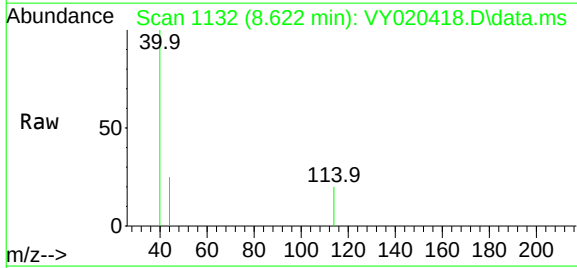



Tgt Ion:114 Resp: 204
Ion Ratio Lower Upper
114 100
63 0.0 0.0 44.8
88 0.0 0.0 32.0

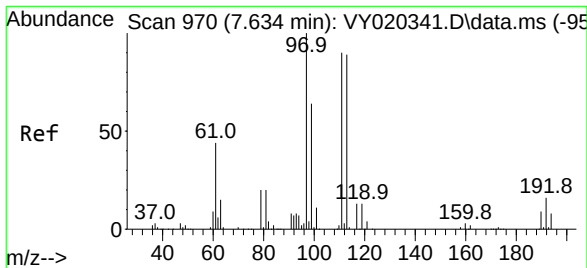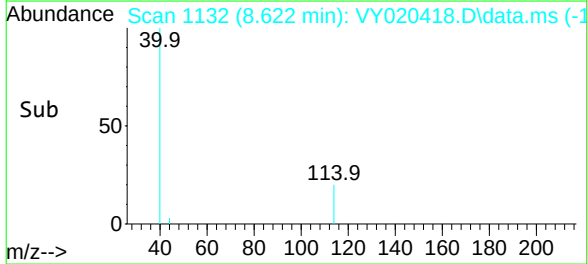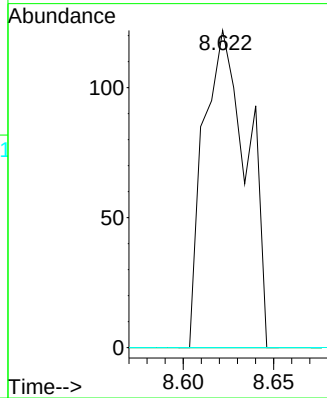

#35
Dibromofluoromethane
Concen: 16.054 ug/l
RT: 7.628 min Scan# 969
Delta R.T. -0.006 min
Lab File: VY020418.D
Acq: 22 Nov 2024 17:10

Tgt Ion:113 Resp: 21
Ion Ratio Lower Upper
113 100
111 209.5 81.4 122.0#
192 0.0 15.1 22.7#

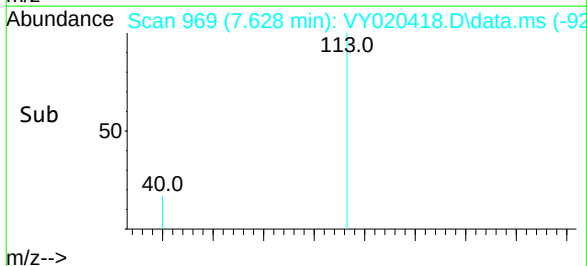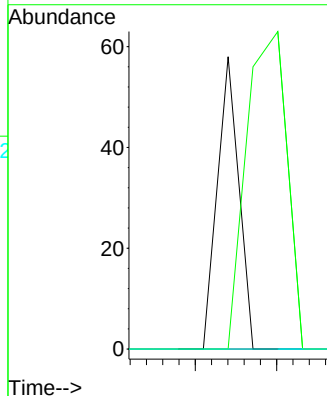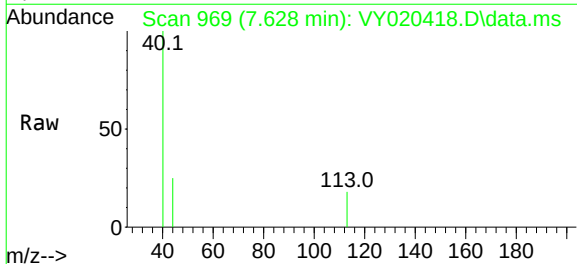

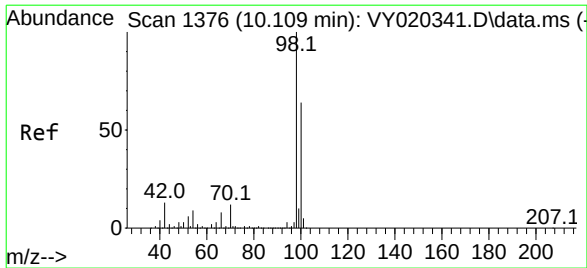

#50

Toluene-d8

Concen: 15.331 ug/l

RT: 10.109 min Scan# 13

Delta R.T. 0.000 min

Lab File: VY020418.D

Acq: 22 Nov 2024 17:10

Instrument :

MSVOA_Y

ClientSampleId :





SW3

Tgt Ion: 98 Resp: 79

Ion Ratio Lower Upper

98 100

100 0.0 51.3 76.9#

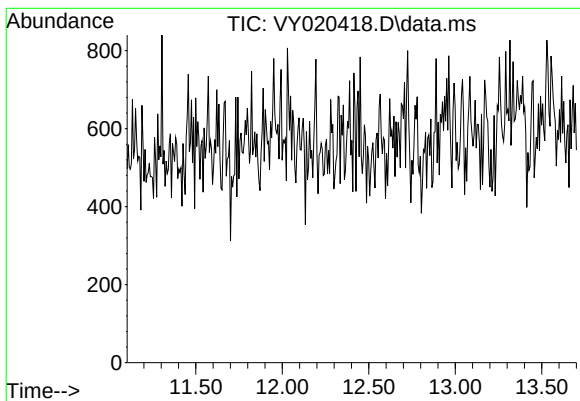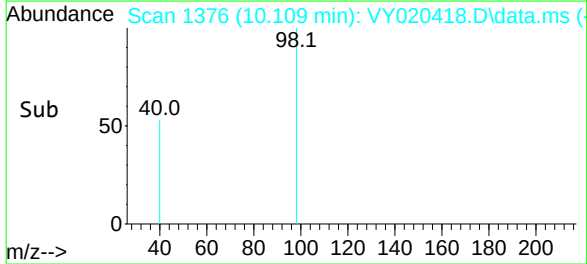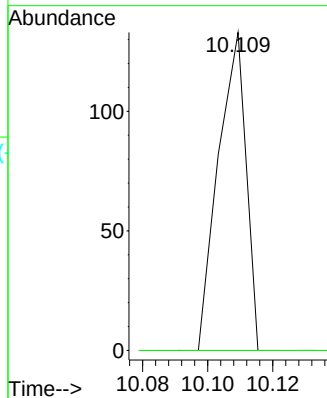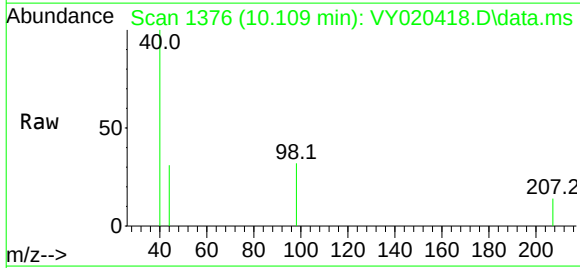

#62

4-Bromofluorobenzene

Concen: 0.000 ug/l

Expected RT: 12.40 min

Lab File: VY020418.D

Acq: 22 Nov 2024 17:10


Tgt Ion: 95


Sig Exp Ratio

95 100

174 78.4

176 76.0

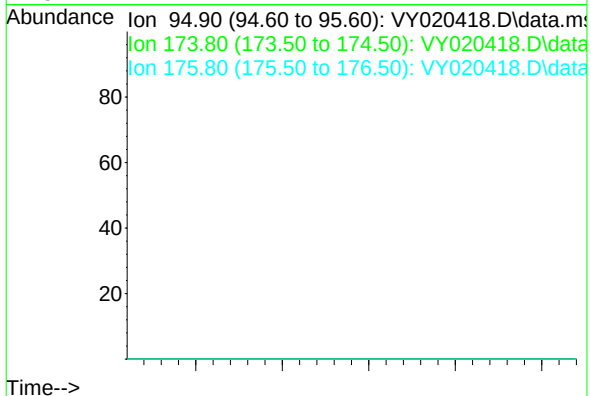


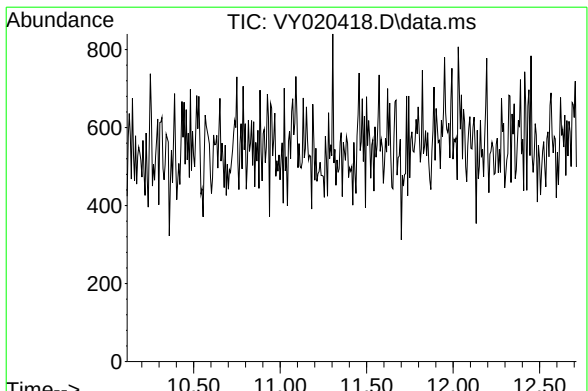


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.41 min

Lab File: VY020418.D
Acq: 22 Nov 2024 17:10

Instrument :
MSVOA_Y
ClientSampleId :
SW3

Tgt Ion: 117	
Sig	Exp Ratio
117	100
82	60.3
119	32.3

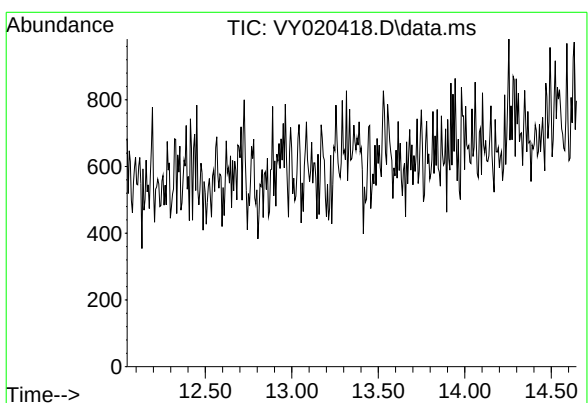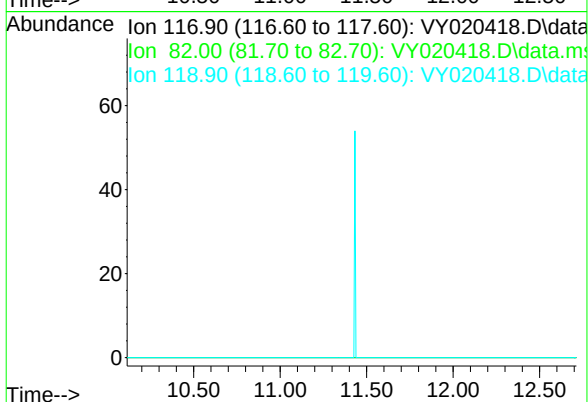

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.35 min

Lab File: VY020418.D
Acq: 22 Nov 2024 17:10

Tgt Ion: 152	
Sig	Exp Ratio
152	100
115	60.0
150	174.1

