
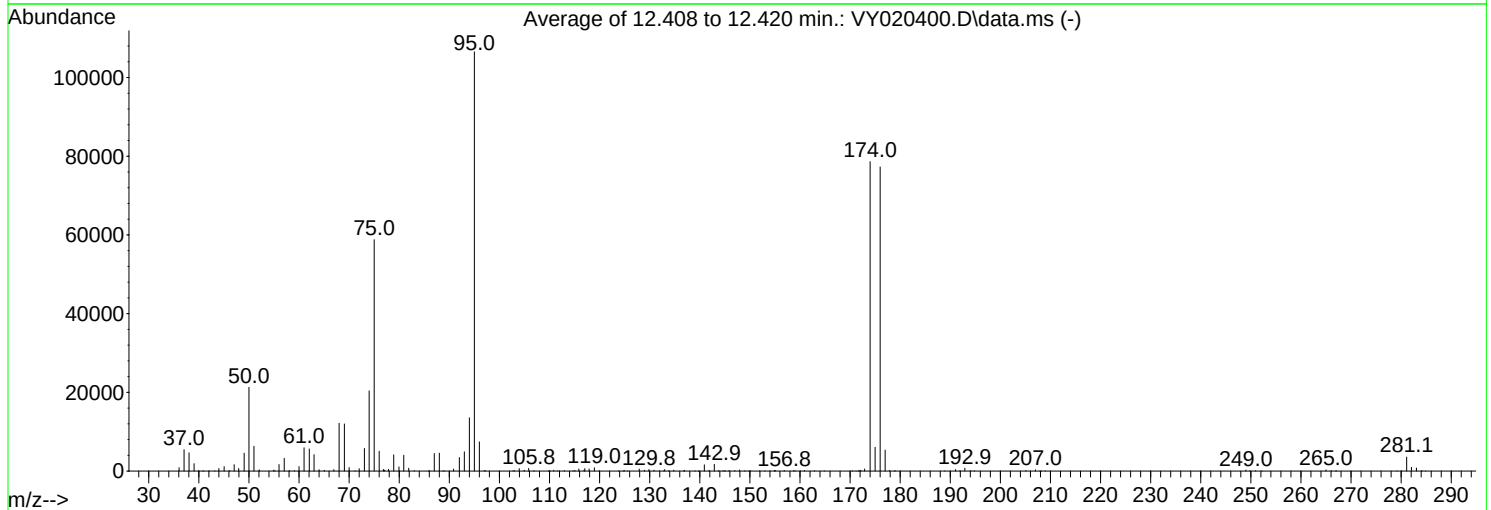


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112224\
Data File : VY020400.D
Acq On : 22 Nov 2024 08:56
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Title : SW846 8260
Last Update : Wed Nov 20 04:38:24 2024

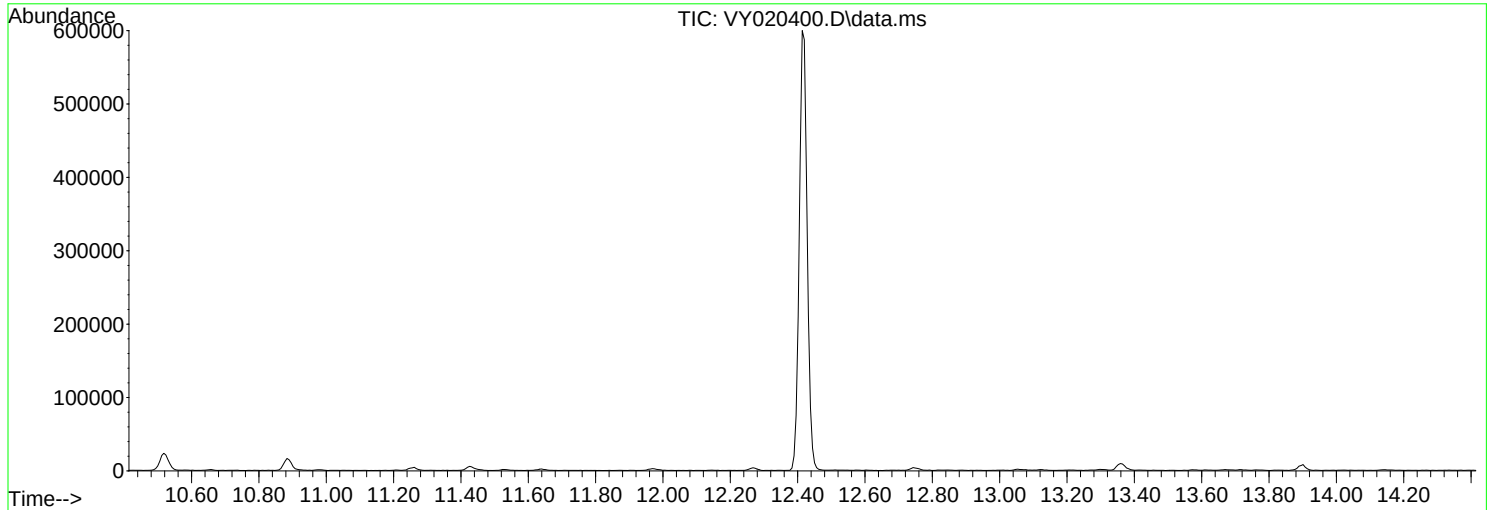

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1746

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	21291	PASS
75	95	30	60	55.2	58803	PASS
95	95	100	100	100.0	106549	PASS
96	95	5	9	7.0	7433	PASS
173	174	0.00	2	0.7	521	PASS
174	95	50	100	73.8	78624	PASS
175	174	5	9	7.7	6067	PASS
176	174	95	101	98.3	77283	PASS
177	176	5	9	6.9	5341	PASS