
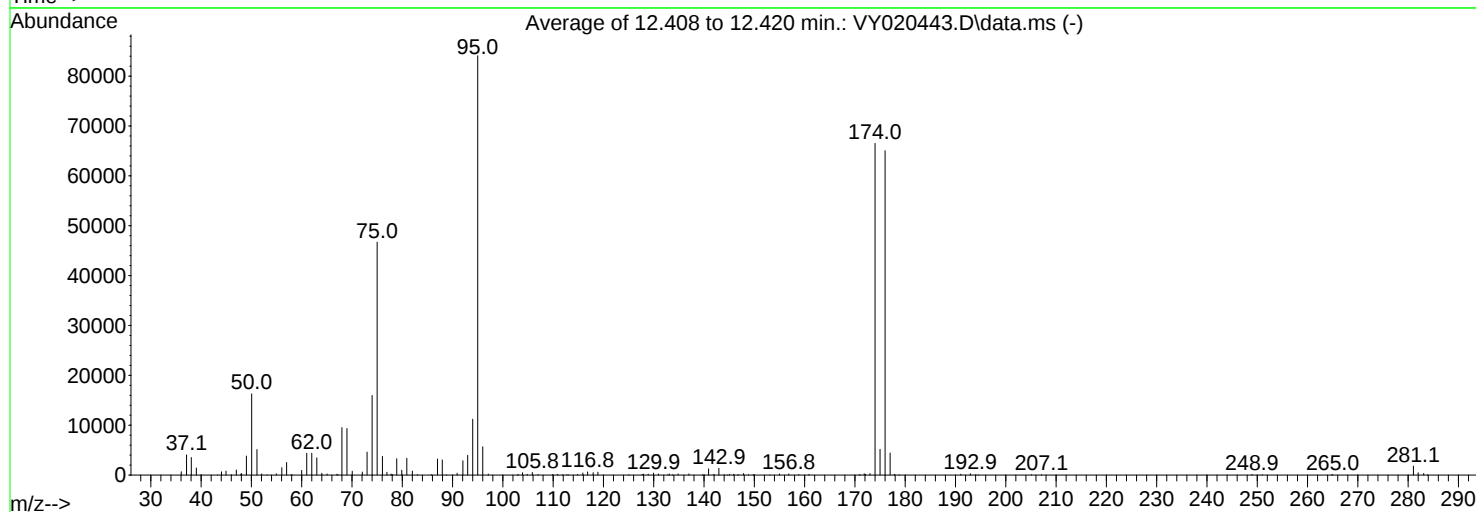


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112624\
Data File : VY020443.D
Acq On : 26 Nov 2024 09:11
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Title : SW846 8260
Last Update : Wed Nov 20 04:38:24 2024

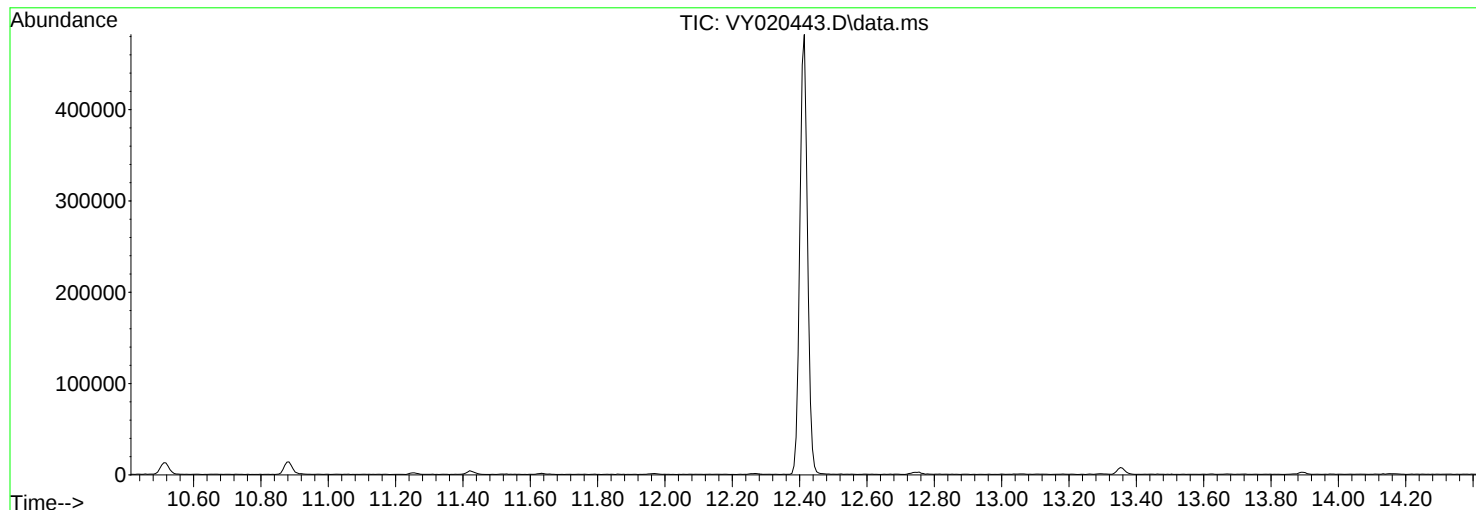

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	16285	PASS
75	95	30	60	55.6	46723	PASS
95	95	100	100	100.0	84088	PASS
96	95	5	9	6.8	5682	PASS
173	174	0.00	2	0.5	300	PASS
174	95	50	100	79.1	66531	PASS
175	174	5	9	7.8	5172	PASS
176	174	95	101	97.8	65045	PASS
177	176	5	9	6.8	4426	PASS