



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112724\
Data File : VY020454.D
Acq On : 27 Nov 2024 08:48
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111924S.M
Title : SW846 8260
Last Update : Wed Nov 20 04:38:24 2024

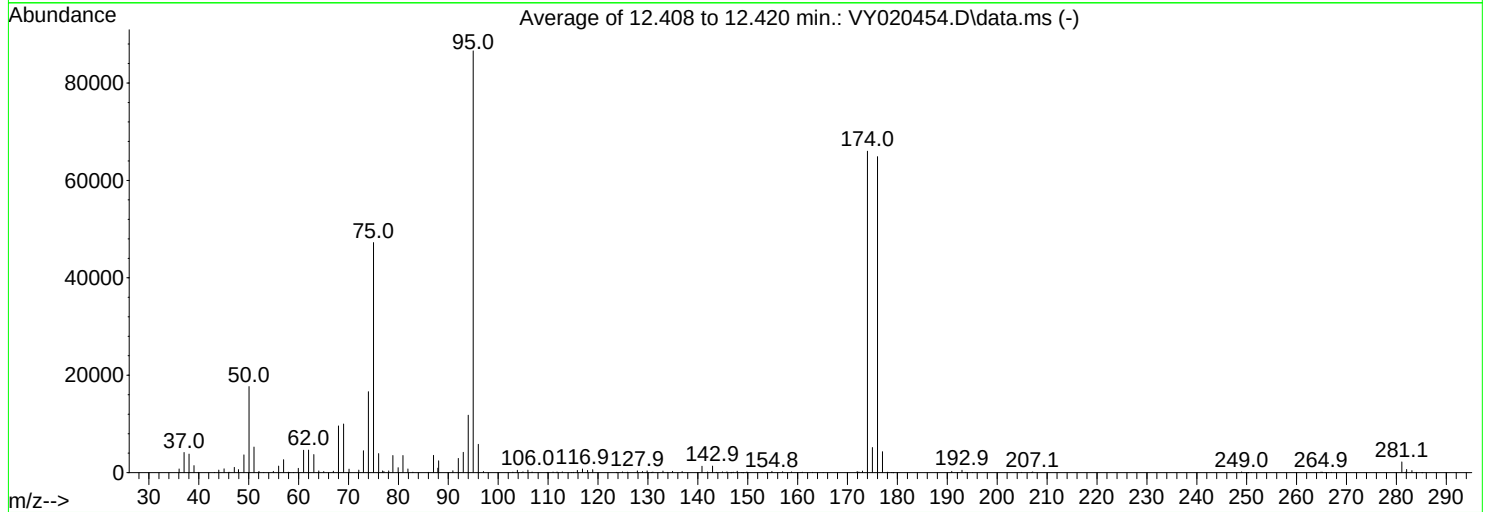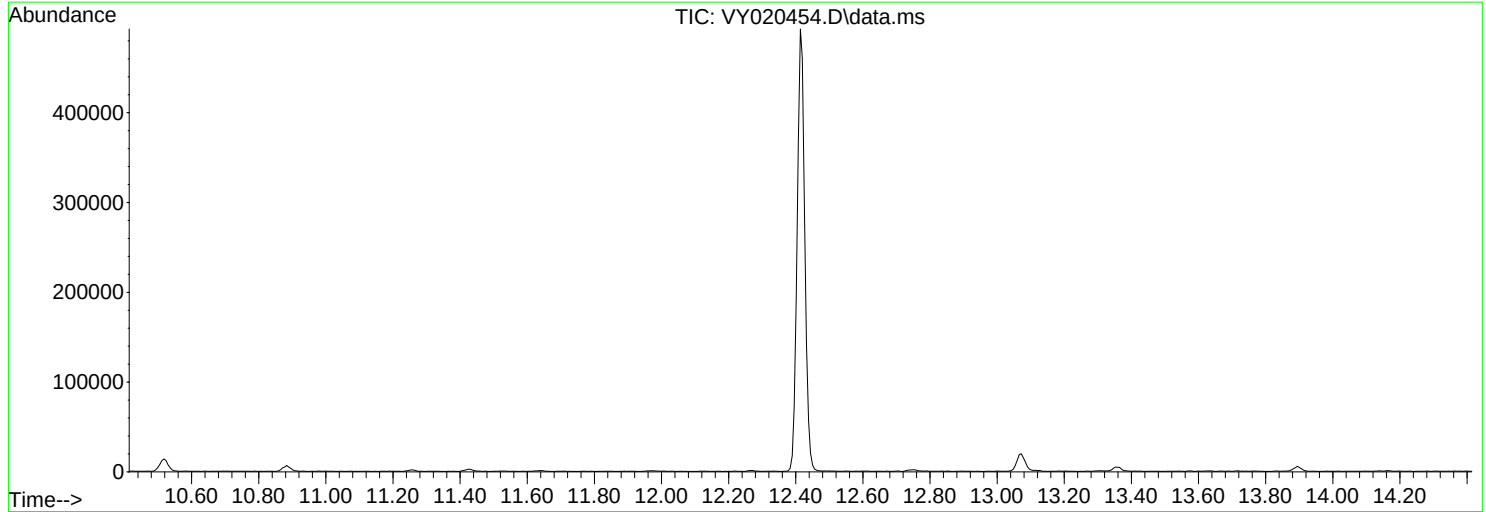

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	17668	PASS
75	95	30	60	54.6	47259	PASS
95	95	100	100	100.0	86605	PASS
96	95	5	9	6.7	5820	PASS
173	174	0.00	2	0.5	344	PASS
174	95	50	100	76.2	65997	PASS
175	174	5	9	7.8	5171	PASS
176	174	95	101	98.3	64875	PASS
177	176	5	9	6.6	4307	PASS