

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112922\
 Data File : VY011615.D
 Acq On : 29 Nov 2022 12:26
 Operator : KP/MD
 Sample : N5754-01
 Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PSC-124019

Quant Time: Nov 29 12:52:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 19 22:37:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	128115	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	237784	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	229524	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	98265	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	95388	73.326	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	146.660%
35) Dibromofluoromethane	7.722	113	80981	55.323	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.640%
50) Toluene-d8	10.179	98	287197	53.992	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	107.980%
62) 4-Bromofluorobenzene	12.483	95	93652	47.619	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	95.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY112922\
Data File : VY011615.D
Acq On : 29 Nov 2022 12:26
Operator : KP/MD
Sample : N5754-01
Misc : 5.03g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PSC-124019

Quant Time: Nov 29 12:52:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y111822S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 19 22:37:14 2022
Response via : Initial Calibration




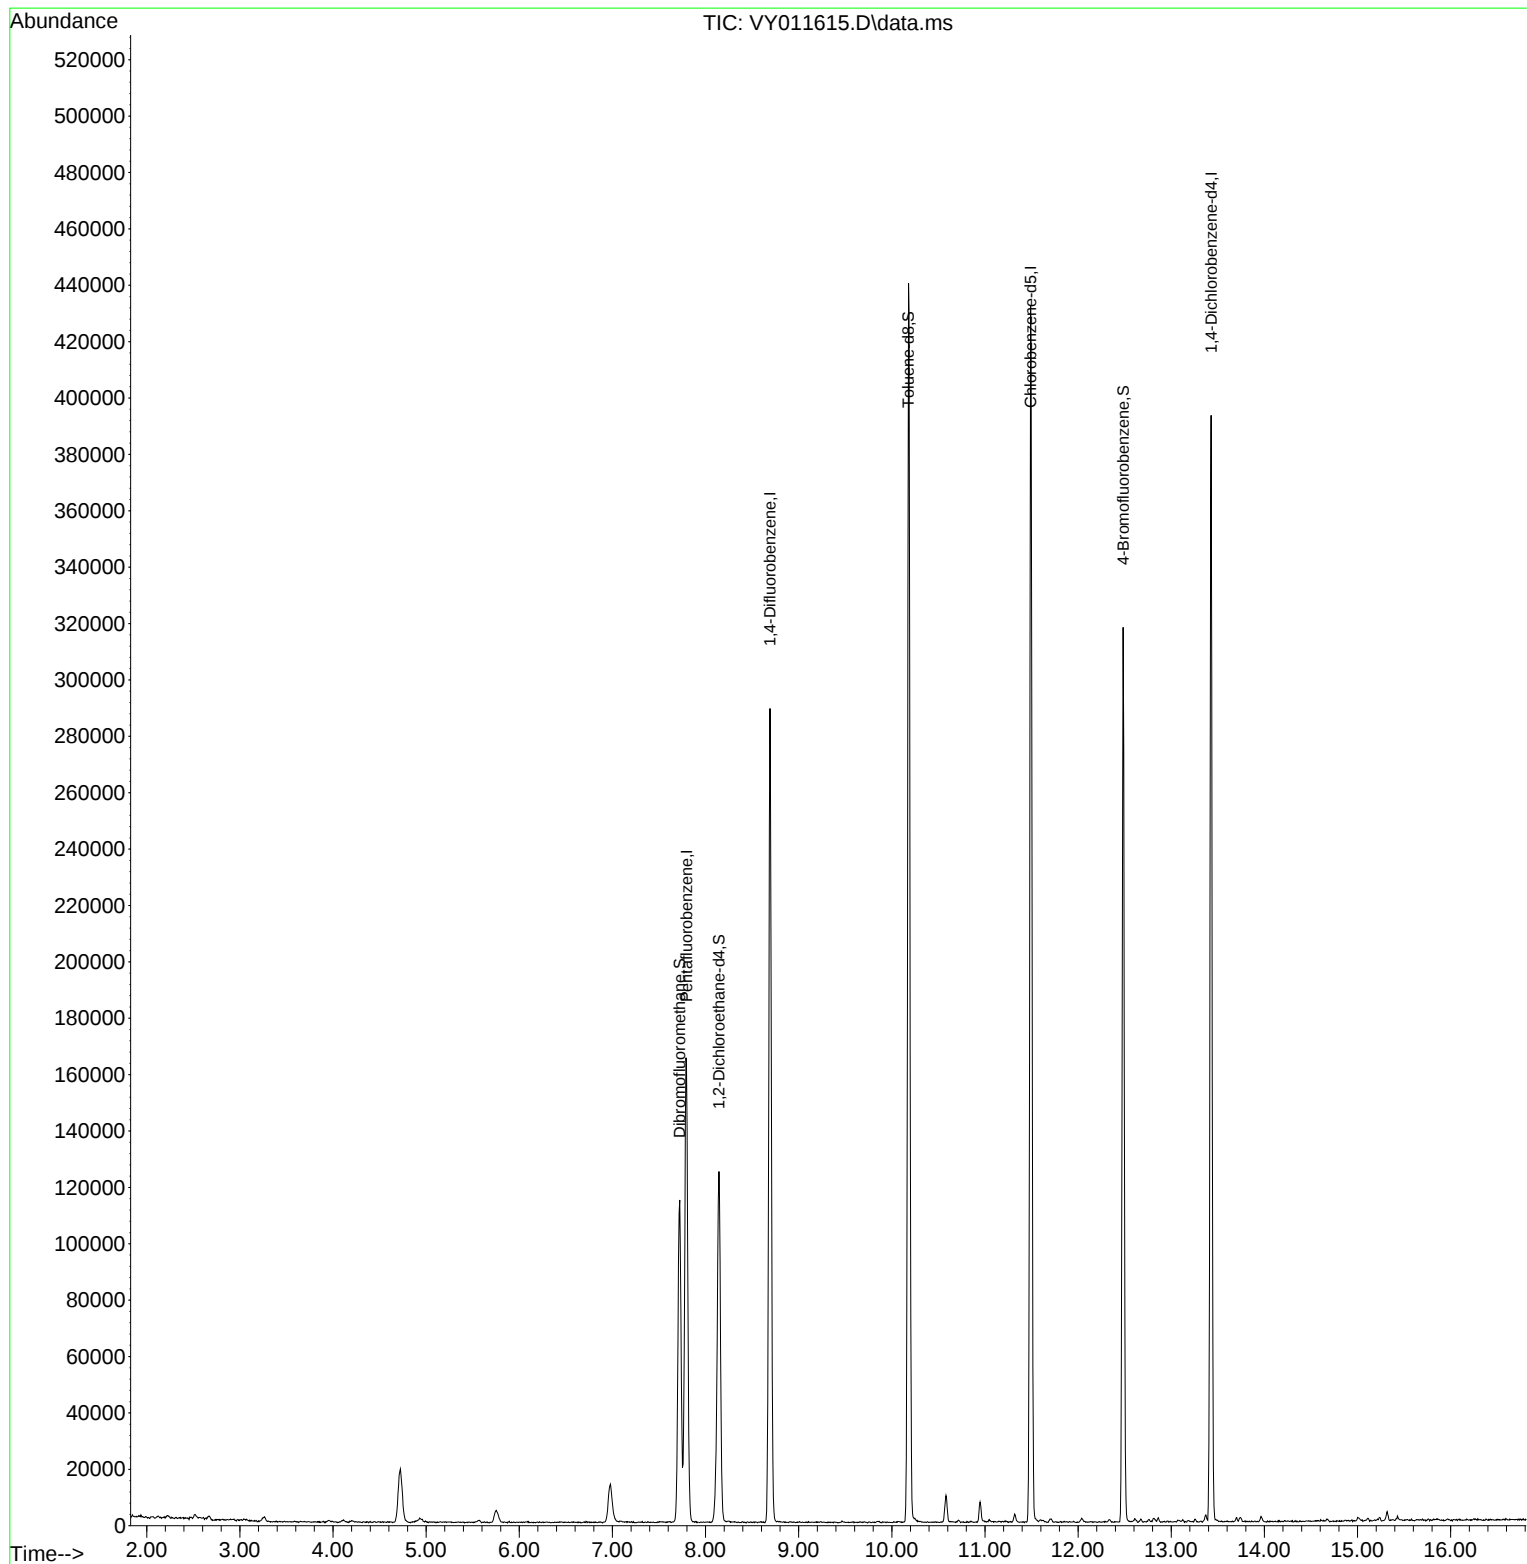


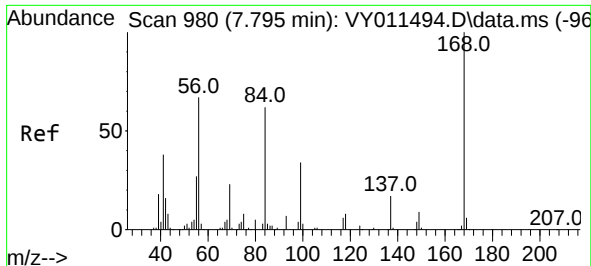

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26




Instrument :
MSVOA_Y
ClientSampleId :
PSC-124019


Tgt Ion:168 Resp: 128115
Ion Ratio Lower Upper
168 100
99 54.6 46.9 70.3

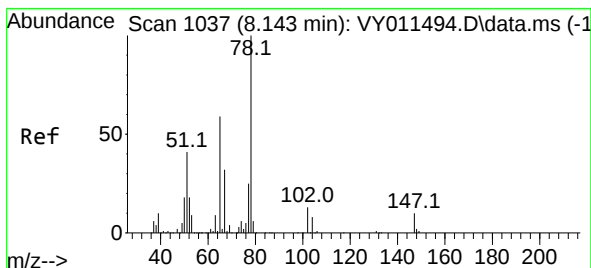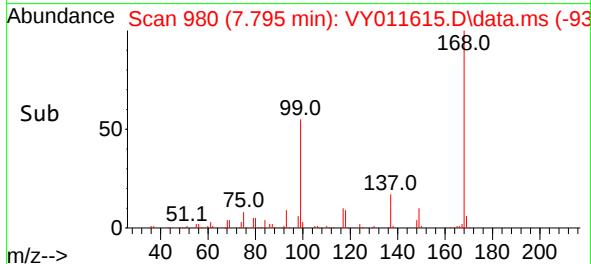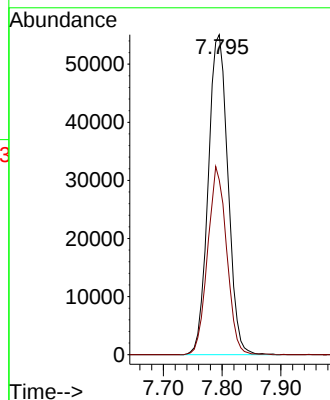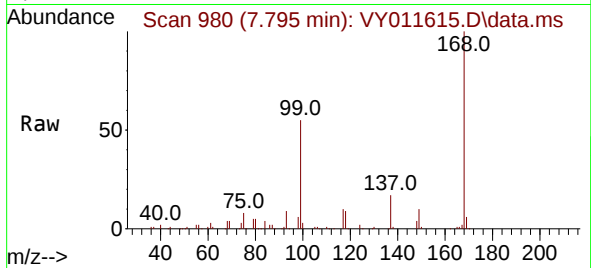

#33
1,2-Dichloroethane-d4
Concen: 73.326 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26

Tgt Ion: 65 Resp: 95388
Ion Ratio Lower Upper
65 100
67 52.4 0.0 99.4

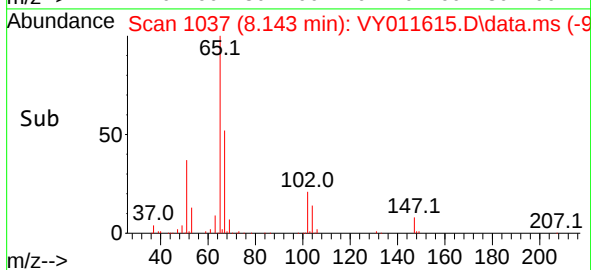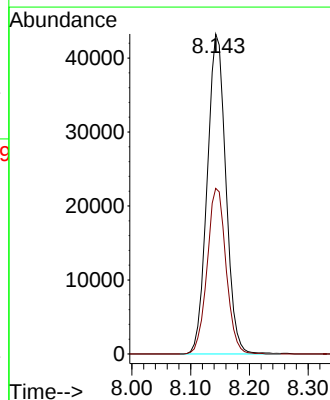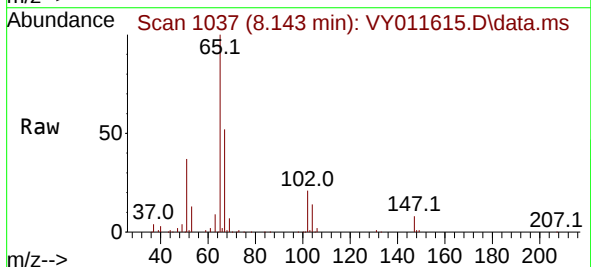

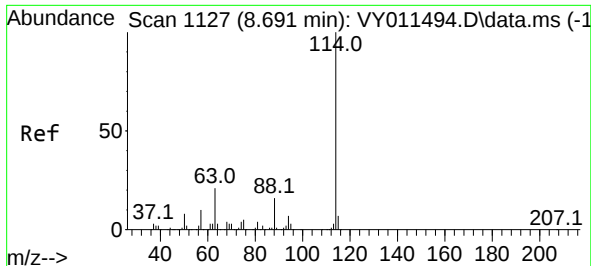

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY011615.D

Acq: 29 Nov 2022 12:26

Instrument :

MSVOA_Y

ClientSampleId :

PSC-124019





Tgt Ion:114 Resp: 237784

Ion Ratio Lower Upper

114 100

63 20.2 0.0 43.2

88 15.3 0.0 31.8

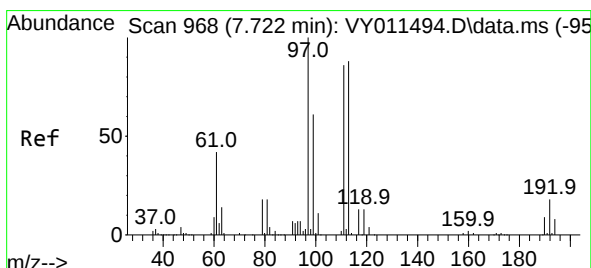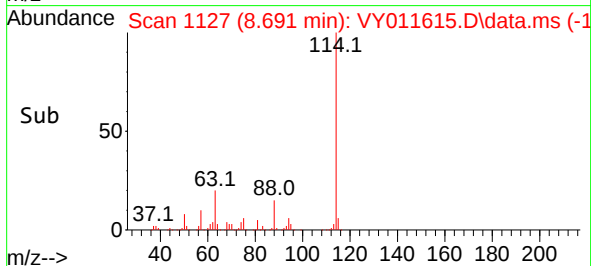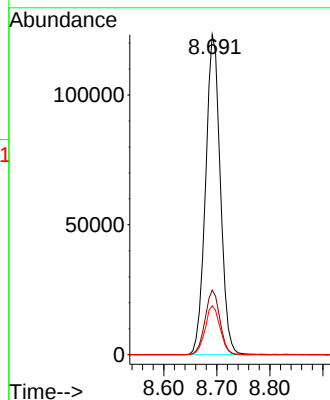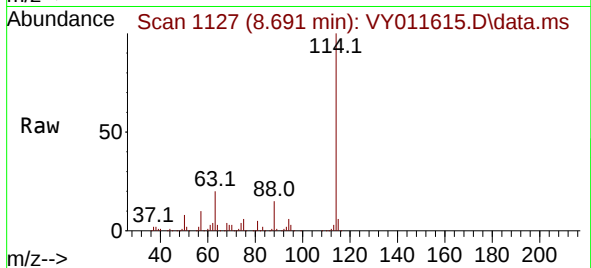

#35

Dibromofluoromethane

Concen: 55.323 ug/l

RT: 7.722 min Scan# 968

Delta R.T. 0.000 min

Lab File: VY011615.D

Acq: 29 Nov 2022 12:26




Tgt Ion:113 Resp: 80981


Ion Ratio Lower Upper

113 100

111 101.4 82.6 124.0

192 19.8 17.6 26.4


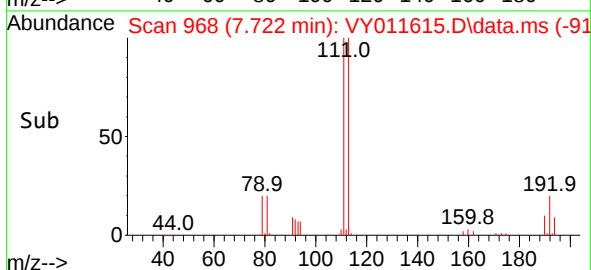
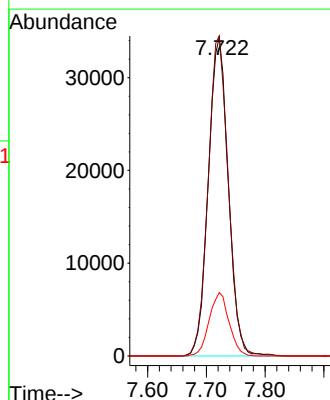
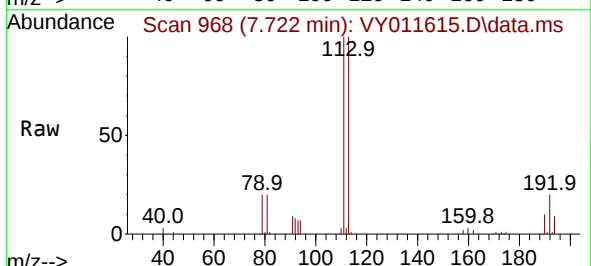


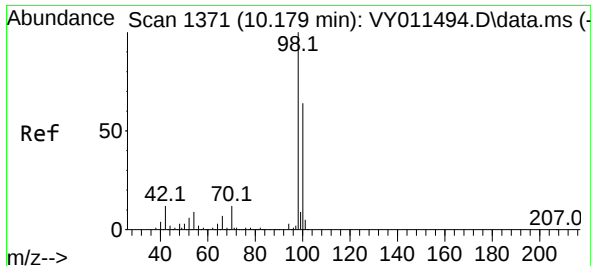

#50
Toluene-d8
Concen: 53.992 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26




Instrument :
MSVOA_Y
ClientSampleId :
PSC-124019


Tgt Ion: 98 Resp: 287197
Ion Ratio Lower Upper
98 100
100 64.4 50.2 75.2

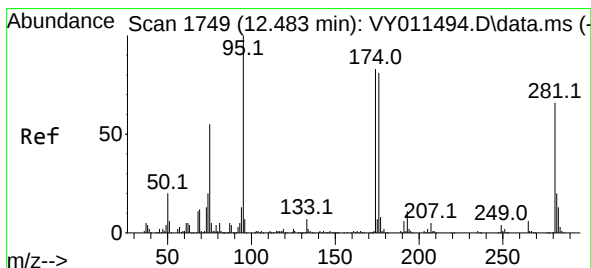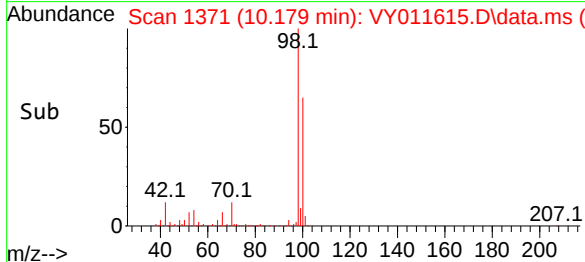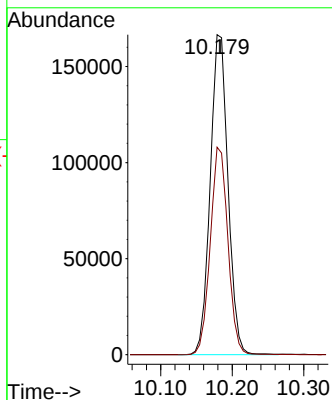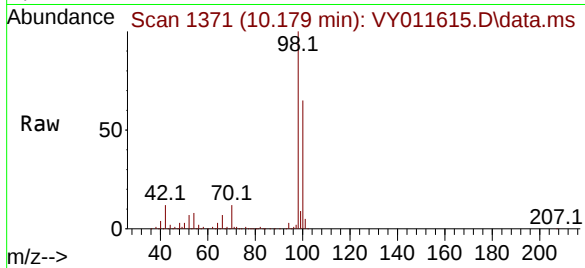

#62
4-Bromofluorobenzene
Concen: 47.619 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26

Tgt Ion: 95 Resp: 93652
Ion Ratio Lower Upper
95 100
174 85.2 0.0 177.0
176 81.3 0.0 175.8


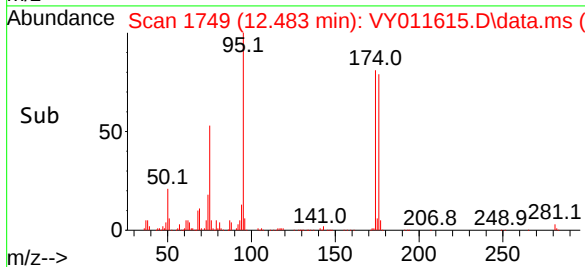
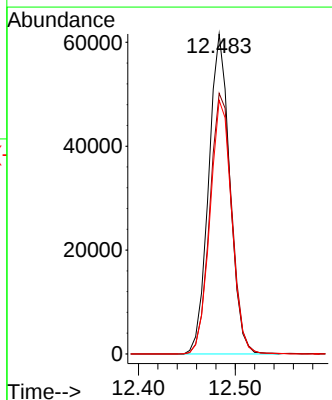
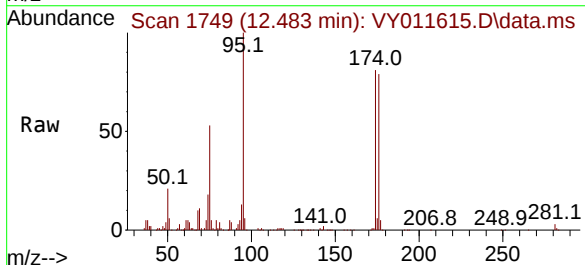


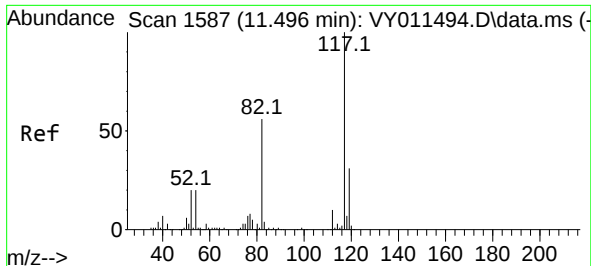

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26

Instrument :
MSVOA_Y
ClientSampleId :
PSC-124019

Tgt Ion:117 Resp: 229524
Ion Ratio Lower Upper
117 100
82 57.9 43.0 64.4
119 31.7 25.4 38.0

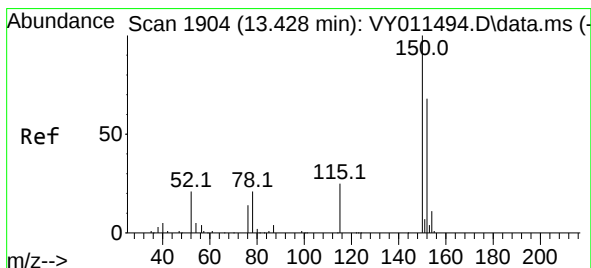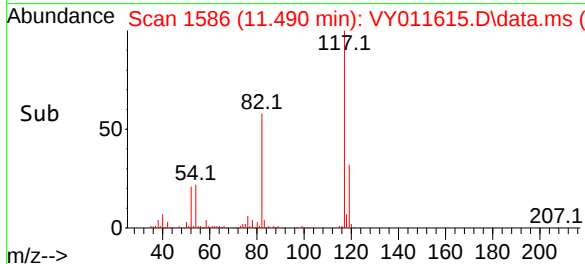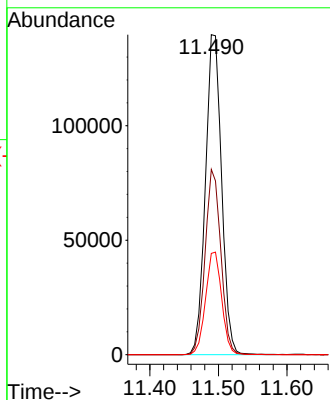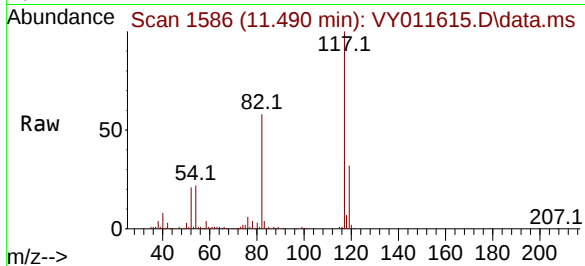

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY011615.D
Acq: 29 Nov 2022 12:26

Tgt Ion:152 Resp: 98265
Ion Ratio Lower Upper
152 100
115 59.5 28.2 84.7
150 156.7 0.0 347.6

