
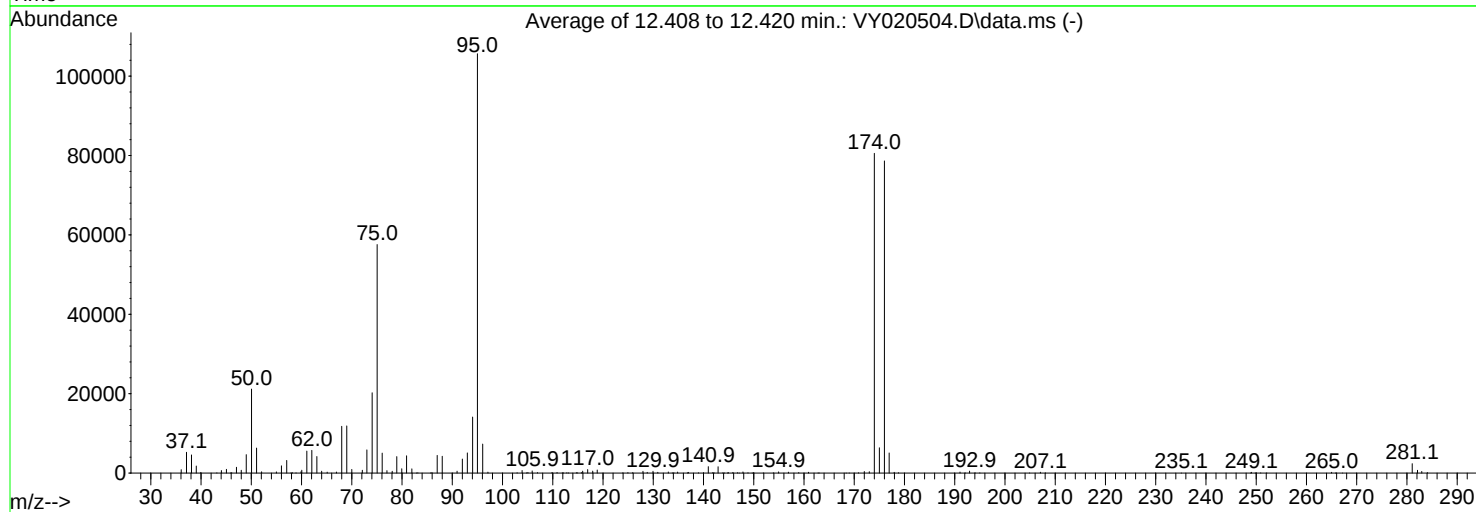


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY120424\
Data File : VY020504.D
Acq On : 04 Dec 2024 09:04
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y120224S.M
Title : SW846 8260
Last Update : Tue Dec 03 01:39:23 2024

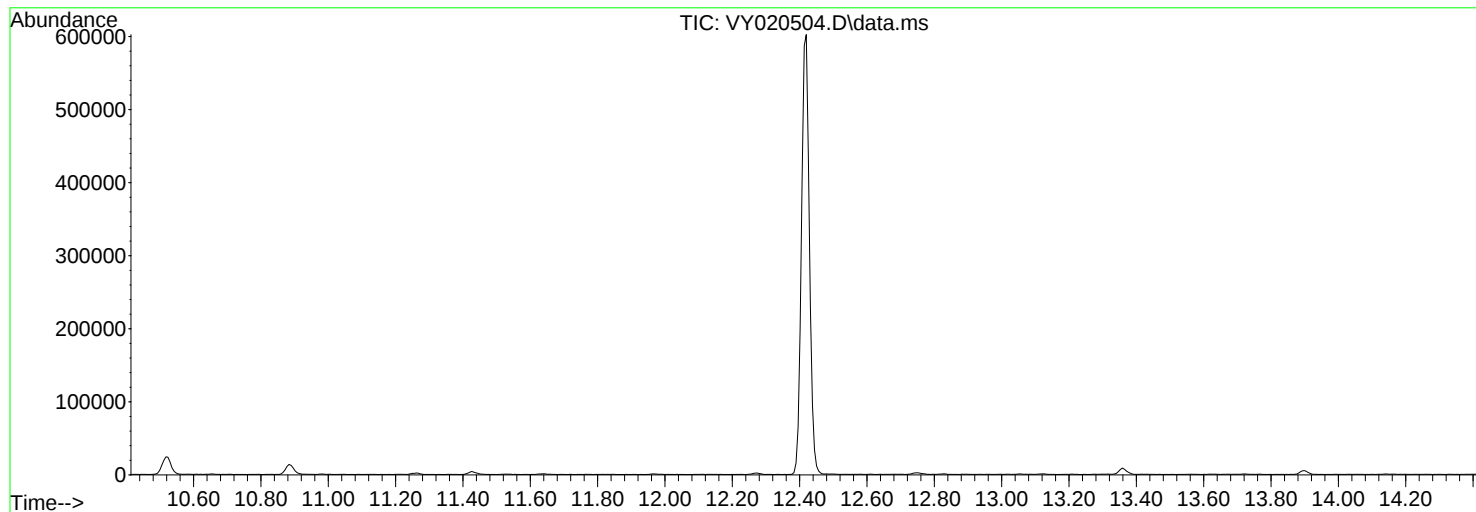

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	21163	PASS
75	95	30	60	54.5	57571	PASS
95	95	100	100	100.0	105645	PASS
96	95	5	9	6.9	7308	PASS
173	174	0.00	2	0.4	352	PASS
174	95	50	100	76.2	80544	PASS
175	174	5	9	7.9	6373	PASS
176	174	95	101	97.6	78637	PASS
177	176	5	9	6.4	5067	PASS