
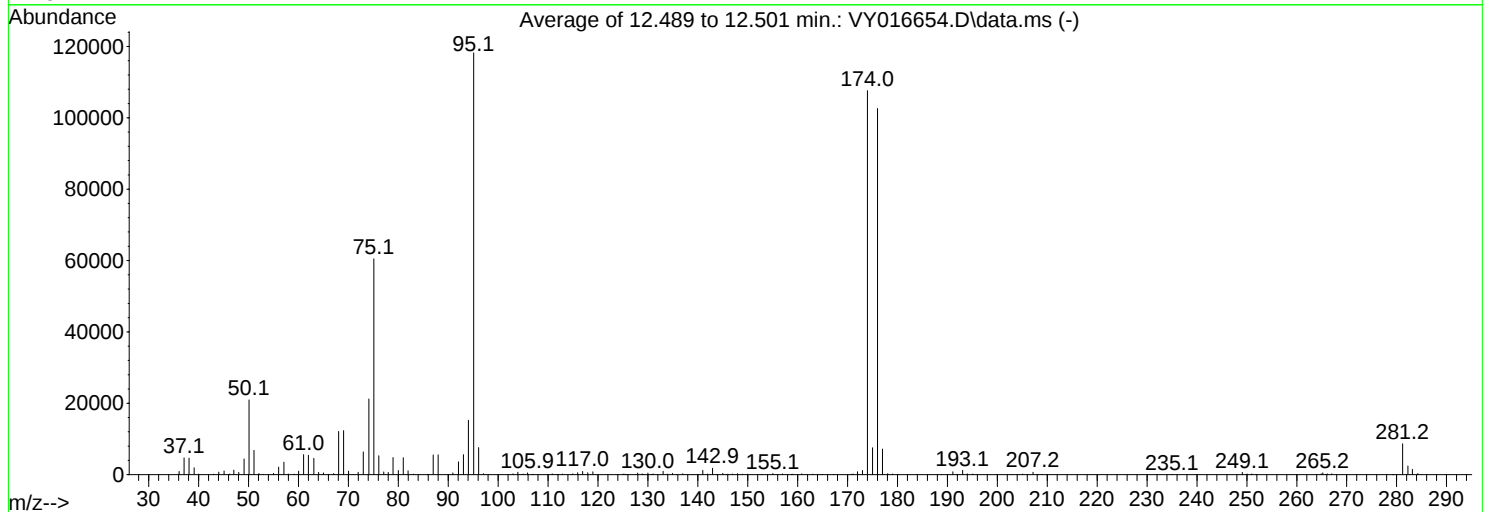


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121523\
Data File : VY016654.D
Acq On : 15 Dec 2023 14:09
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121523S.M
Title : SW846 8260
Last Update : Sat Dec 16 00:39:52 2023

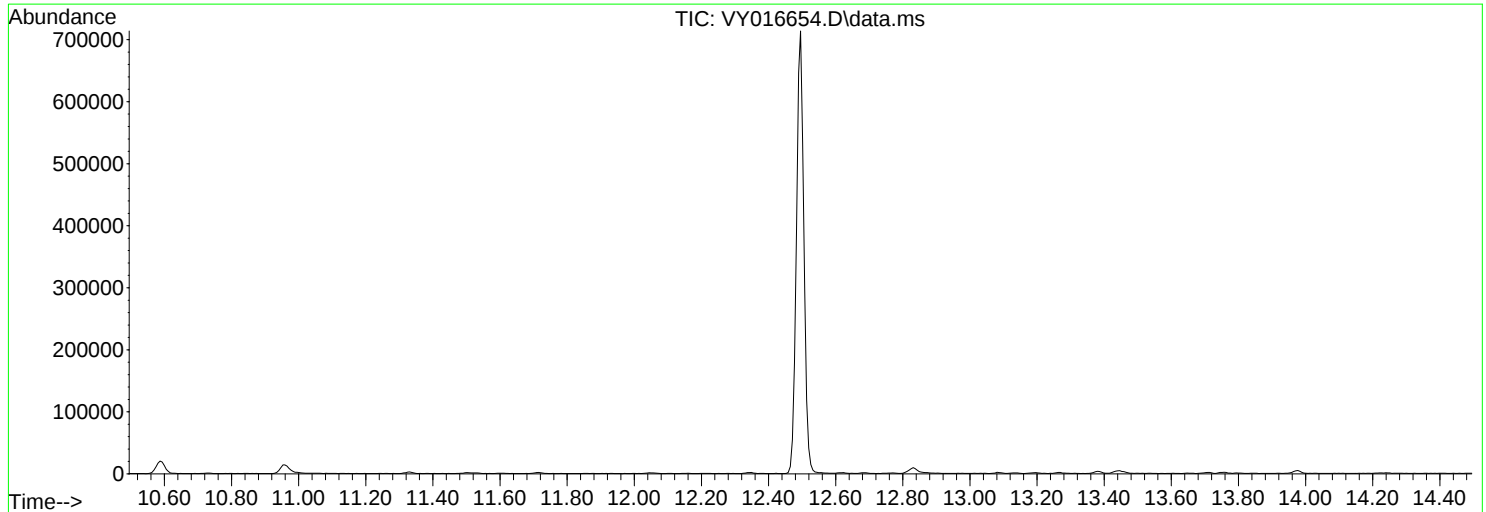

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	20954	PASS
75	95	30	60	51.2	60499	PASS
95	95	100	100	100.0	118205	PASS
96	95	5	9	6.4	7573	PASS
173	174	0.00	2	1.1	1162	PASS
174	95	50	100	91.0	107597	PASS
175	174	5	9	7.0	7516	PASS
176	174	95	101	95.4	102600	PASS
177	176	5	9	7.0	7160	PASS