
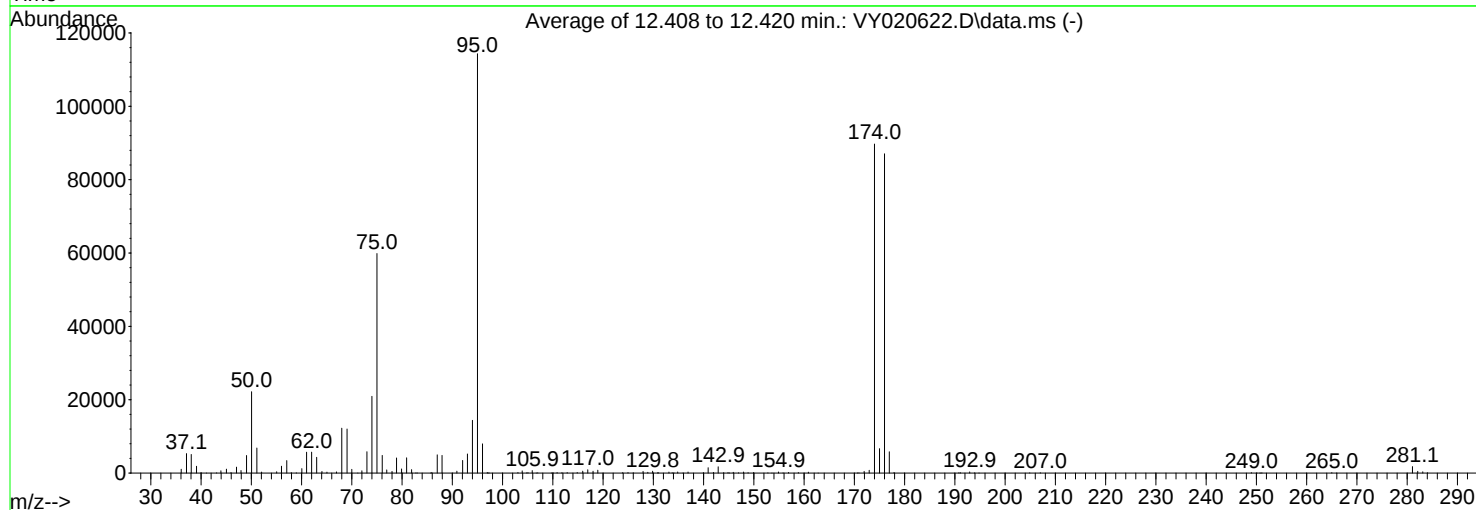


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121824\
Data File : VY020622.D
Acq On : 18 Dec 2024 08:46
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121724S.M
Title : SW846 8260
Last Update : Wed Dec 18 05:27:13 2024

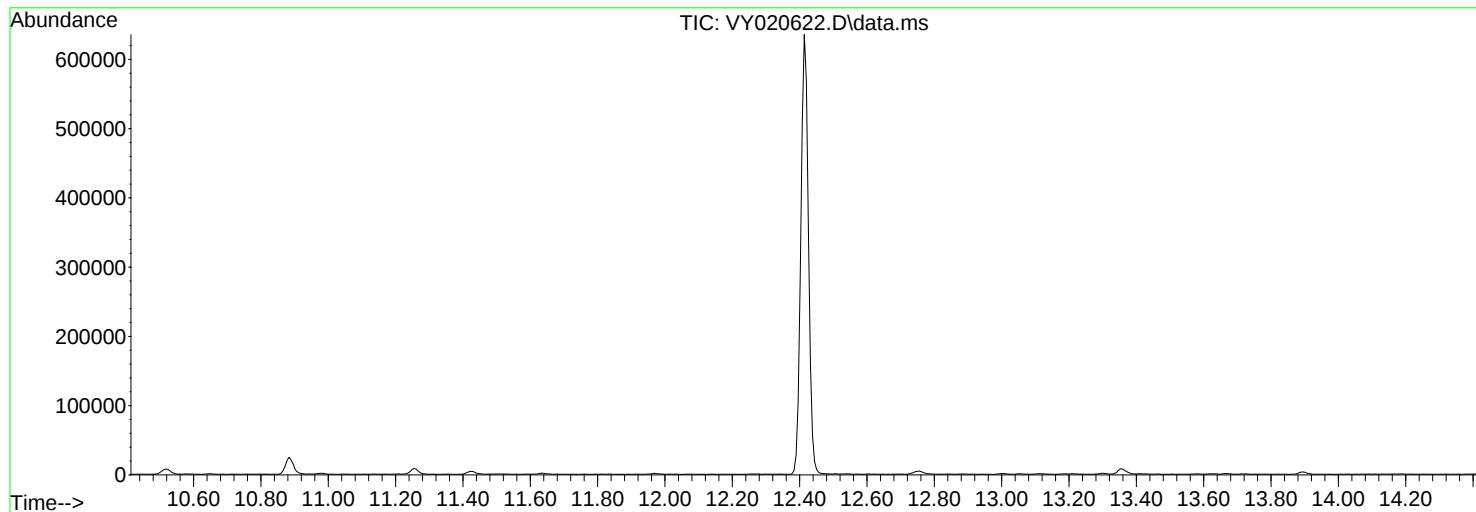

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	22181	PASS
75	95	30	60	52.4	59867	PASS
95	95	100	100	100.0	114336	PASS
96	95	5	9	7.0	7972	PASS
173	174	0.00	2	0.9	765	PASS
174	95	50	100	78.5	89720	PASS
175	174	5	9	7.4	6659	PASS
176	174	95	101	97.0	87059	PASS
177	176	5	9	6.7	5814	PASS