

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122023\
 Data File : VY016746.D
 Acq On : 21 Dec 2023 07:31
 Operator : SY/MD
 Sample : 05876-15
 Misc : 2.15g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 COLY0

Quant Time: Dec 21 08:14:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 21 01:49:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.825	168	108615	50.000	ug/l	0.02
34) 1,4-Difluorobenzene	8.722	114	320934	50.000	ug/l	0.02
63) Chlorobenzene-d5	11.514	117	355830	50.000	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.446	152	142112	50.000	ug/l	0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.173	65	95636	96.452	ug/l	0.02
Spiked Amount	50.000	Range	50 - 163	Recovery	=	192.900%#
35) Dibromofluoromethane	7.752	113	114822	62.458	ug/l	0.02
Spiked Amount	50.000	Range	54 - 147	Recovery	=	124.920%
50) Toluene-d8	10.203	98	423945	63.970	ug/l	0.01
Spiked Amount	50.000	Range	58 - 134	Recovery	=	127.940%
62) 4-Bromofluorobenzene	12.501	95	150877	70.173	ug/l	0.01
Spiked Amount	50.000	Range	30 - 143	Recovery	=	140.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122023\
Data File : VY016746.D
Acq On : 21 Dec 2023 07:31
Operator : SY/MD
Sample : 05876-15
Misc : 2.15g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
COLY0

Quant Time: Dec 21 08:14:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 21 01:49:45 2023
Response via : Initial Calibration




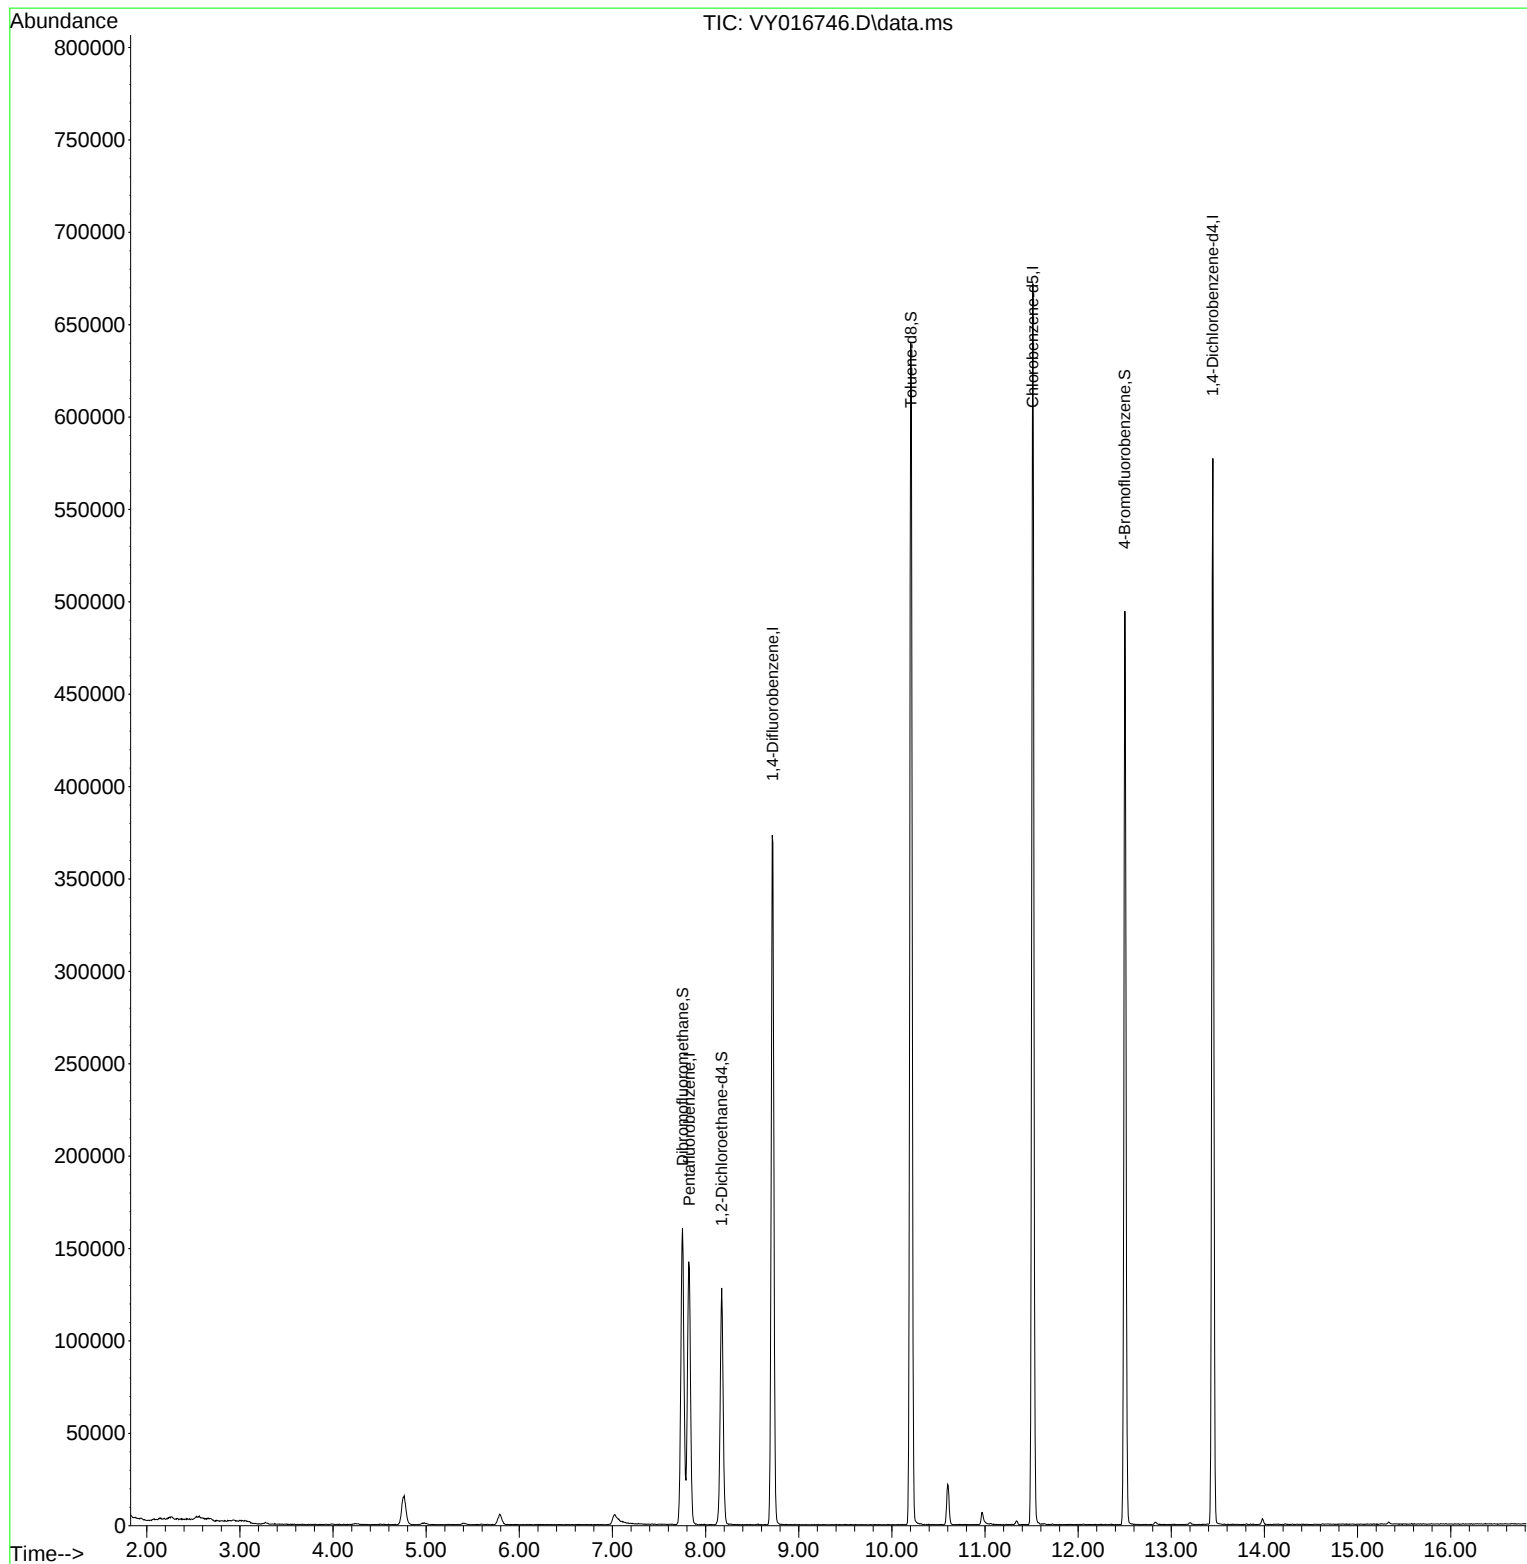


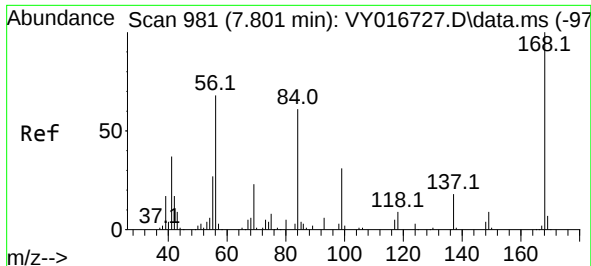

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.825 min Scan# 91
Delta R.T. 0.024 min
Lab File: VY016746.D
Acq: 21 Dec 2023 07:31




Instrument :
MSVOA_Y
ClientSampleId :
COLY0


Tgt Ion:168 Resp: 108615
Ion Ratio Lower Upper
168 100
99 54.5 44.2 66.4

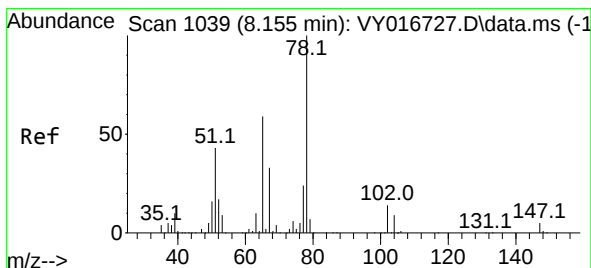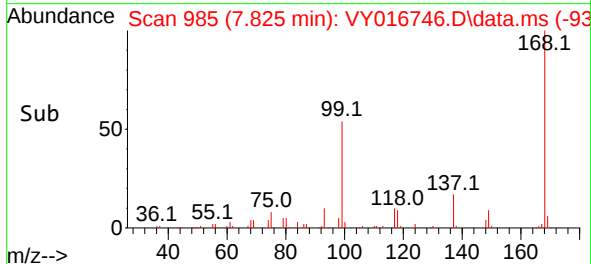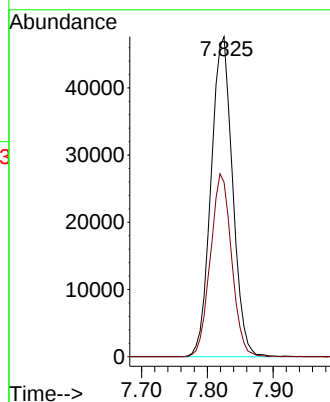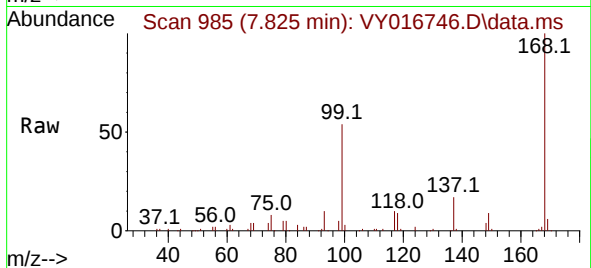

#33
1,2-Dichloroethane-d4
Concen: 96.452 ug/l
RT: 8.173 min Scan# 1042
Delta R.T. 0.018 min
Lab File: VY016746.D
Acq: 21 Dec 2023 07:31

Tgt Ion: 65 Resp: 95636
Ion Ratio Lower Upper
65 100
67 54.6 0.0 109.0

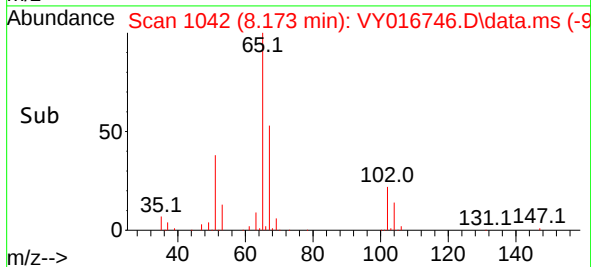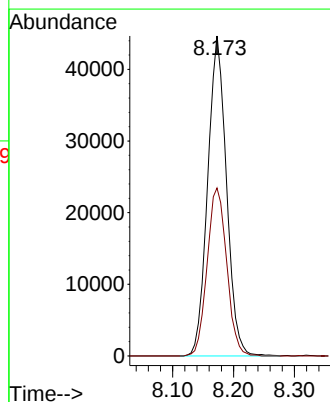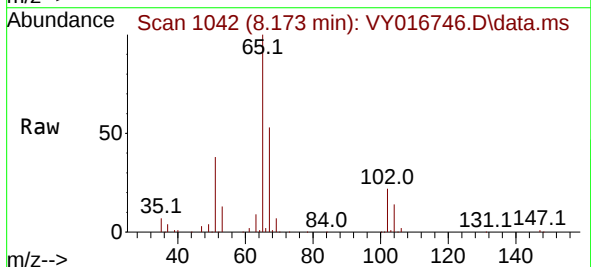

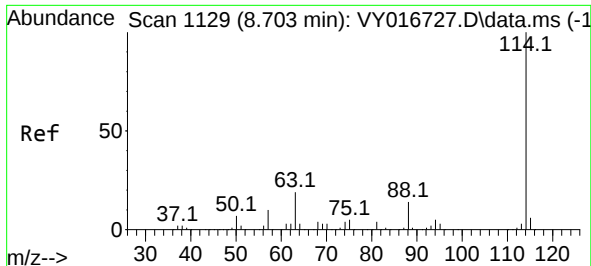

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.722 min Scan# 1129

Delta R.T. 0.019 min

Lab File: VY016746.D

Acq: 21 Dec 2023 07:31

Instrument :

MSVOA_Y

ClientSampleId :

COLY0





Tgt Ion:114 Resp: 320934

Ion Ratio Lower Upper

114 100

63 19.7 0.0 37.4

88 14.8 0.0 29.0

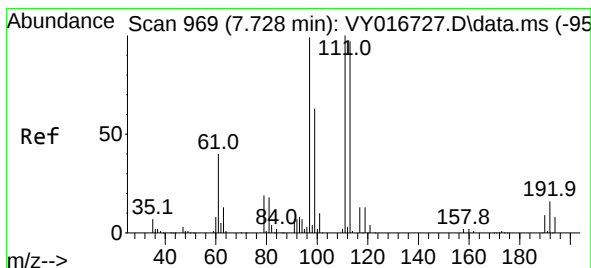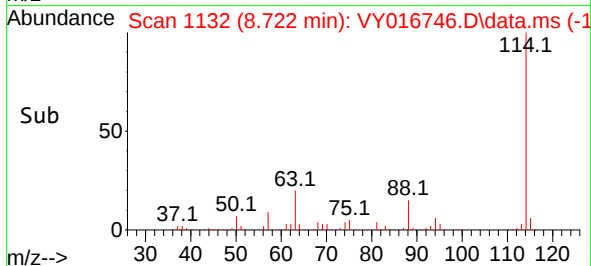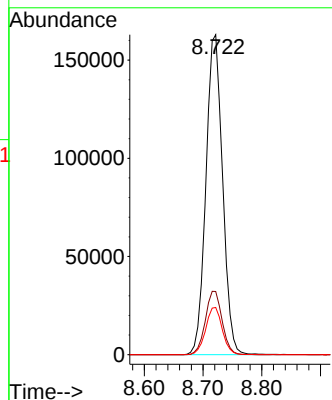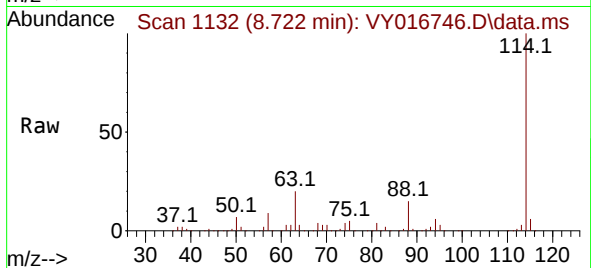

#35

Dibromofluoromethane

Concen: 62.458 ug/l

RT: 7.752 min Scan# 973

Delta R.T. 0.024 min

Lab File: VY016746.D

Acq: 21 Dec 2023 07:31




Tgt Ion:113 Resp: 114822


Ion Ratio Lower Upper

113 100

111 103.8 83.8 125.6

192 18.0 14.5 21.7


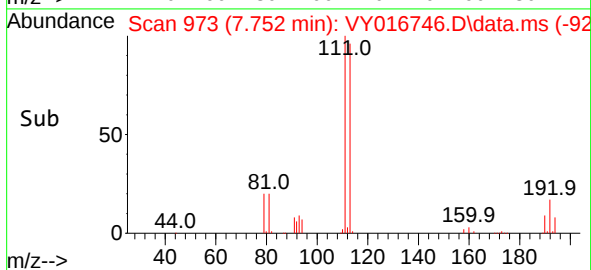
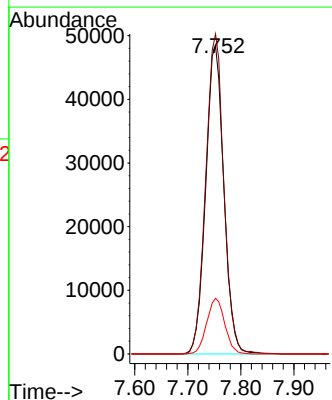
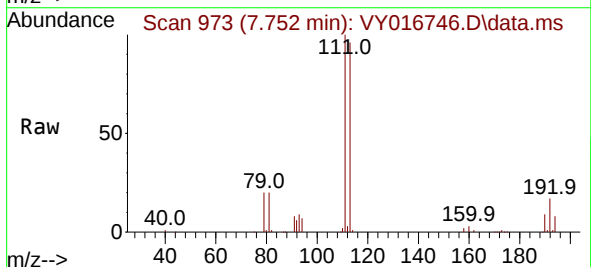


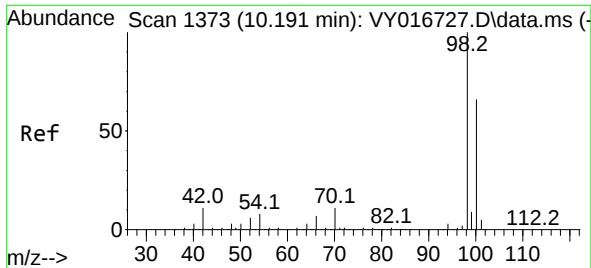

#50
Toluene-d8
Concen: 63.970 ug/l
RT: 10.203 min Scan# 11
Delta R.T. 0.012 min
Lab File: VY016746.D
Acq: 21 Dec 2023 07:31




Instrument :
MSVOA_Y
ClientSampleId :
COLY0


Tgt Ion: 98 Resp: 423945
Ion Ratio Lower Upper
98 100
100 65.6 52.3 78.5

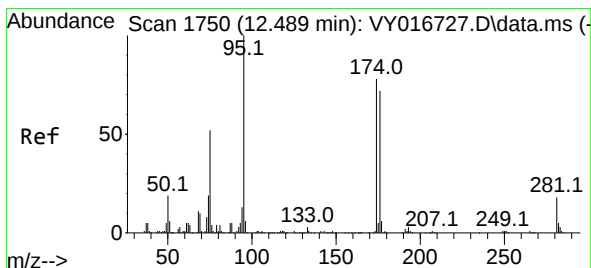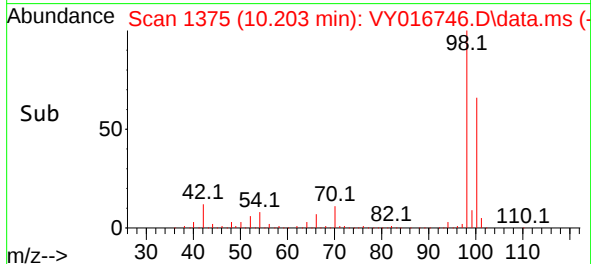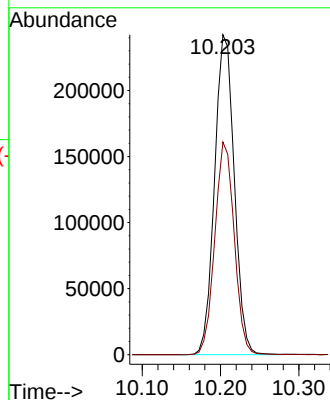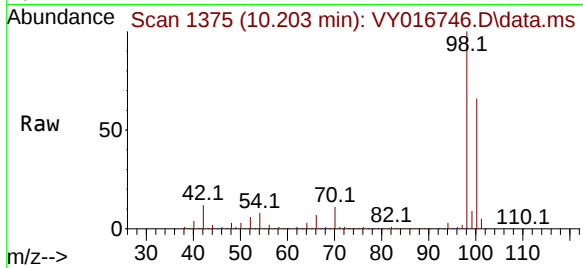

#62
4-Bromofluorobenzene
Concen: 70.173 ug/l
RT: 12.501 min Scan# 1752
Delta R.T. 0.012 min
Lab File: VY016746.D
Acq: 21 Dec 2023 07:31

Tgt Ion: 95 Resp: 150877
Ion Ratio Lower Upper
95 100
174 79.1 0.0 160.0
176 75.4 0.0 151.8

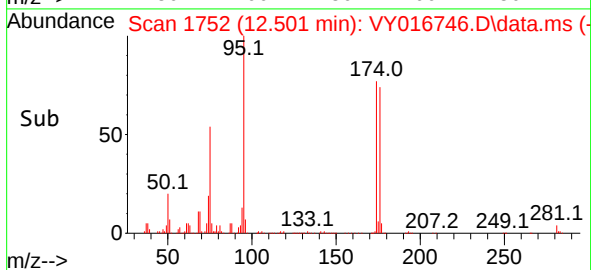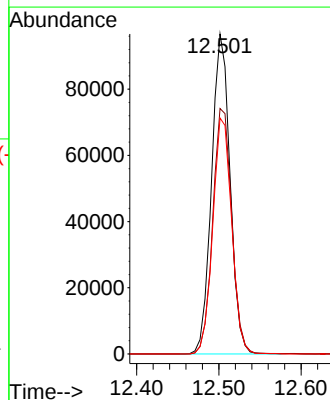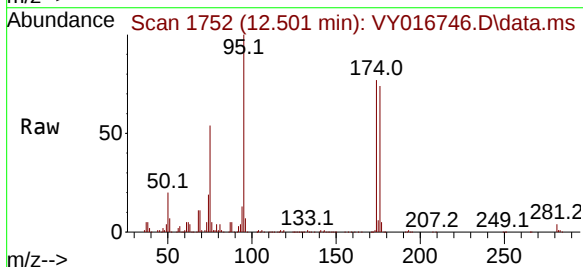

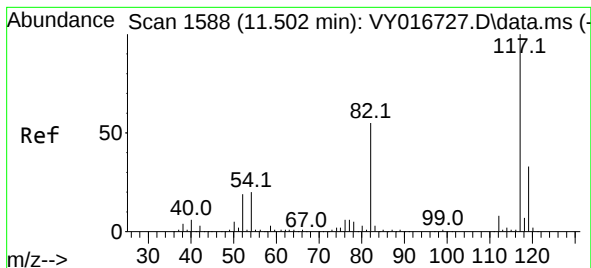

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.514 min Scan# 11

Delta R.T. 0.012 min

Lab File: VY016746.D

Acq: 21 Dec 2023 07:31

Instrument :

MSVOA_Y

ClientSampleId :

COLY0





Tgt Ion:117 Resp: 355830

Ion Ratio Lower Upper

117 100

82 55.5 43.8 65.8

119 31.9 26.5 39.7

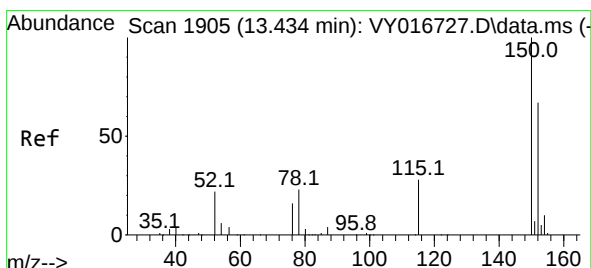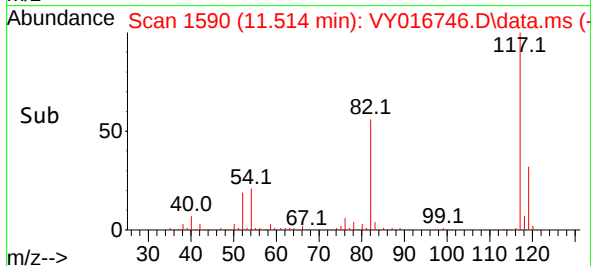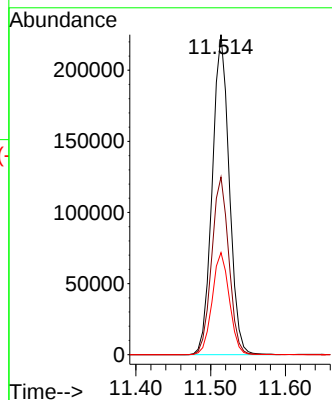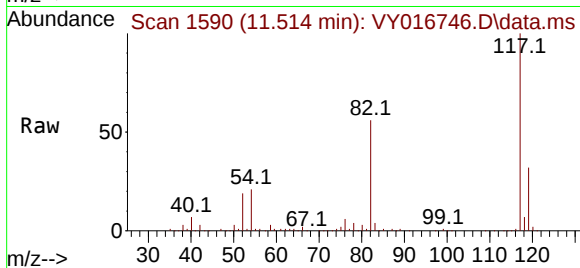

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.446 min Scan# 1907

Delta R.T. 0.012 min

Lab File: VY016746.D

Acq: 21 Dec 2023 07:31

Tgt Ion:152 Resp: 142112

Ion Ratio Lower Upper

152 100

115 59.6 30.0 90.0

150 157.5 0.0 344.6

