
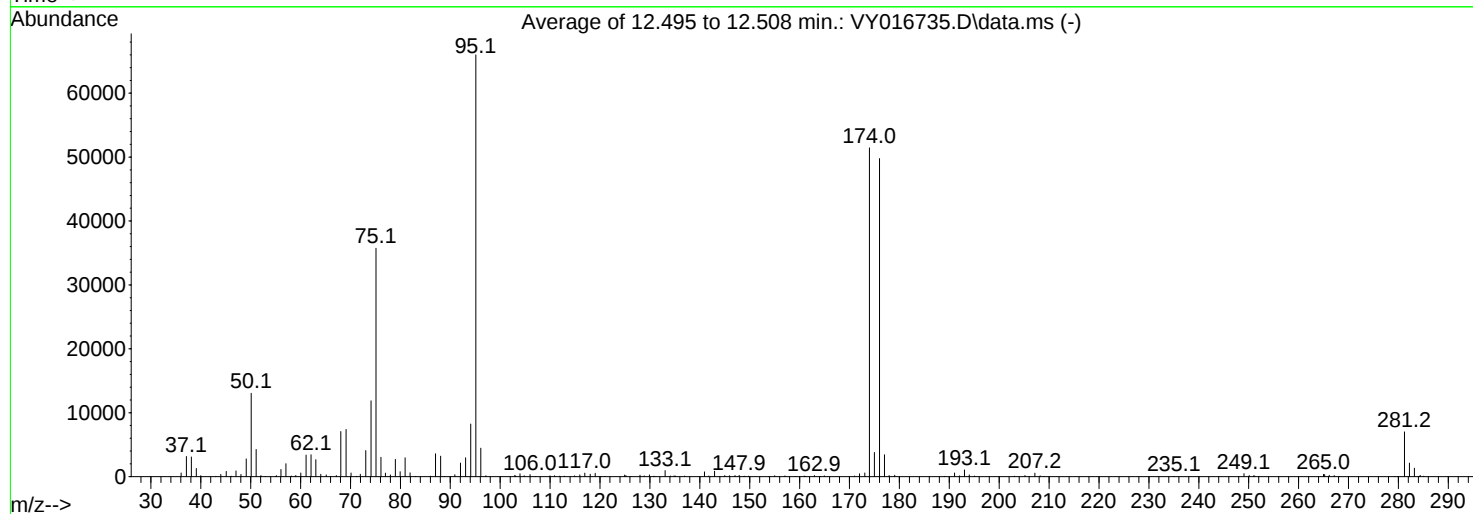


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY122023\  
Data File : VY016735.D  
Acq On : 21 Dec 2023 01:51  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y122023S.M  
Title : SW846 8260  
Last Update : Thu Dec 21 01:49:45 2023

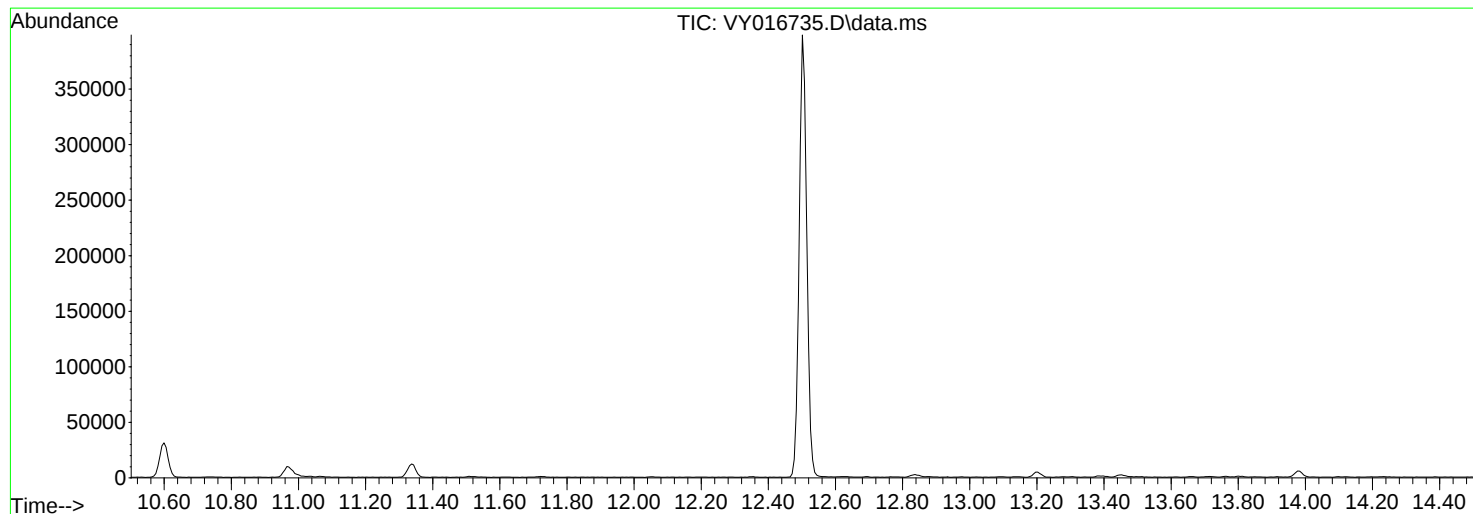

AutoFind: Scans 1751, 1752, 1753; Background Corrected with Scan 1743

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.8  | 13048 | PASS      |
| 75     | 95      | 30     | 60     | 54.1  | 35733 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 66003 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 4448  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 571   | PASS      |
| 174    | 95      | 50     | 100    | 77.9  | 51445 | PASS      |
| 175    | 174     | 5      | 9      | 7.4   | 3787  | PASS      |
| 176    | 174     | 95     | 101    | 96.7  | 49768 | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 3435  | PASS      |