
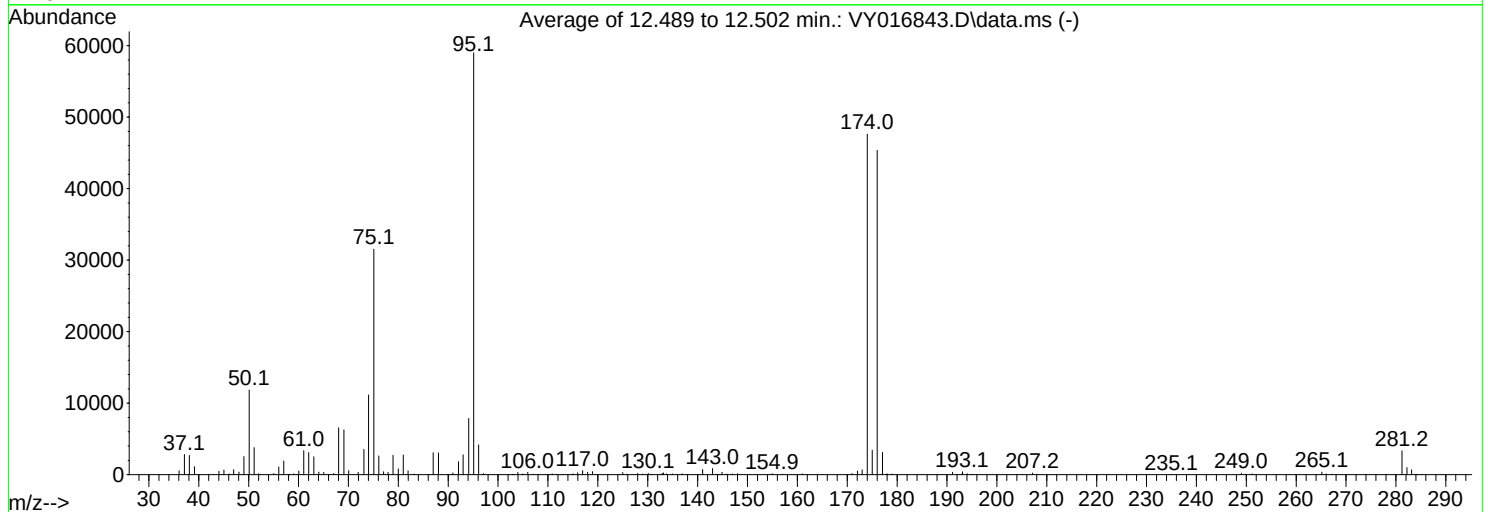


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122623\
Data File : VY016843.D
Acq On : 26 Dec 2023 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122023S.M
Title : SW846 8260
Last Update : Thu Dec 21 01:49:45 2023

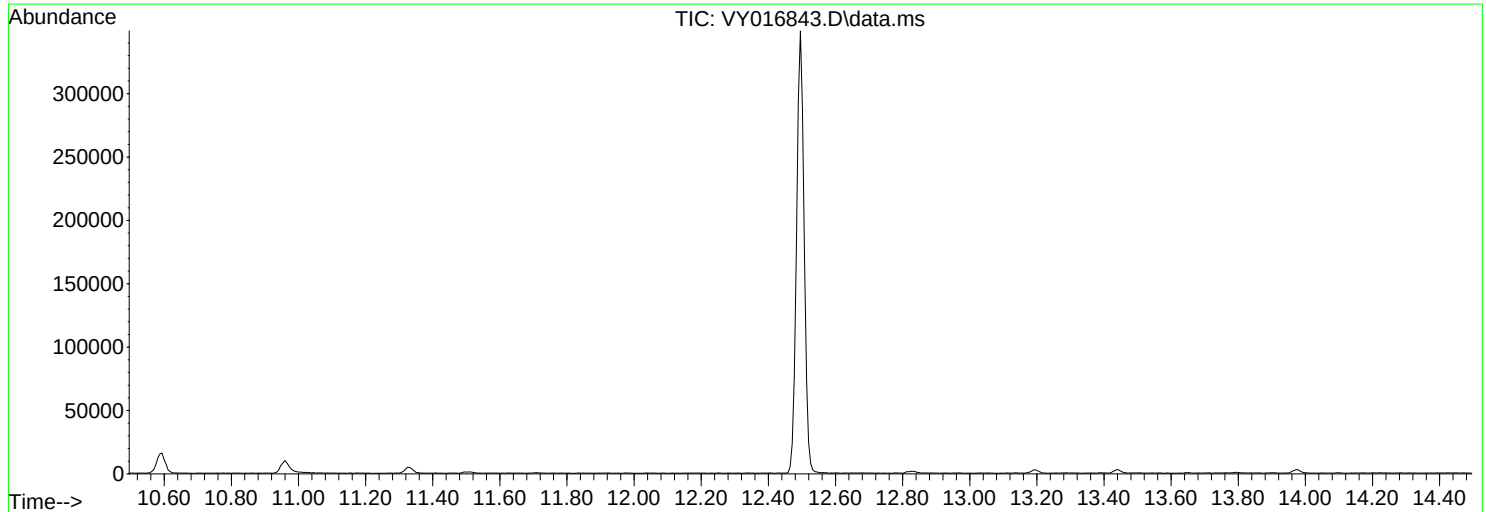

AutoFind: Scans 1750, 1751, 1752; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	11829	PASS
75	95	30	60	53.4	31528	PASS
95	95	100	100	100.0	58987	PASS
96	95	5	9	7.1	4168	PASS
173	174	0.00	2	1.4	676	PASS
174	95	50	100	80.7	47621	PASS
175	174	5	9	7.2	3425	PASS
176	174	95	101	95.3	45360	PASS
177	176	5	9	6.8	3101	PASS