

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122922\
 Data File : VY012022.D
 Acq On : 29 Dec 2022 12:54
 Operator : KP/MD
 Sample : VY1229SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY1229SBL01

Quant Time: Dec 30 03:56:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 20 12:37:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	167940	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	268958	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	244089	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	118615	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	96879	57.258	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.520%
35) Dibromofluoromethane	7.716	113	86110	53.180	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	106.360%
50) Toluene-d8	10.179	98	327753	49.890	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.780%
62) 4-Bromofluorobenzene	12.483	95	107929	48.849	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	97.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122922\
Data File : VY012022.D
Acq On : 29 Dec 2022 12:54
Operator : KP/MD
Sample : VY1229SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY1229SBL01

Quant Time: Dec 30 03:56:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 20 12:37:37 2022
Response via : Initial Calibration




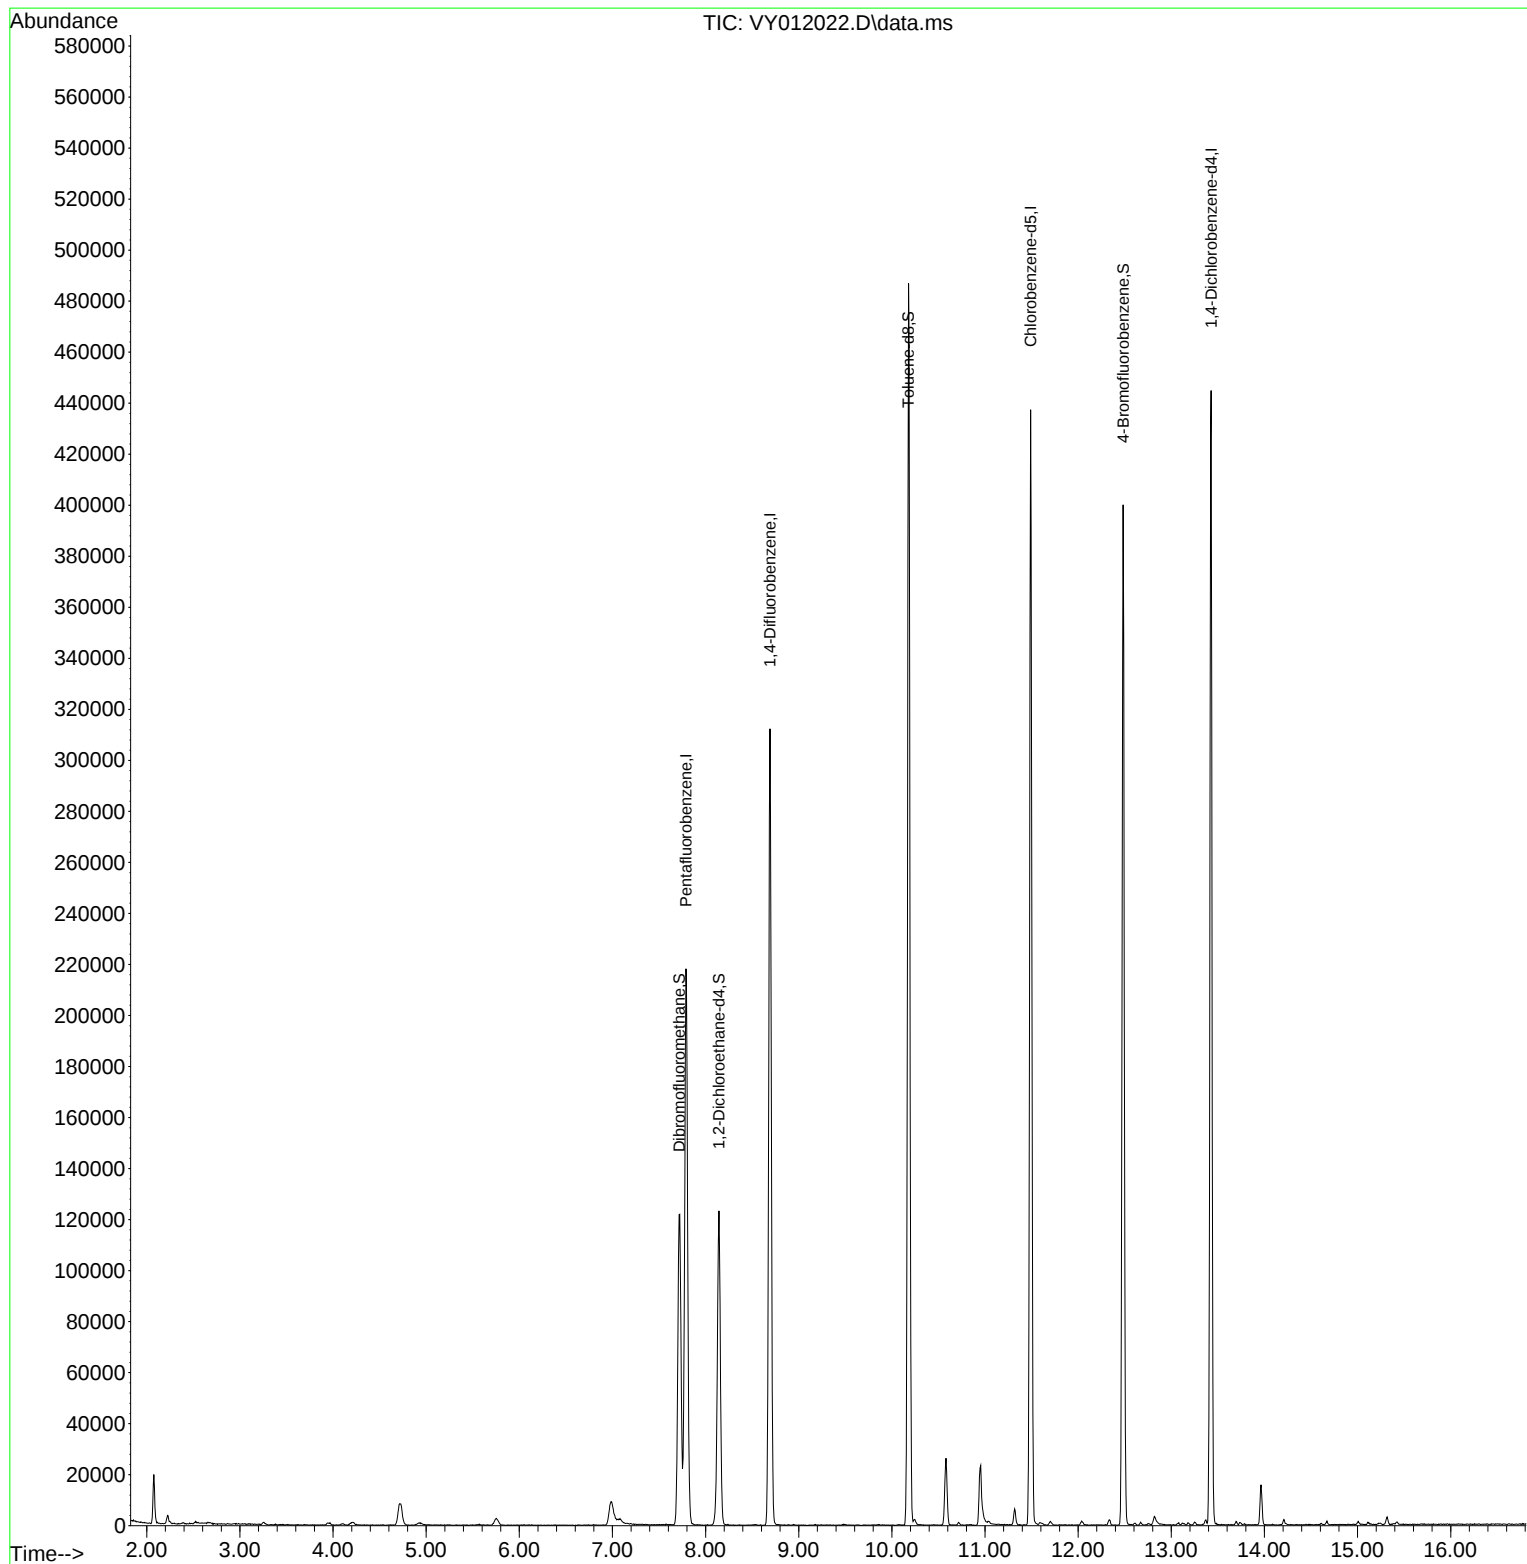


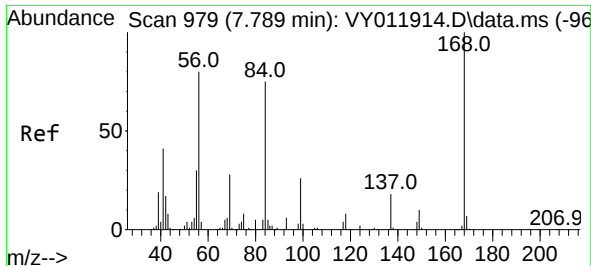

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54




Instrument :
MSVOA_Y
ClientSampleId :
VY1229SBL01


Tgt Ion:168 Resp: 167940
Ion Ratio Lower Upper
168 100
99 56.9 44.0 66.0

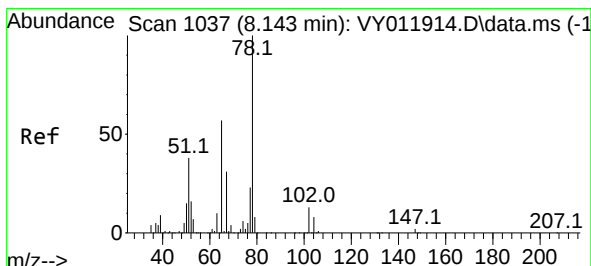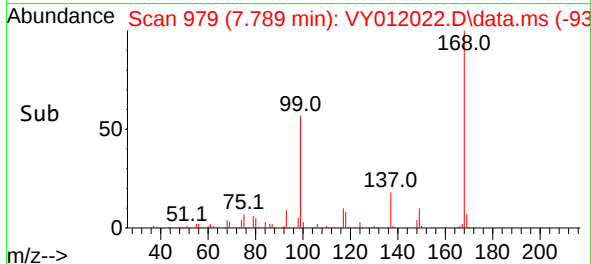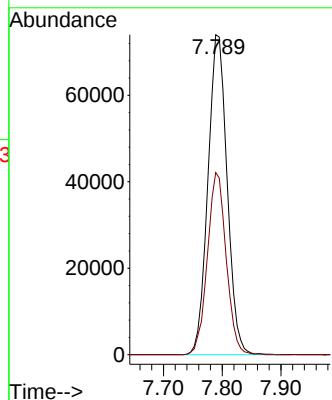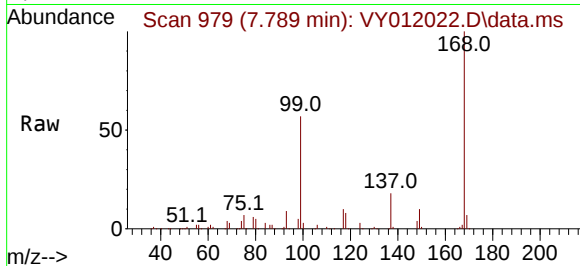

#33
1,2-Dichloroethane-d4
Concen: 57.258 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54

Tgt Ion: 65 Resp: 96879
Ion Ratio Lower Upper
65 100
67 50.0 0.0 103.2

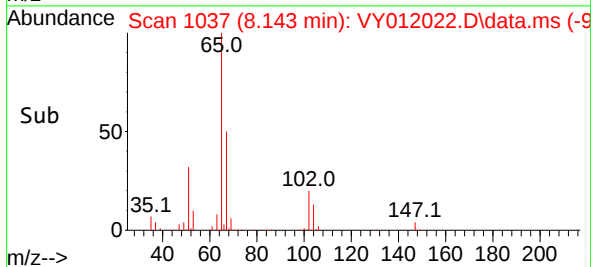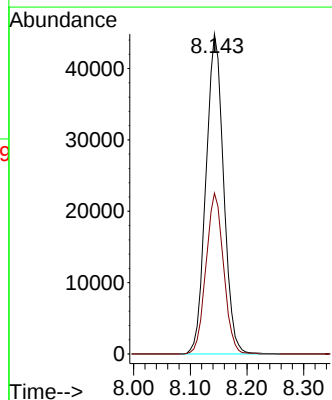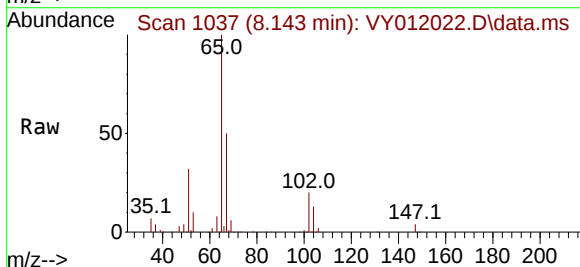

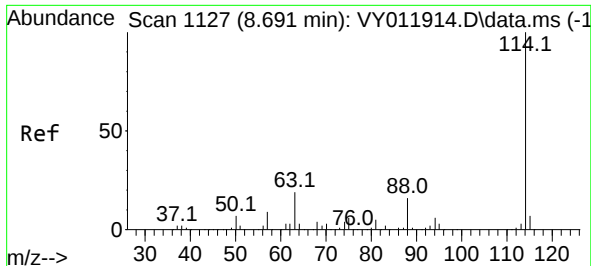

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012022.D

Acq: 29 Dec 2022 12:54

Instrument :

MSVOA_Y

ClientSampleId :

VY1229SBL01





Tgt Ion:114 Resp: 268958

Ion Ratio Lower Upper

114 100

63 18.2 0.0 39.6

88 15.5 0.0 32.2

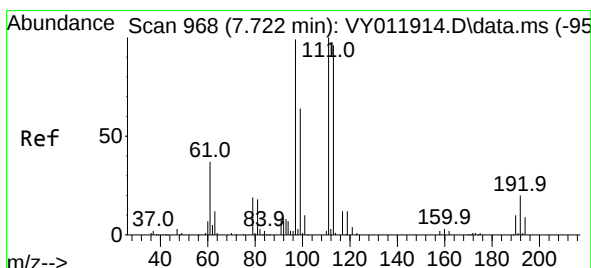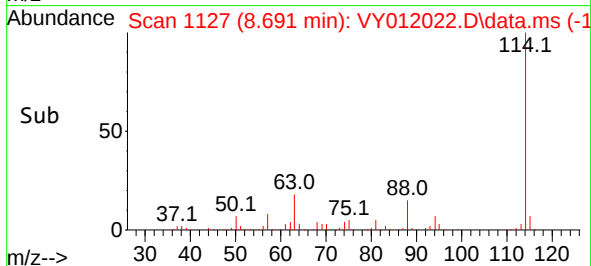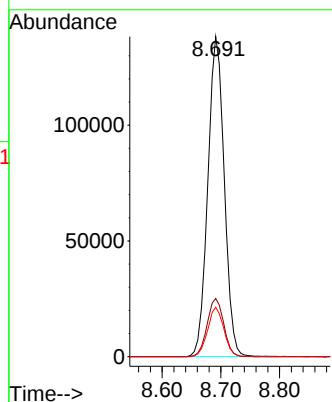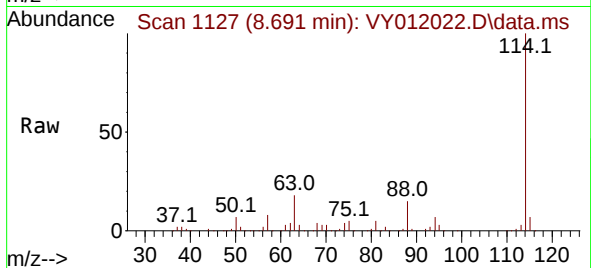

#35

Dibromofluoromethane

Concen: 53.180 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012022.D

Acq: 29 Dec 2022 12:54




Tgt Ion:113 Resp: 86110


Ion Ratio Lower Upper

113 100

111 102.7 83.0 124.4

192 21.3 16.0 24.0


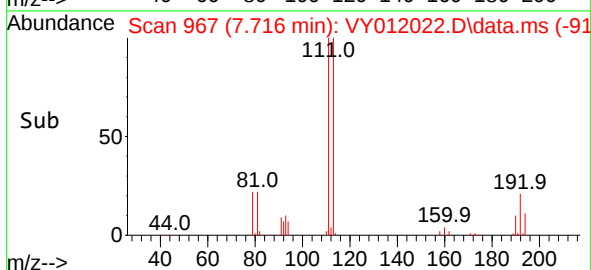
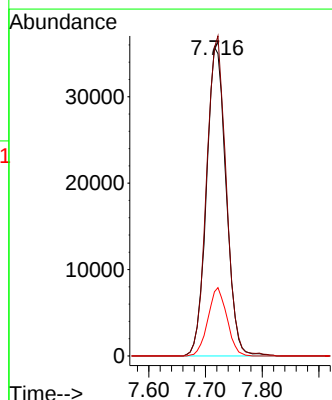
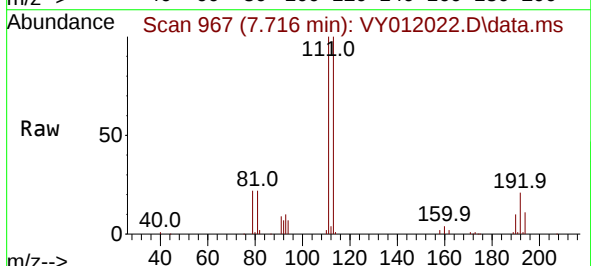


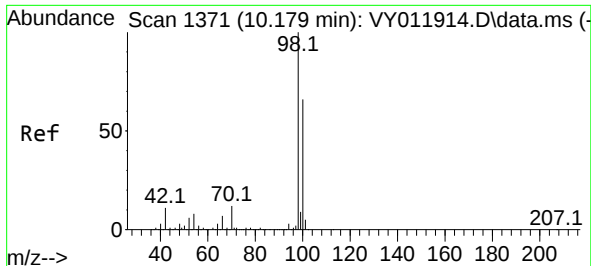

#50
Toluene-d8
Concen: 49.890 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54




Instrument :
MSVOA_Y
ClientSampleId :
VY1229SBL01


Tgt Ion: 98 Resp: 327753
Ion Ratio Lower Upper
98 100
100 64.3 51.9 77.9

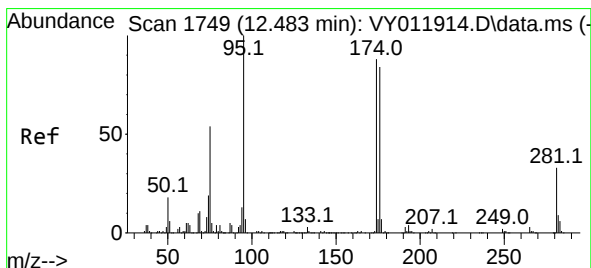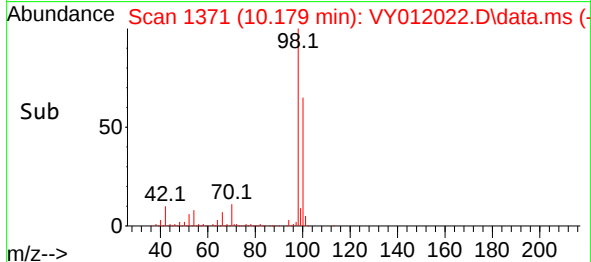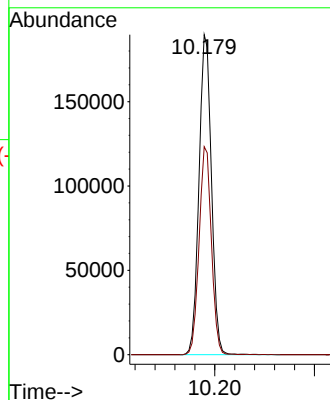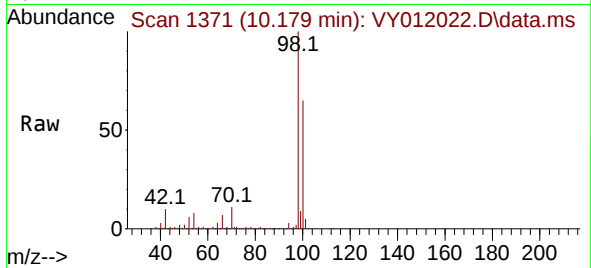

#62
4-Bromofluorobenzene
Concen: 48.849 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54

Tgt Ion: 95 Resp: 107929
Ion Ratio Lower Upper
95 100
174 92.3 0.0 172.0
176 88.4 0.0 167.6


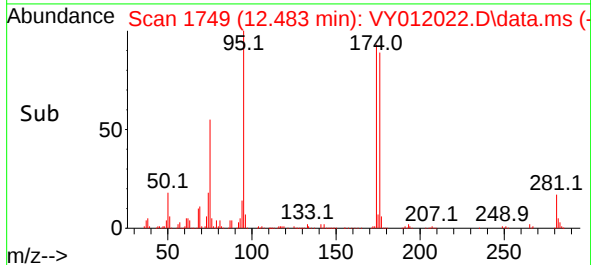
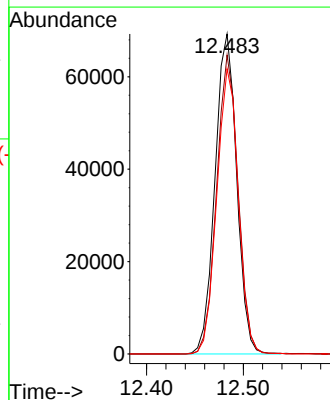
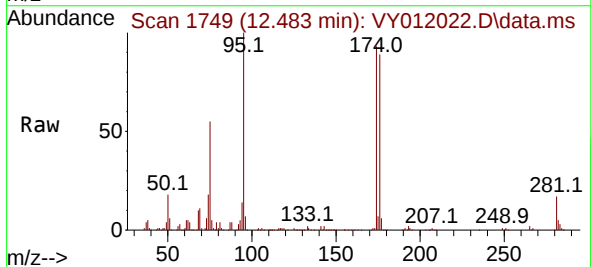


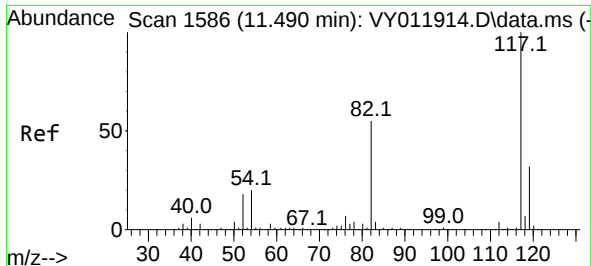

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54

Instrument :
MSVOA_Y
ClientSampleId :
VY1229SBL01

Tgt Ion:117 Resp: 244089
Ion Ratio Lower Upper
117 100
82 54.1 44.8 67.2
119 31.9 25.4 38.2

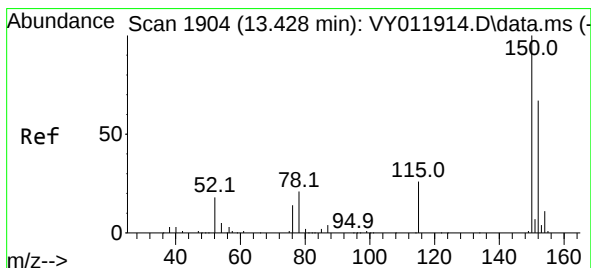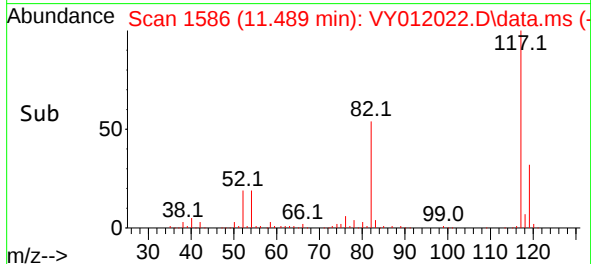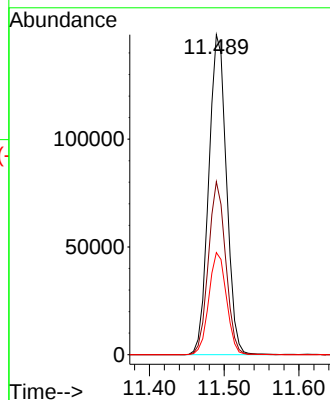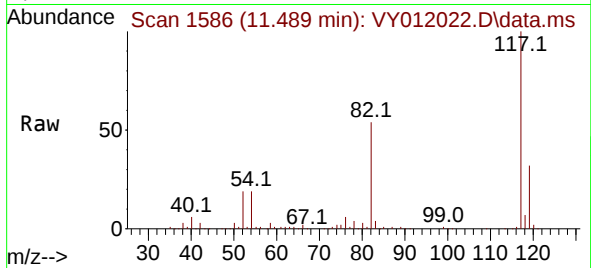

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012022.D
Acq: 29 Dec 2022 12:54

Tgt Ion:152 Resp: 118615
Ion Ratio Lower Upper
152 100
115 56.9 29.1 87.3
150 156.7 0.0 342.6

