

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122922\
 Data File : VY012025.D
 Acq On : 29 Dec 2022 14:05
 Operator : KP/MD
 Sample : N6229-01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NB-8-122822

Quant Time: Dec 30 03:58:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 20 12:37:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	11363	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	18900	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.495	117	17449	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	6751	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	7929	69.261	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	138.520%
35) Dibromofluoromethane	7.716	113	6161	54.147	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.300%
50) Toluene-d8	10.179	98	22735	49.248	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.500%
62) 4-Bromofluorobenzene	12.483	95	6321	40.712	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	81.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY122922\
Data File : VY012025.D
Acq On : 29 Dec 2022 14:05
Operator : KP/MD
Sample : N6229-01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NB-8-122822

Quant Time: Dec 30 03:58:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y122022S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 20 12:37:37 2022
Response via : Initial Calibration




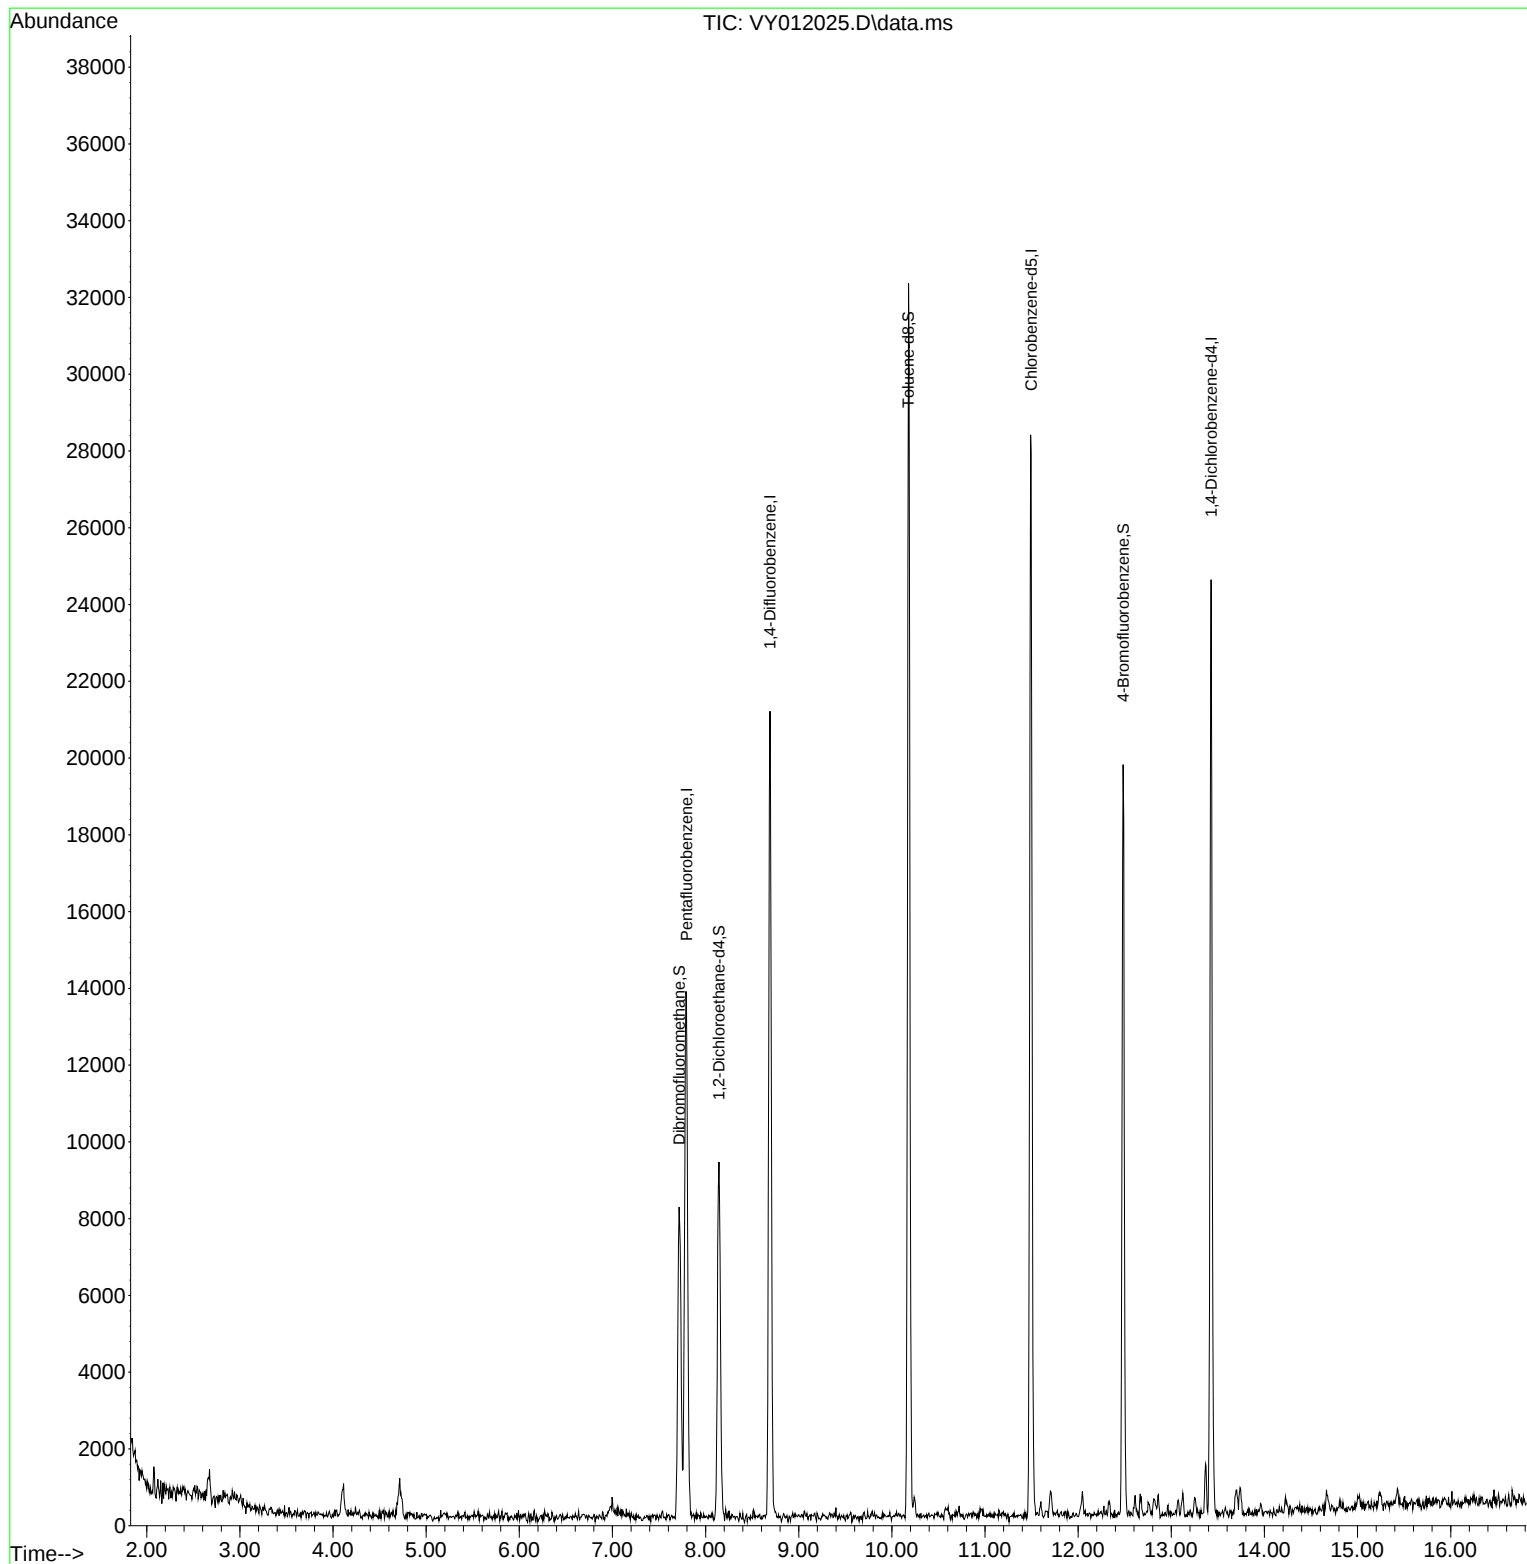


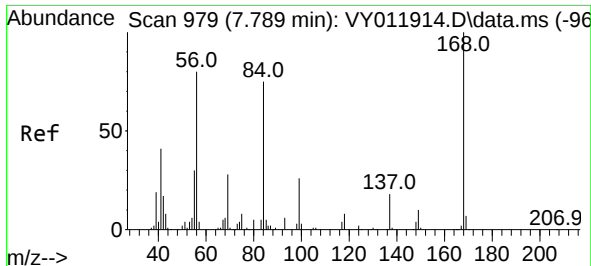

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05




Instrument :
MSVOA_Y
ClientSampleId :
NB-8-122822


Tgt Ion:168 Resp: 11363
Ion Ratio Lower Upper
168 100
99 54.1 44.0 66.0

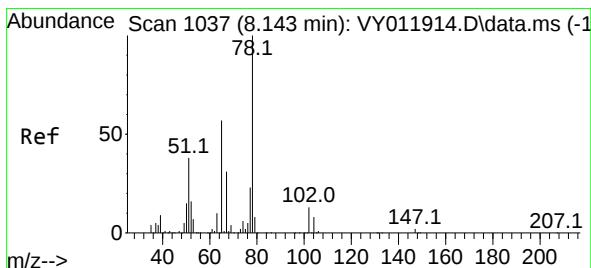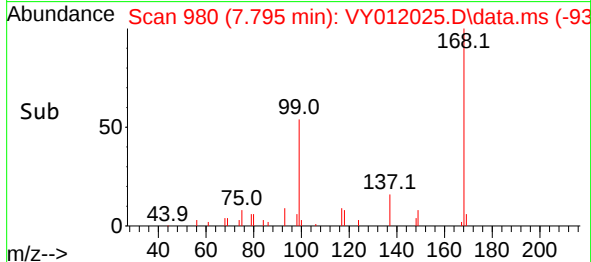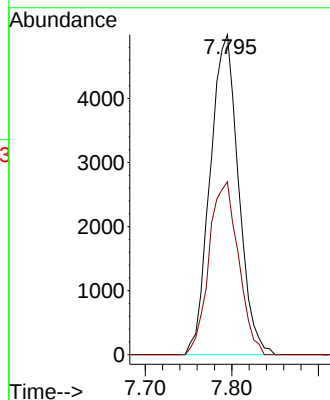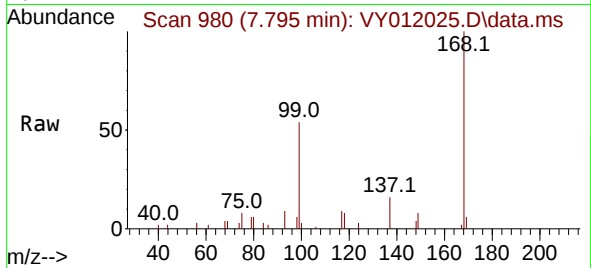

#33
1,2-Dichloroethane-d4
Concen: 69.261 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. -0.001 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05

Tgt Ion: 65 Resp: 7929
Ion Ratio Lower Upper
65 100
67 47.0 0.0 103.2

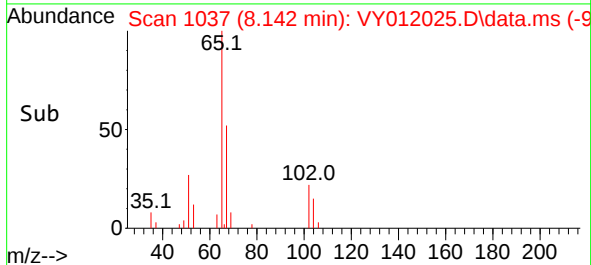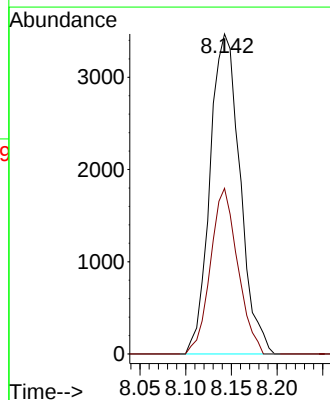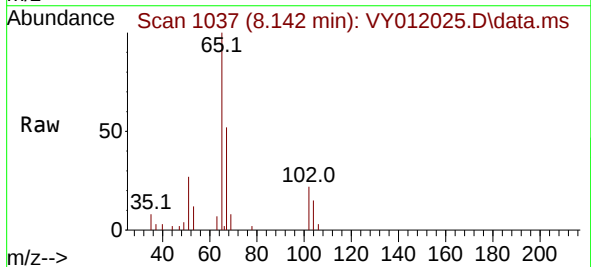

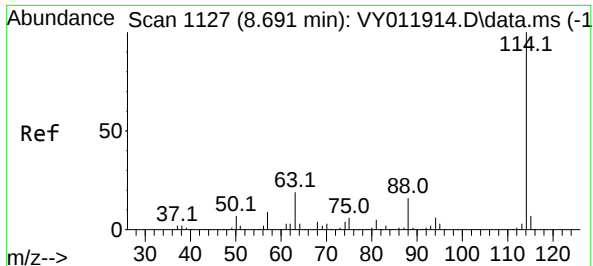

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VY012025.D

Acq: 29 Dec 2022 14:05

Instrument :

MSVOA_Y

ClientSampleId :

NB-8-122822





Tgt Ion:114 Resp: 18900

Ion Ratio Lower Upper

114 100

63 16.8 0.0 39.6

88 14.0 0.0 32.2

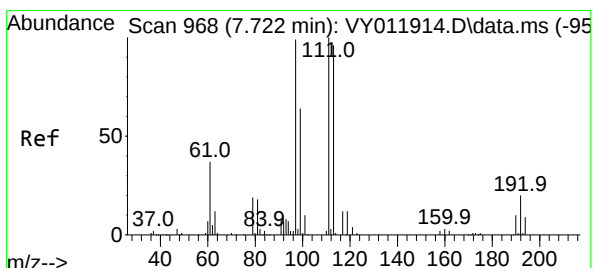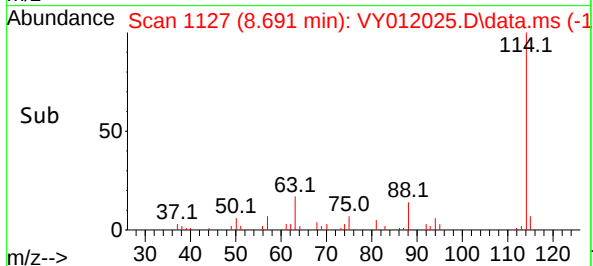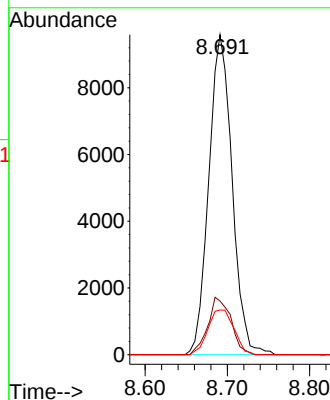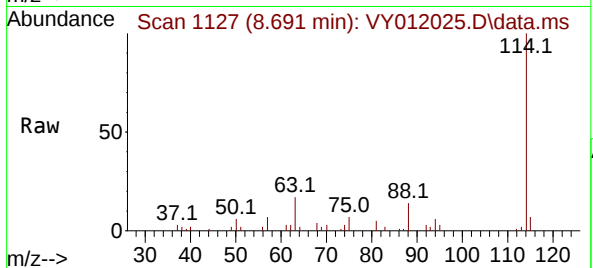

#35

Dibromofluoromethane

Concen: 54.147 ug/l

RT: 7.716 min Scan# 967

Delta R.T. -0.000 min

Lab File: VY012025.D

Acq: 29 Dec 2022 14:05




Tgt Ion:113 Resp: 6161


Ion Ratio Lower Upper

113 100

111 97.2 83.0 124.4

192 20.5 16.0 24.0


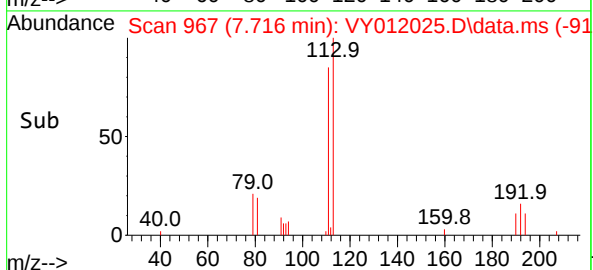
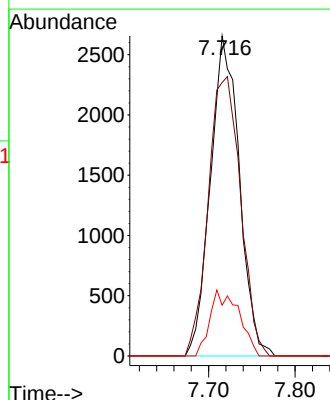
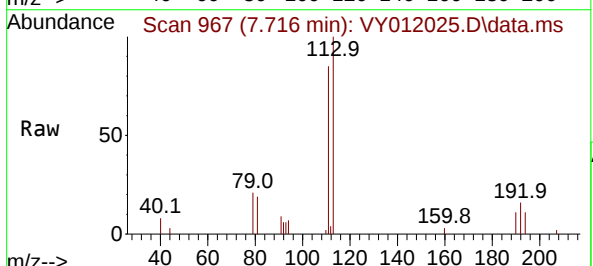


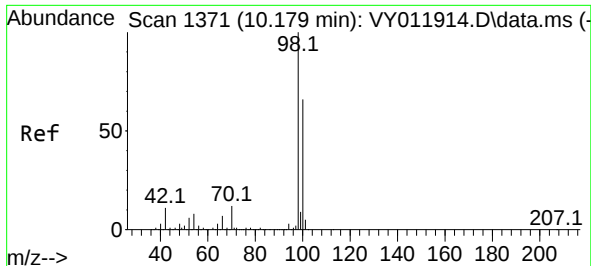

#50
Toluene-d8
Concen: 49.248 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05




Instrument :
MSVOA_Y
ClientSampleId :
NB-8-122822


Tgt Ion: 98 Resp: 22735
Ion Ratio Lower Upper
98 100
100 62.9 51.9 77.9

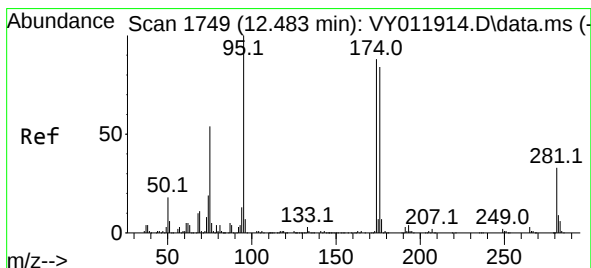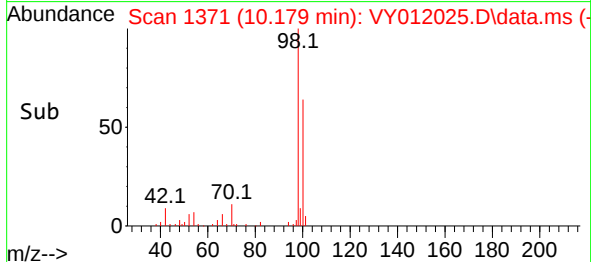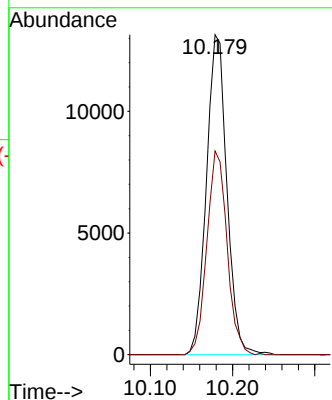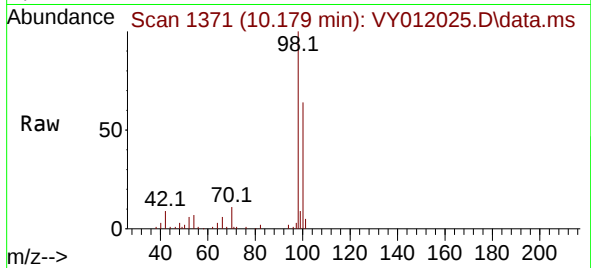

#62
4-Bromofluorobenzene
Concen: 40.712 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05

Tgt Ion: 95 Resp: 6321
Ion Ratio Lower Upper
95 100
174 92.5 0.0 172.0
176 86.8 0.0 167.6


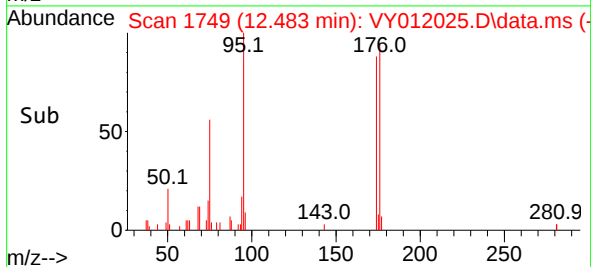
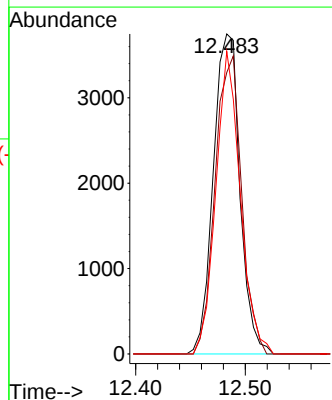
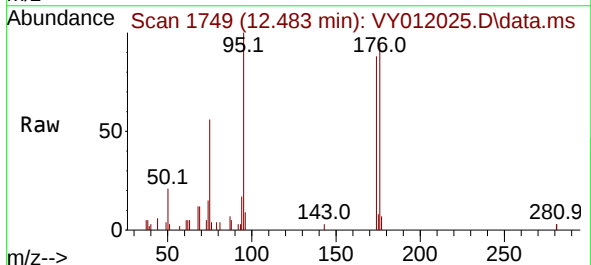


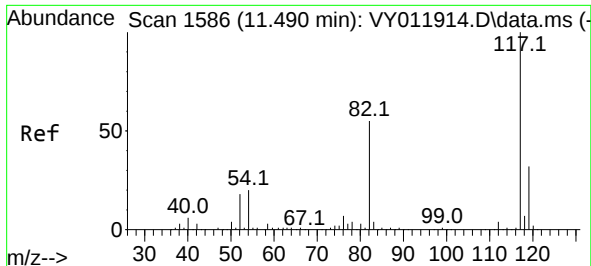

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.495 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05

Instrument :
MSVOA_Y
ClientSampleId :
NB-8-122822

Tgt Ion:117 Resp: 17449
Ion Ratio Lower Upper
117 100
82 51.8 44.8 67.2
119 31.8 25.4 38.2

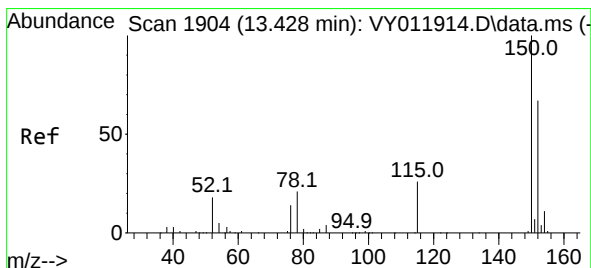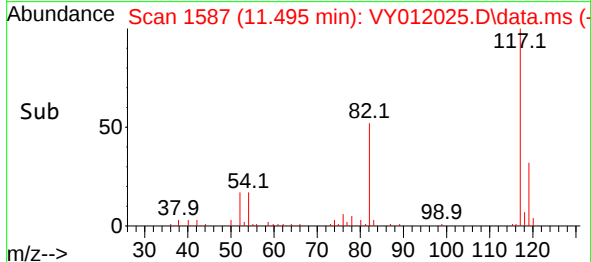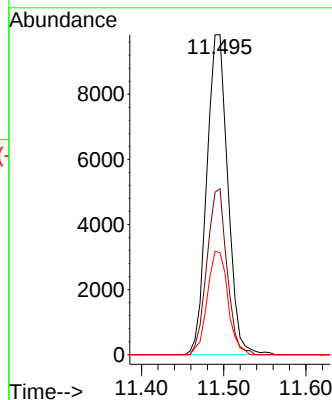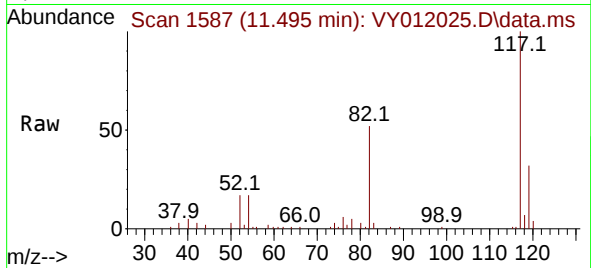

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY012025.D
Acq: 29 Dec 2022 14:05

Tgt Ion:152 Resp: 6751
Ion Ratio Lower Upper
152 100
115 60.0 29.1 87.3
150 159.9 0.0 342.6

