

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD010220\
 Data File : VD064717.D
 Acq On : 02 Jan 2020 15:03
 Operator : VA/SY
 Sample : K6465-01
 Misc : 7.81G/5.00ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 GP-11-(1-3)

Quant Time: Jan 03 01:18:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 24 13:19:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	517669	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	802033	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	701181	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	324241	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	233896	51.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.48%	
35) Dibromofluoromethane	7.92	113	245594	49.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.82%	
50) Toluene-d8	10.34	98	955560	50.71	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.42%	
62) 4-Bromofluorobenzene	12.64	95	288982	48.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.98%	
Target Compounds						
30) Chloroform	7.71	83	10957	1.228	ug/l	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD010220\
Data File : VD064717.D
Acq On : 02 Jan 2020 15:03
Operator : VA/SY
Sample : K6465-01
Misc : 7.81G/5.00ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
GP-11-(1-3)

Quant Time: Jan 03 01:18:19 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 24 13:19:06 2019
Response via : Initial Calibration

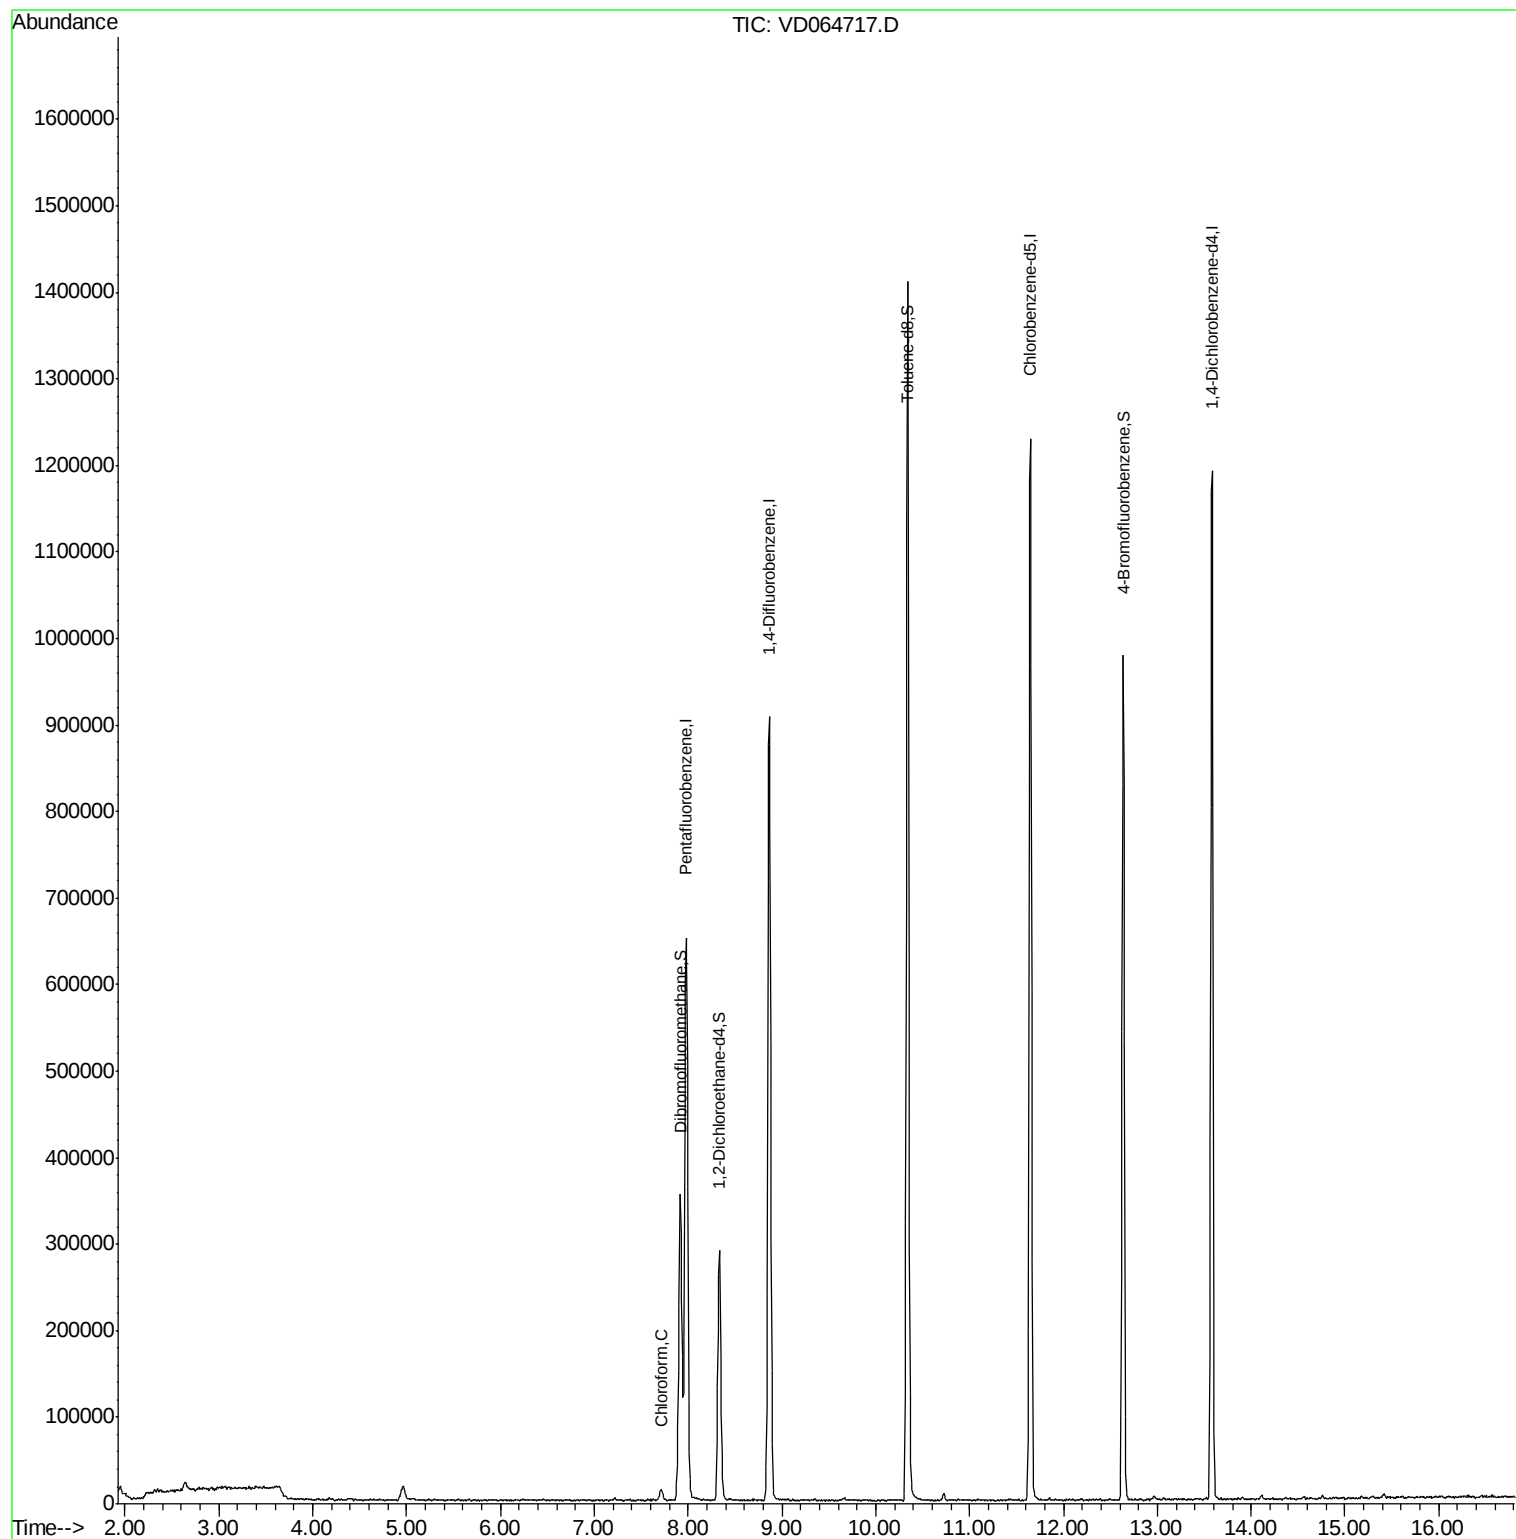

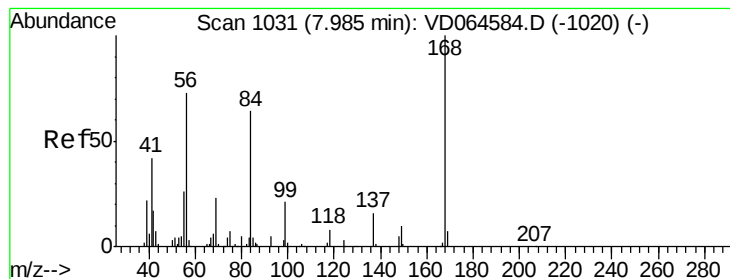

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD064717.D

Acq: 02 Jan 2020 15:03

Instrument :

MSVOA_D

ClientSampleId :


GP-11-(1-3)

Tot Ion:168 Resp: 517669

Ion Ratio Lower Upper

168 100

99 51.9 41.8 62.6

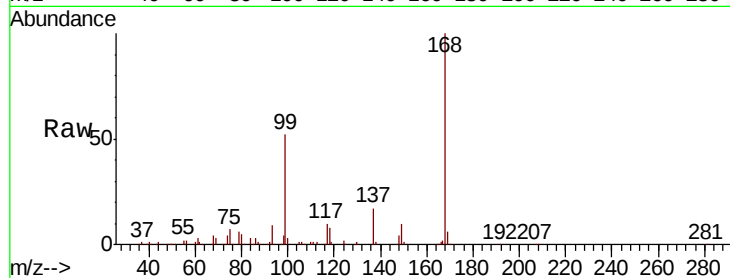

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

250000

200000



150000

100000

50000

0

Time-->

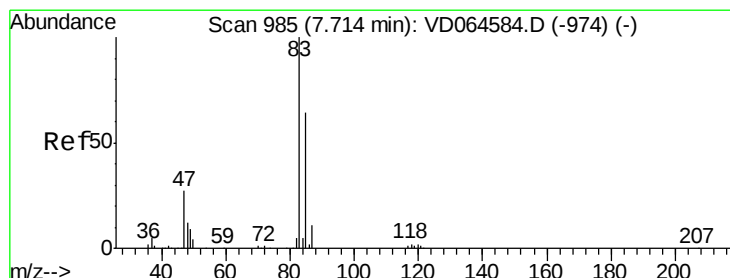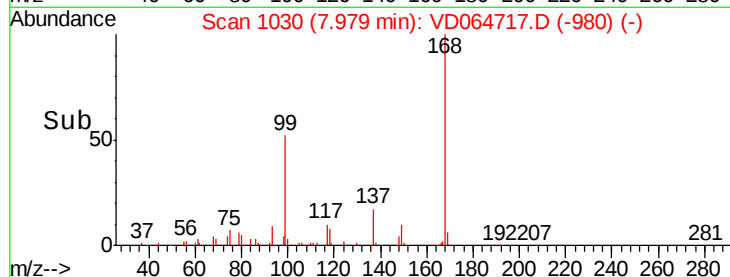

#30

Chloroform

Concen: 1.228 ug/l

RT: 7.71 min Scan# 984

Delta R.T. -0.01 min

Lab File: VD064717.D


Acq: 02 Jan 2020 15:03

Tgt Ion: 83 Resp: 10957

Ion Ratio Lower Upper

83 100

85 55.4 51.1 76.7

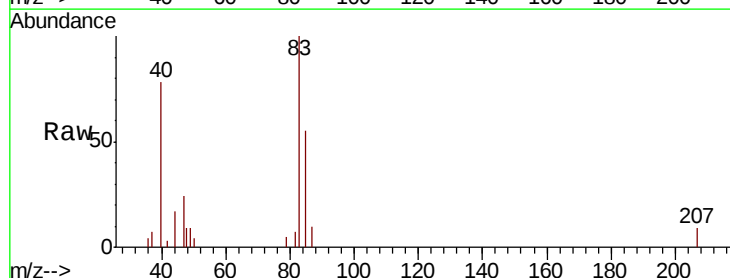

Abundance Ion 82.90 (82.60 to 83.60): VDC

Ion 84.90 (84.60 to 85.60): VDC

7.71

5000

4000


3000


2000

1000

0

Time-->




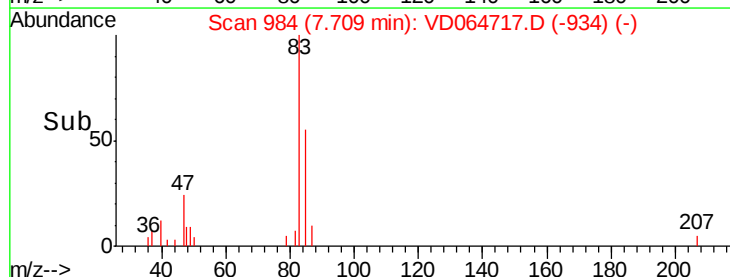


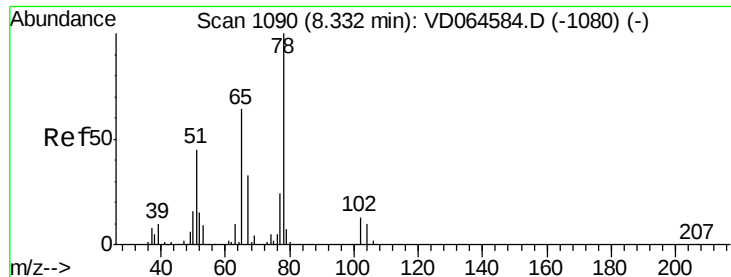

#33
 1,2-Dichloroethane-d4
 Concen: 51.240 ug/l
 RT: 8.33 min Scan# 1090
 Delta R.T. 0.00 min
 Lab File: VD064717.D
 Acq: 02 Jan 2020 15:03




Instrument :
 MSVOA_D
 ClientSampleId :
 GP-11-(1-3)


Tot Ion: 65 Resp: 233896
 Ion Ratio Lower Upper
 65 100
 67 51.9 0.0 106.2

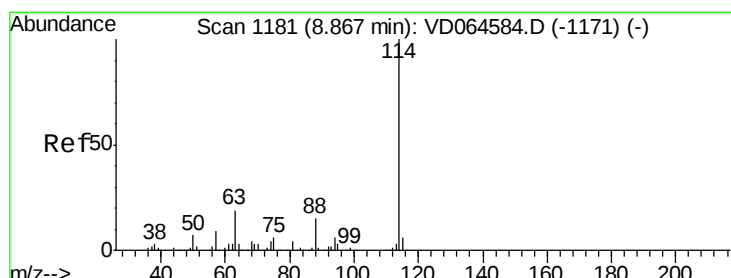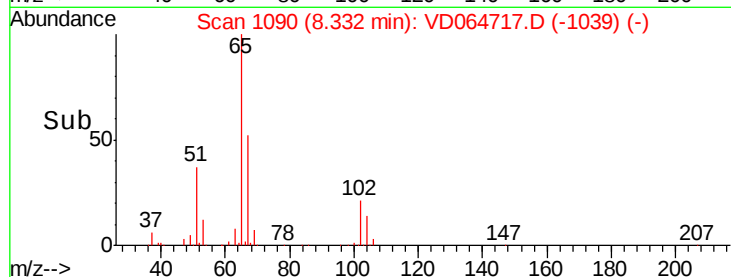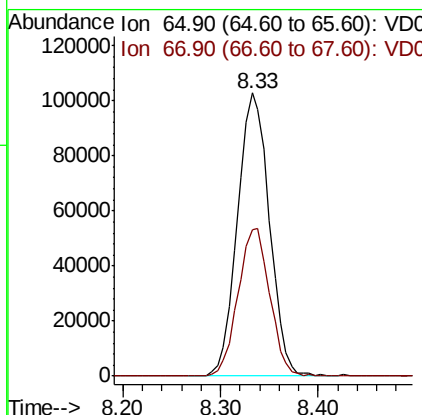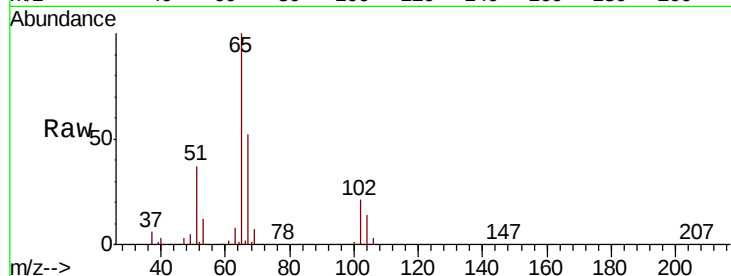

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD064717.D
 Acq: 02 Jan 2020 15:03

Tgt Ion: 114 Resp: 802033
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 38.0
 88 13.7 0.0 29.2

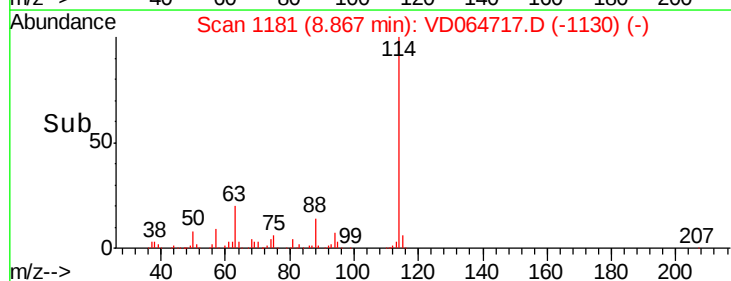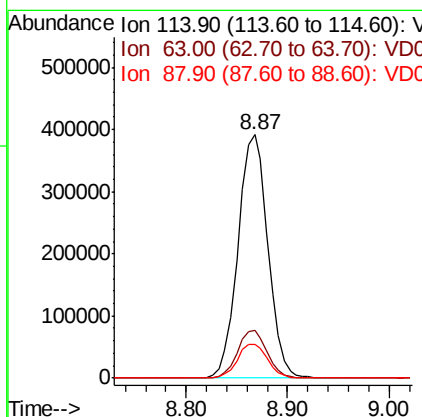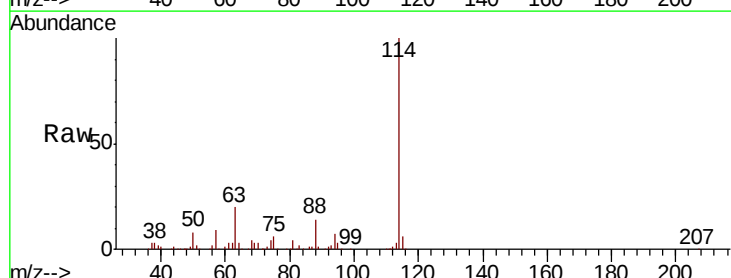


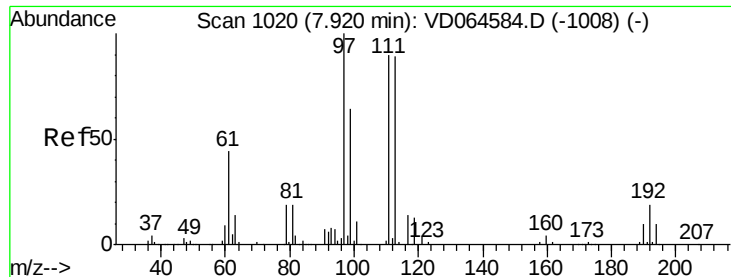

#35
 Dibromofluoromethane
 Concen: 49.911 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD064717.D
 Acq: 02 Jan 2020 15:03

Instrument :
 MSVOA_D
 ClientSampleId :
 GP-11-(1-3)

Tot Ion	Ratio	Lower	Upper
113	100		
111	103.3	80.6	121.0
192	22.3	17.9	26.9



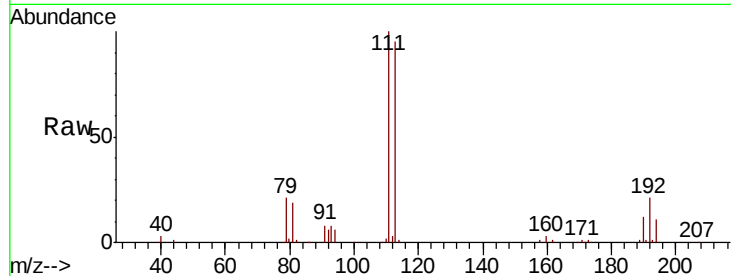


Abundance

Ion 112.80 (112.50 to 113.50): V


Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

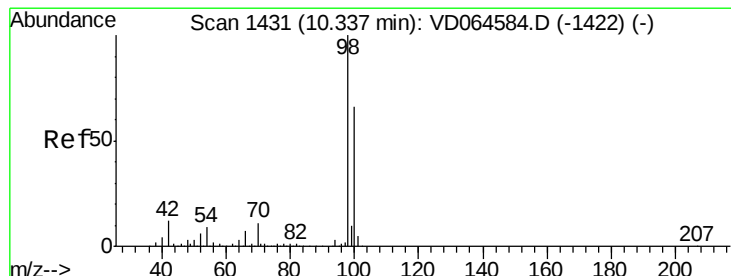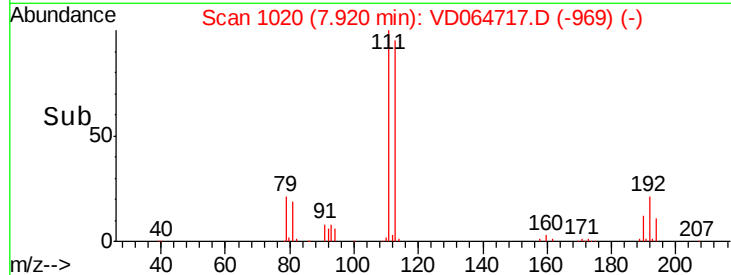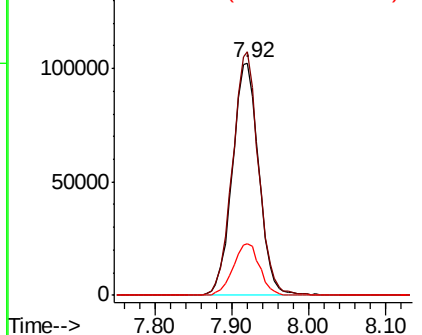

#50
 Toluene-d8
 Concen: 50.705 ug/l
 RT: 10.34 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: VD064717.D
 Acq: 02 Jan 2020 15:03



Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.1	51.7	77.5

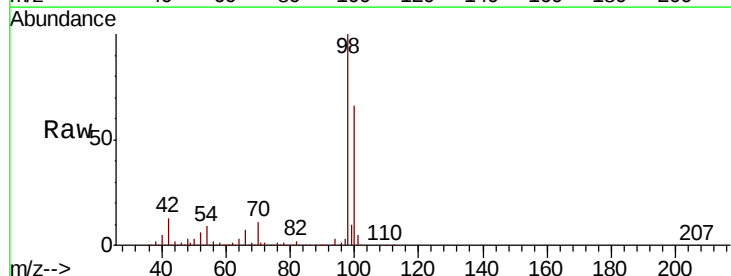


Abundance

Ion 98.00 (97.70 to 98.70): V

Ion 100.00 (99.70 to 100.70): V



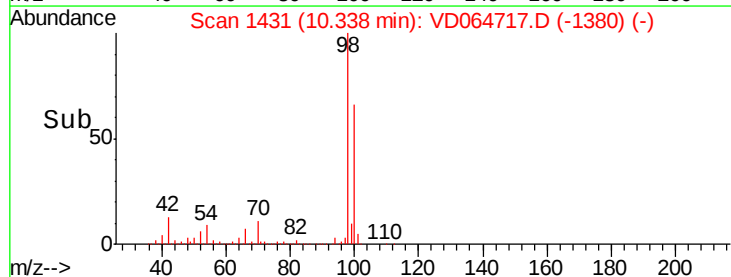
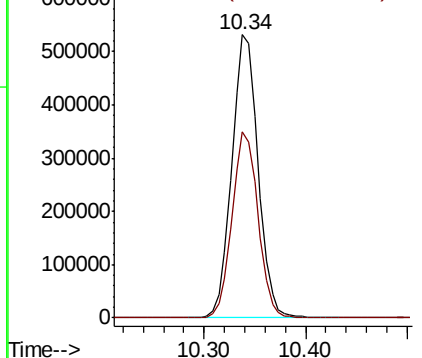


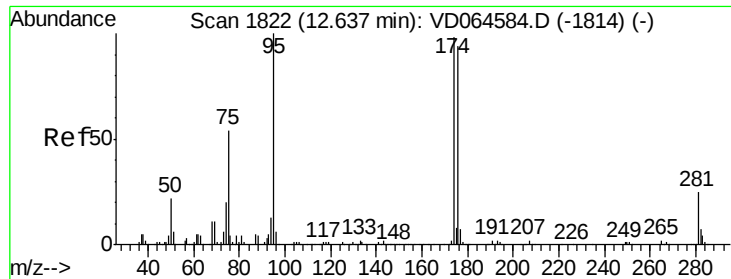

#62
4-Bromofluorobenzene
Concen: 48.494 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD064717.D
Acq: 02 Jan 2020 15:03




Instrument :
MSVOA_D
ClientSampleId :
GP-11-(1-3)


Tot Ion: 95 Resp: 288982
Ion Ratio Lower Upper
95 100
174 93.7 0.0 193.2
176 91.7 0.0 184.2

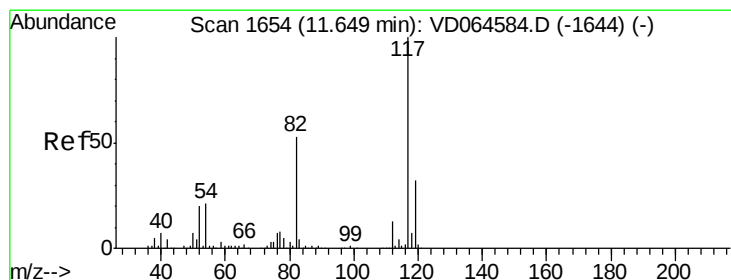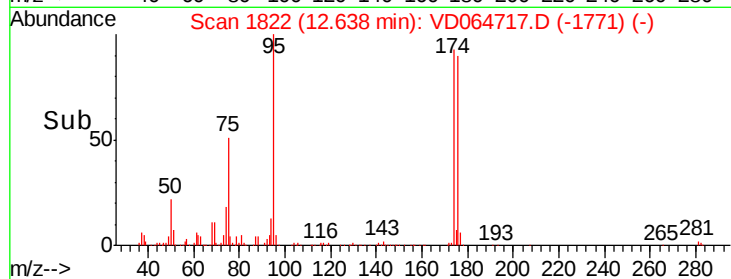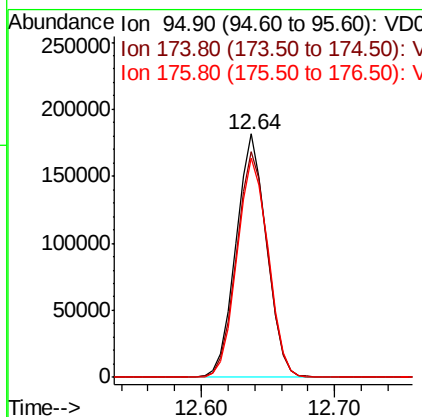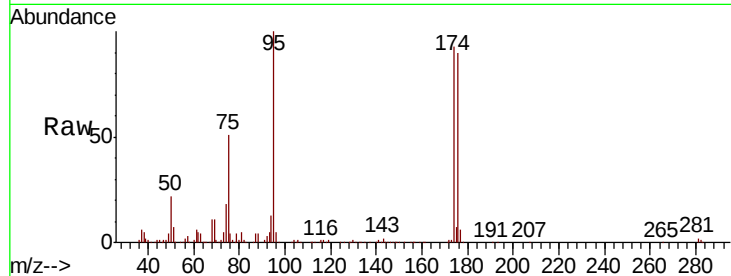

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD064717.D
Acq: 02 Jan 2020 15:03

Tgt Ion: 117 Resp: 701181
Ion Ratio Lower Upper
117 100
82 52.7 42.2 63.4
119 31.2 26.0 39.0

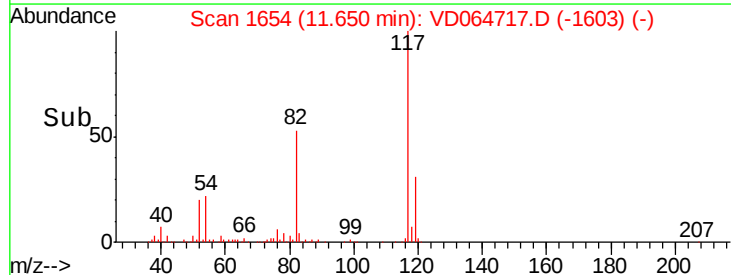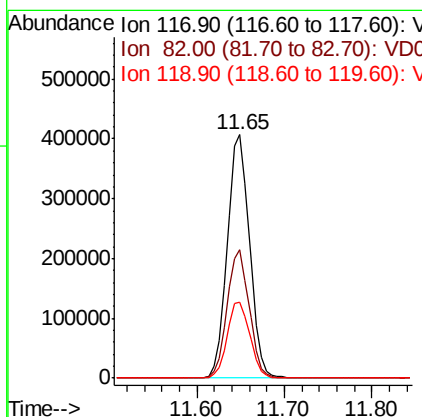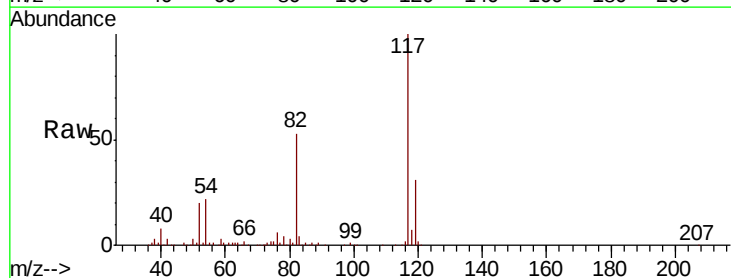

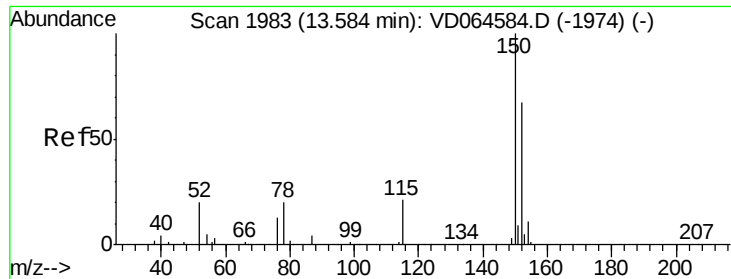

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.00 min

Lab File: VD064717.D

Acq: 02 Jan 2020 15:03

Instrument :

MSVOA_D

ClientSampleId :

GP-11-(1-3)


Tot Ion:152 Resp: 324241

Ion Ratio Lower Upper

152 100

115 54.4 27.8 83.4

150 154.7 0.0 351.4

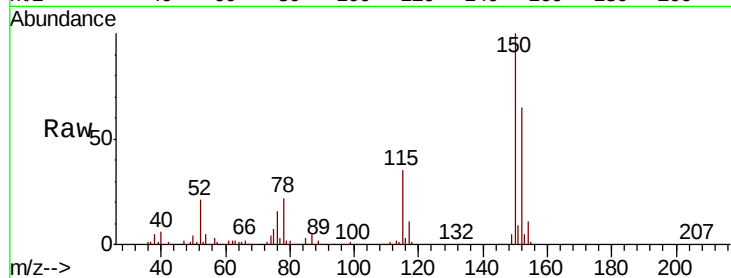

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

