


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD010220\
 Data File : VD064707.D
 Acq On : 02 Jan 2020 09:50
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Title : SW846 8260
 Last Update : Tue Dec 24 13:19:06 2019

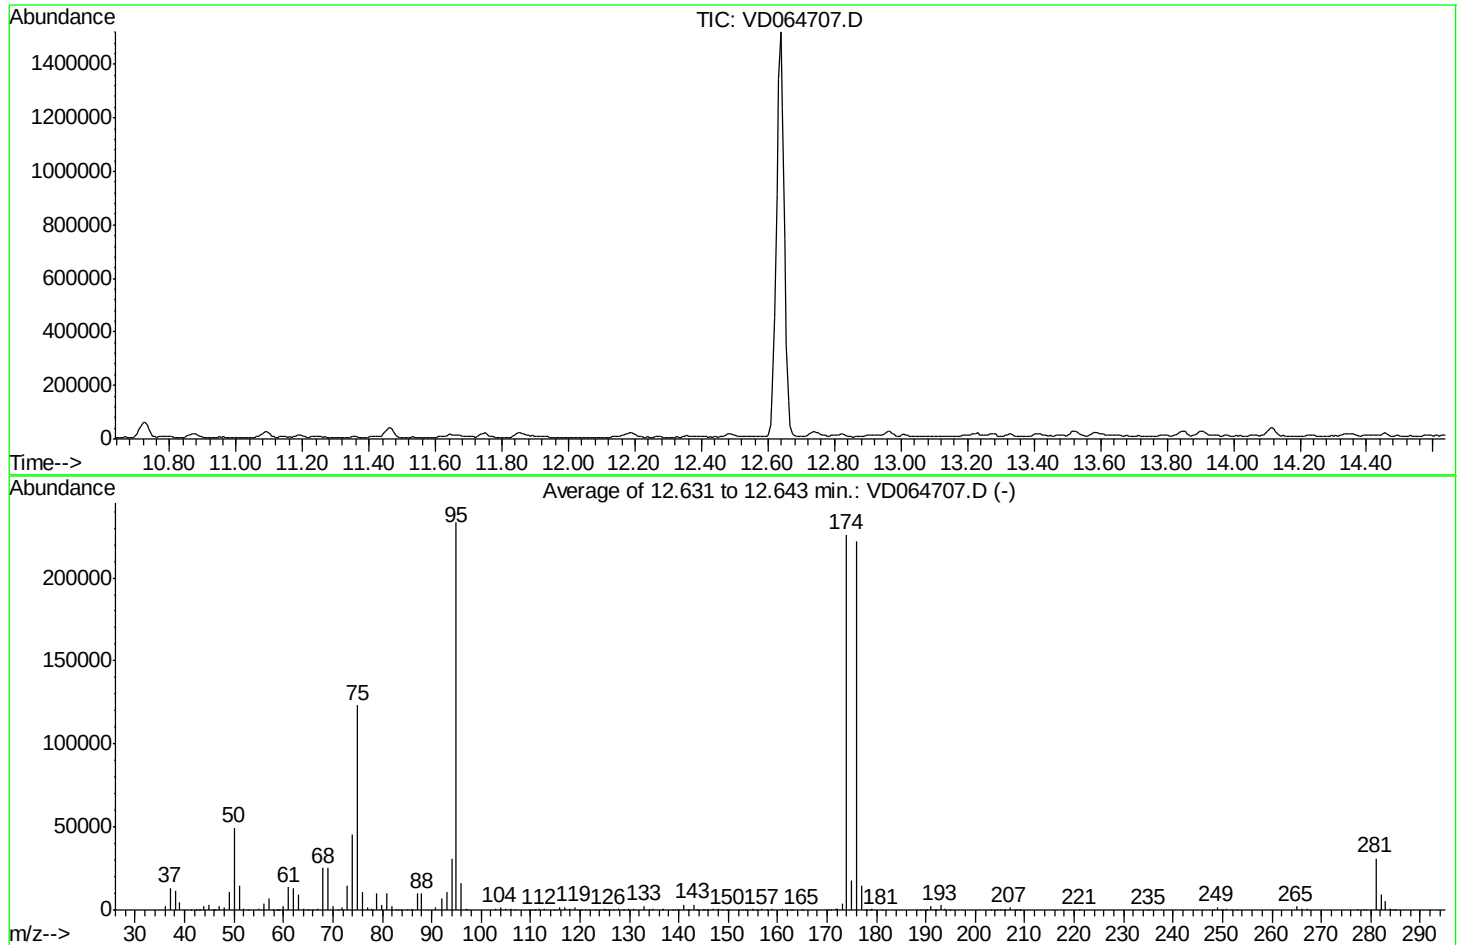

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	49461	PASS
75	95	30	60	52.7	123077	PASS
95	95	100	100	100.0	233429	PASS
96	95	5	9	6.9	16125	PASS
173	174	0.00	2	1.6	3529	PASS
174	95	50	100	96.8	225877	PASS
175	174	5	9	7.9	17914	PASS
176	174	95	101	98.3	222144	PASS
177	176	5	9	6.7	14924	PASS