

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010224\
 Data File : VD078121.D
 Acq On : 02 Jan 2024 14:23
 Operator : RP/MD
 Sample : 06045-01
 Misc : 5.66G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MR-300-0-2

Quant Time: Jan 03 00:06:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122623S.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 27 03:40:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	208985	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	355654	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	313728	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	108675	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	81046	43.585	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	87.180%
35) Dibromofluoromethane	7.811	113	108506	47.416	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.840%
50) Toluene-d8	10.269	98	424103	52.670	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	105.340%
62) 4-Bromofluorobenzene	12.575	95	107910	41.651	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	83.300%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010224\
Data File : VD078121.D
Acq On : 02 Jan 2024 14:23
Operator : RP/MD
Sample : 06045-01
Misc : 5.66G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MR-300-0-2

Quant Time: Jan 03 00:06:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122623S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 27 03:40:16 2023
Response via : Initial Calibration




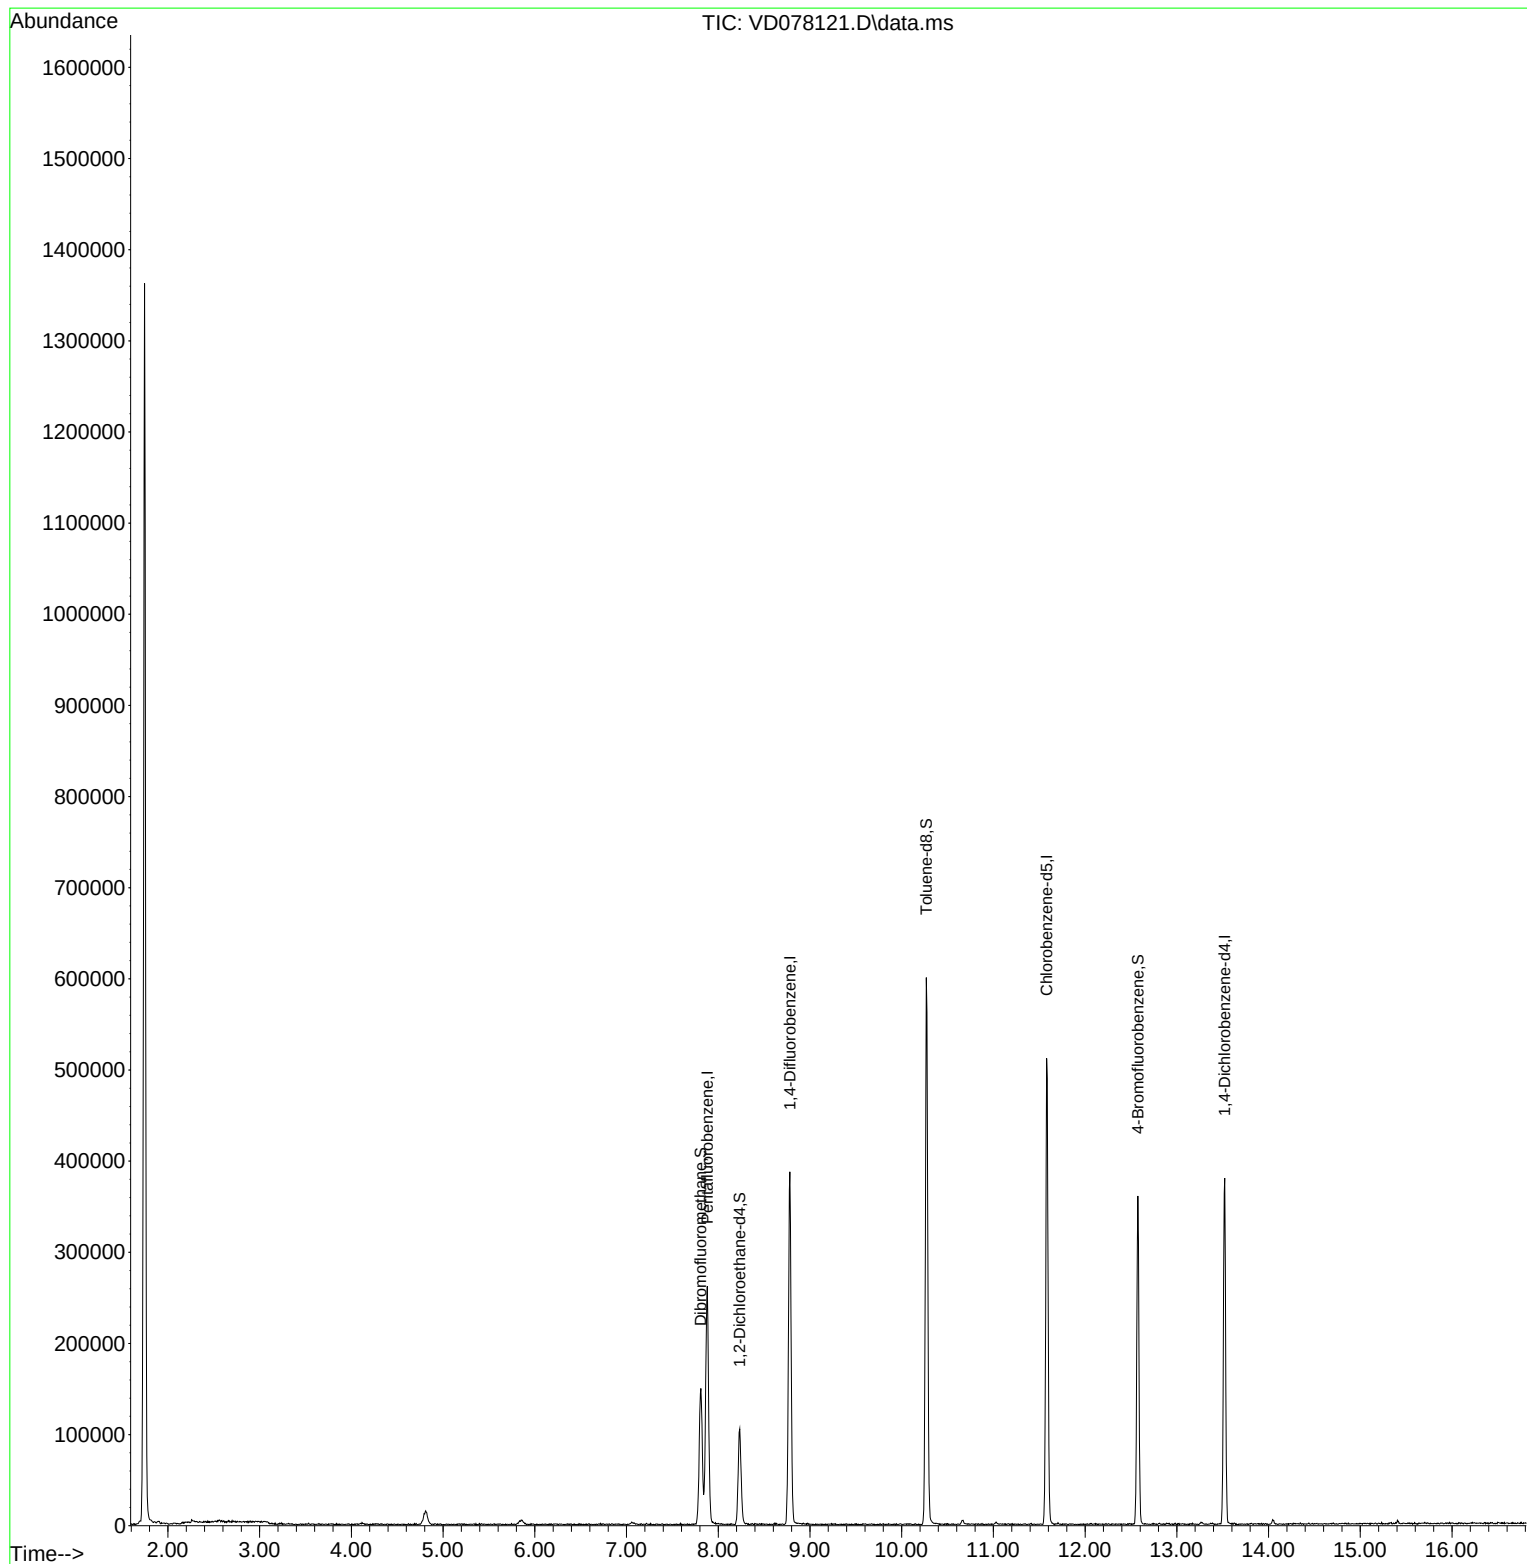


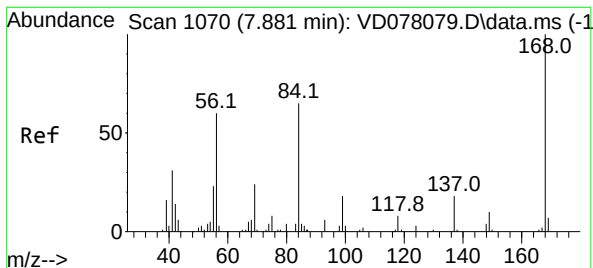

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1070
Delta R.T. 0.000 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23




Instrument :
MSVOA_D
ClientSampleId :
MR-300-0-2


Tgt Ion:168 Resp: 208985
Ion Ratio Lower Upper
168 100
99 48.1 36.7 55.1

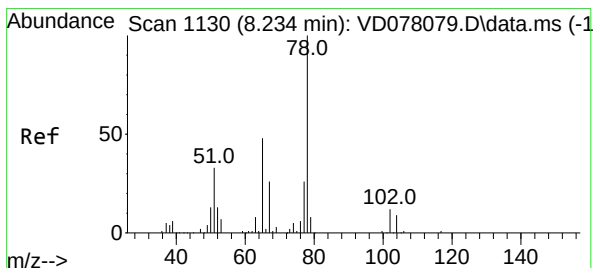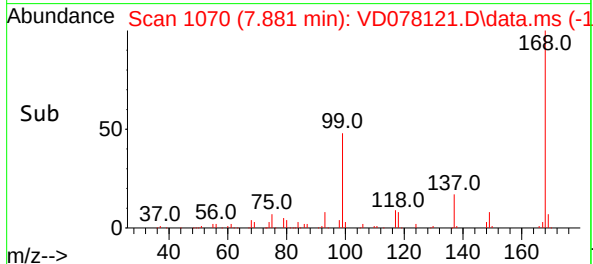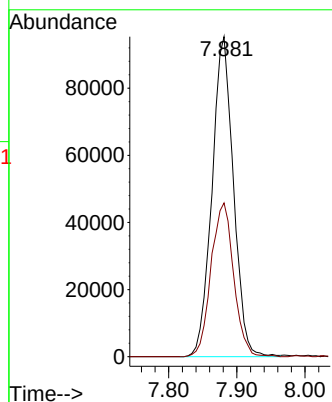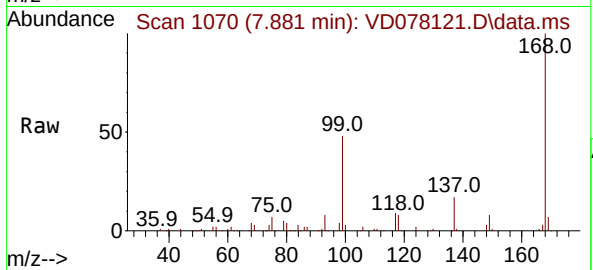

#33
1,2-Dichloroethane-d4
Concen: 43.585 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.000 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23

Tgt Ion: 65 Resp: 81046
Ion Ratio Lower Upper
65 100
67 54.4 0.0 115.0

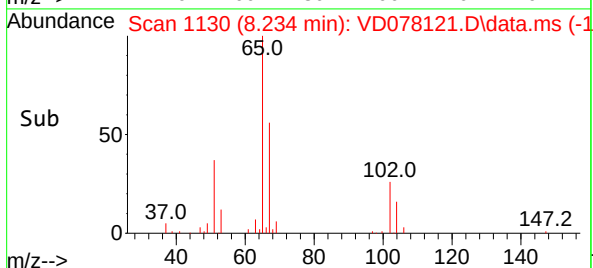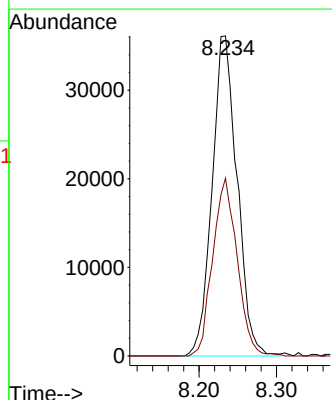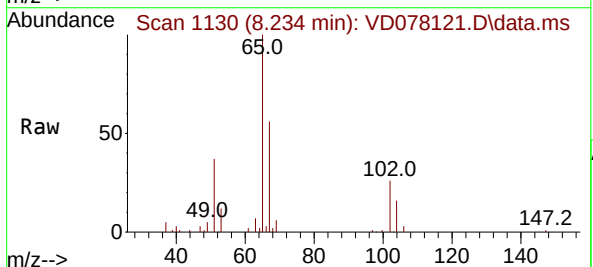

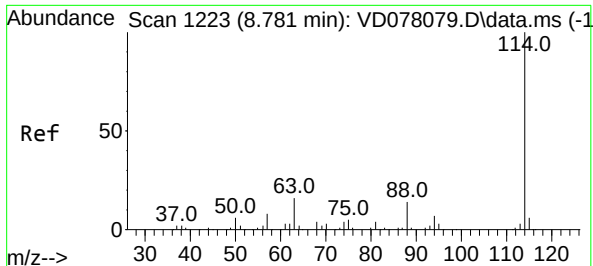

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.000 min

Lab File: VD078121.D

Acq: 02 Jan 2024 14:23

Instrument :

MSVOA_D

ClientSampleId :

MR-300-0-2





Tgt Ion:114 Resp: 355654

Ion Ratio Lower Upper

114 100

63 17.1 0.0 33.4

88 13.7 0.0 26.2

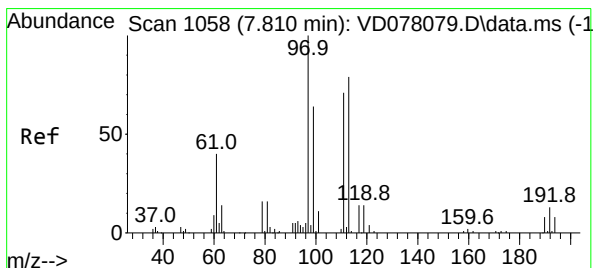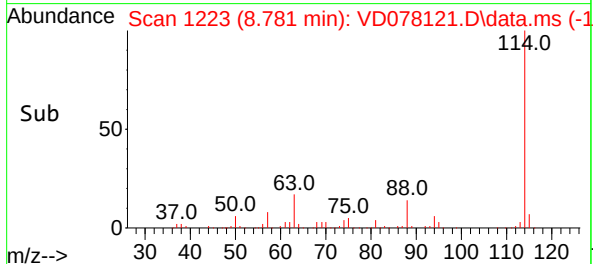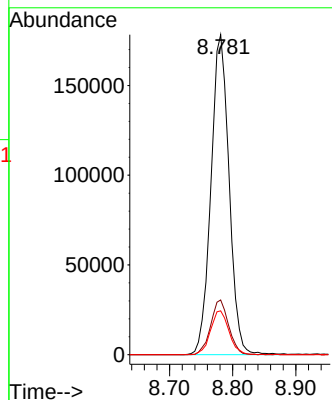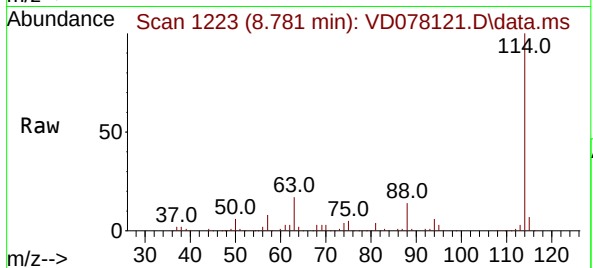

#35

Dibromofluoromethane

Concen: 47.416 ug/l

RT: 7.811 min Scan# 1058

Delta R.T. 0.000 min

Lab File: VD078121.D

Acq: 02 Jan 2024 14:23




Tgt Ion:113 Resp: 108506


Ion Ratio Lower Upper

113 100

111 102.0 84.7 127.1

192 20.9 16.8 25.2


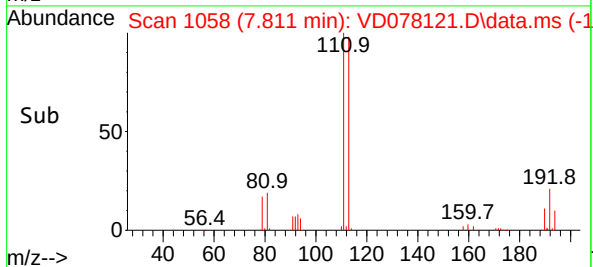
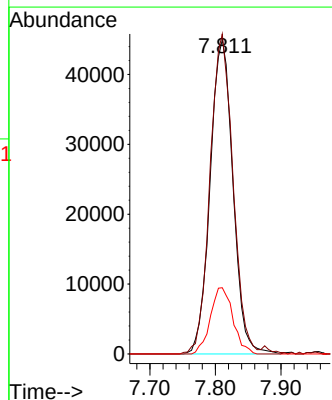
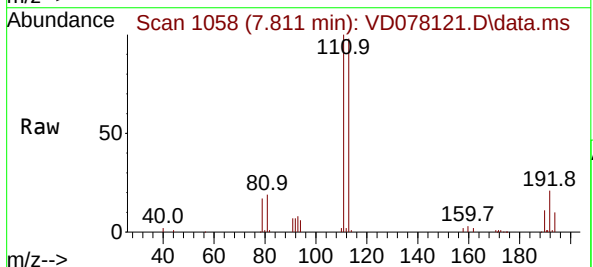


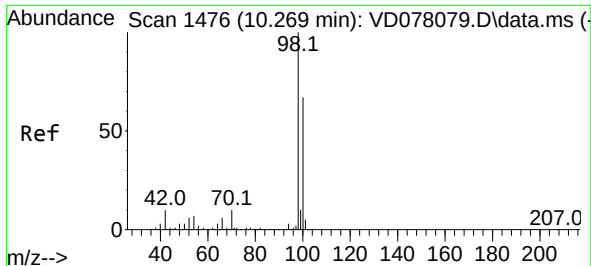

#50
Toluene-d8
Concen: 52.670 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23




Instrument :
MSVOA_D
ClientSampleId :
MR-300-0-2


Tgt Ion: 98 Resp: 424103
Ion Ratio Lower Upper
98 100
100 63.9 50.3 75.5

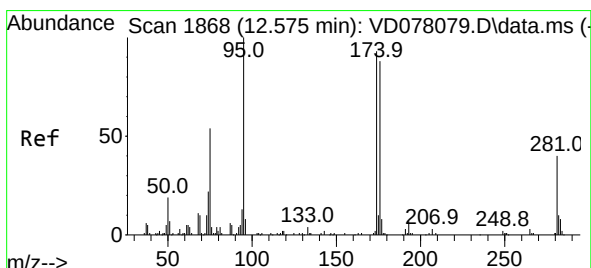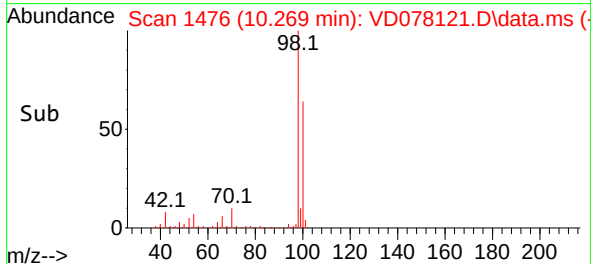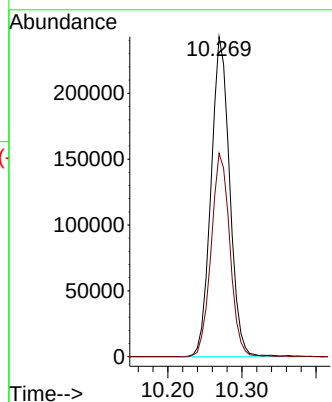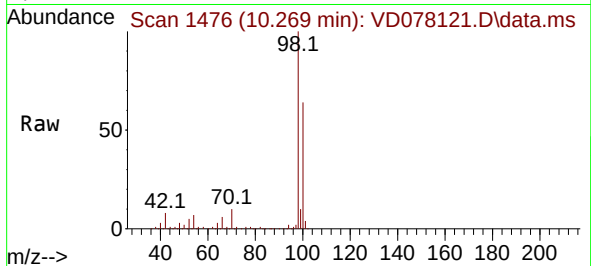

#62
4-Bromofluorobenzene
Concen: 41.651 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.000 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23

Tgt Ion: 95 Resp: 107910
Ion Ratio Lower Upper
95 100
174 93.9 0.0 201.8
176 91.9 0.0 191.8


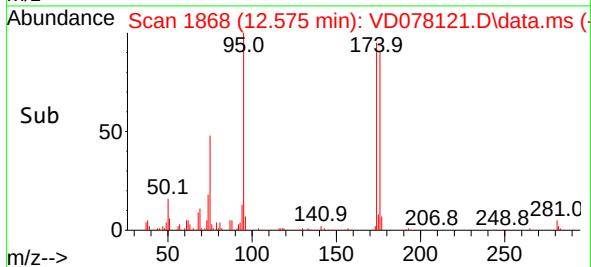
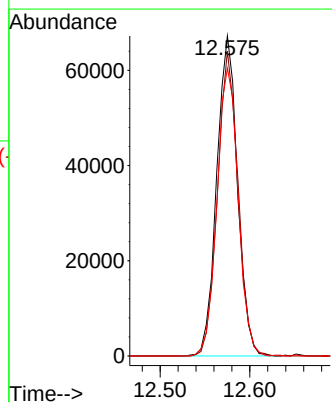
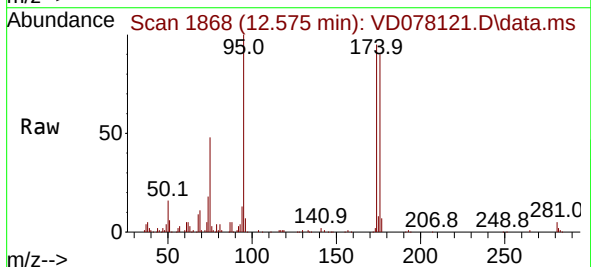


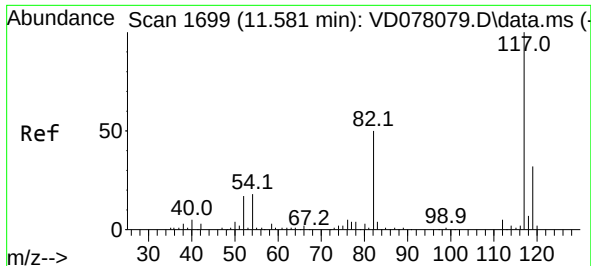

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. 0.000 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23

Instrument :
MSVOA_D
ClientSampleId :
MR-300-0-2

Tgt Ion:117 Resp: 313728
Ion Ratio Lower Upper
117 100
82 51.2 38.3 57.5
119 31.2 25.0 37.4

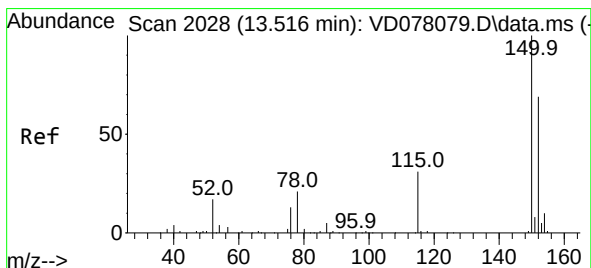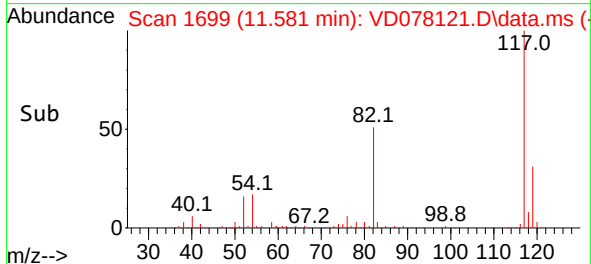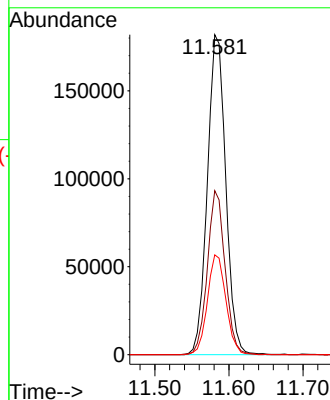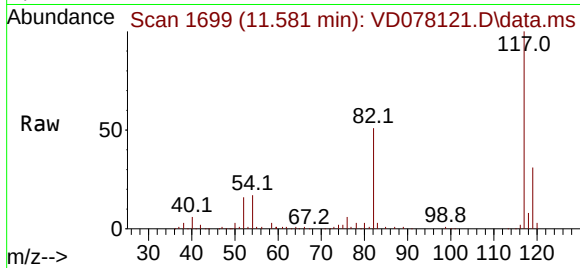

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD078121.D
Acq: 02 Jan 2024 14:23

Tgt Ion:152 Resp: 108675
Ion Ratio Lower Upper
152 100
115 55.4 27.1 81.3
150 159.9 0.0 353.6

