

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_D\DATA\VD010320\
 Data File : VD064736.D
 Acq On : 03 Jan 2020 16:05
 Operator : VA/SY
 Sample : K6472-03
 Misc : 6.49G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 K309-SB-03

Quant Time: Jan 06 07:07:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 24 13:19:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.99	168	487099	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	769894	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	687076	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	321222	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.34	65	241415	56.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.42%	
35) Dibromofluoromethane	7.92	113	239395	50.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.36%	
50) Toluene-d8	10.34	98	928261	51.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.62%	
62) 4-Bromofluorobenzene	12.64	95	282530	49.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.78%	
Target Compounds						
16) Acetone	4.17	43	5274	9.322	ug/l	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD010320\
Data File : VD064736.D
Acq On : 03 Jan 2020 16:05
Operator : VA/SY
Sample : K6472-03
Misc : 6.49G/5.00ml/MSVOA_D/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
K309-SB-03

Quant Time: Jan 06 07:07:40 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 24 13:19:06 2019
Response via : Initial Calibration

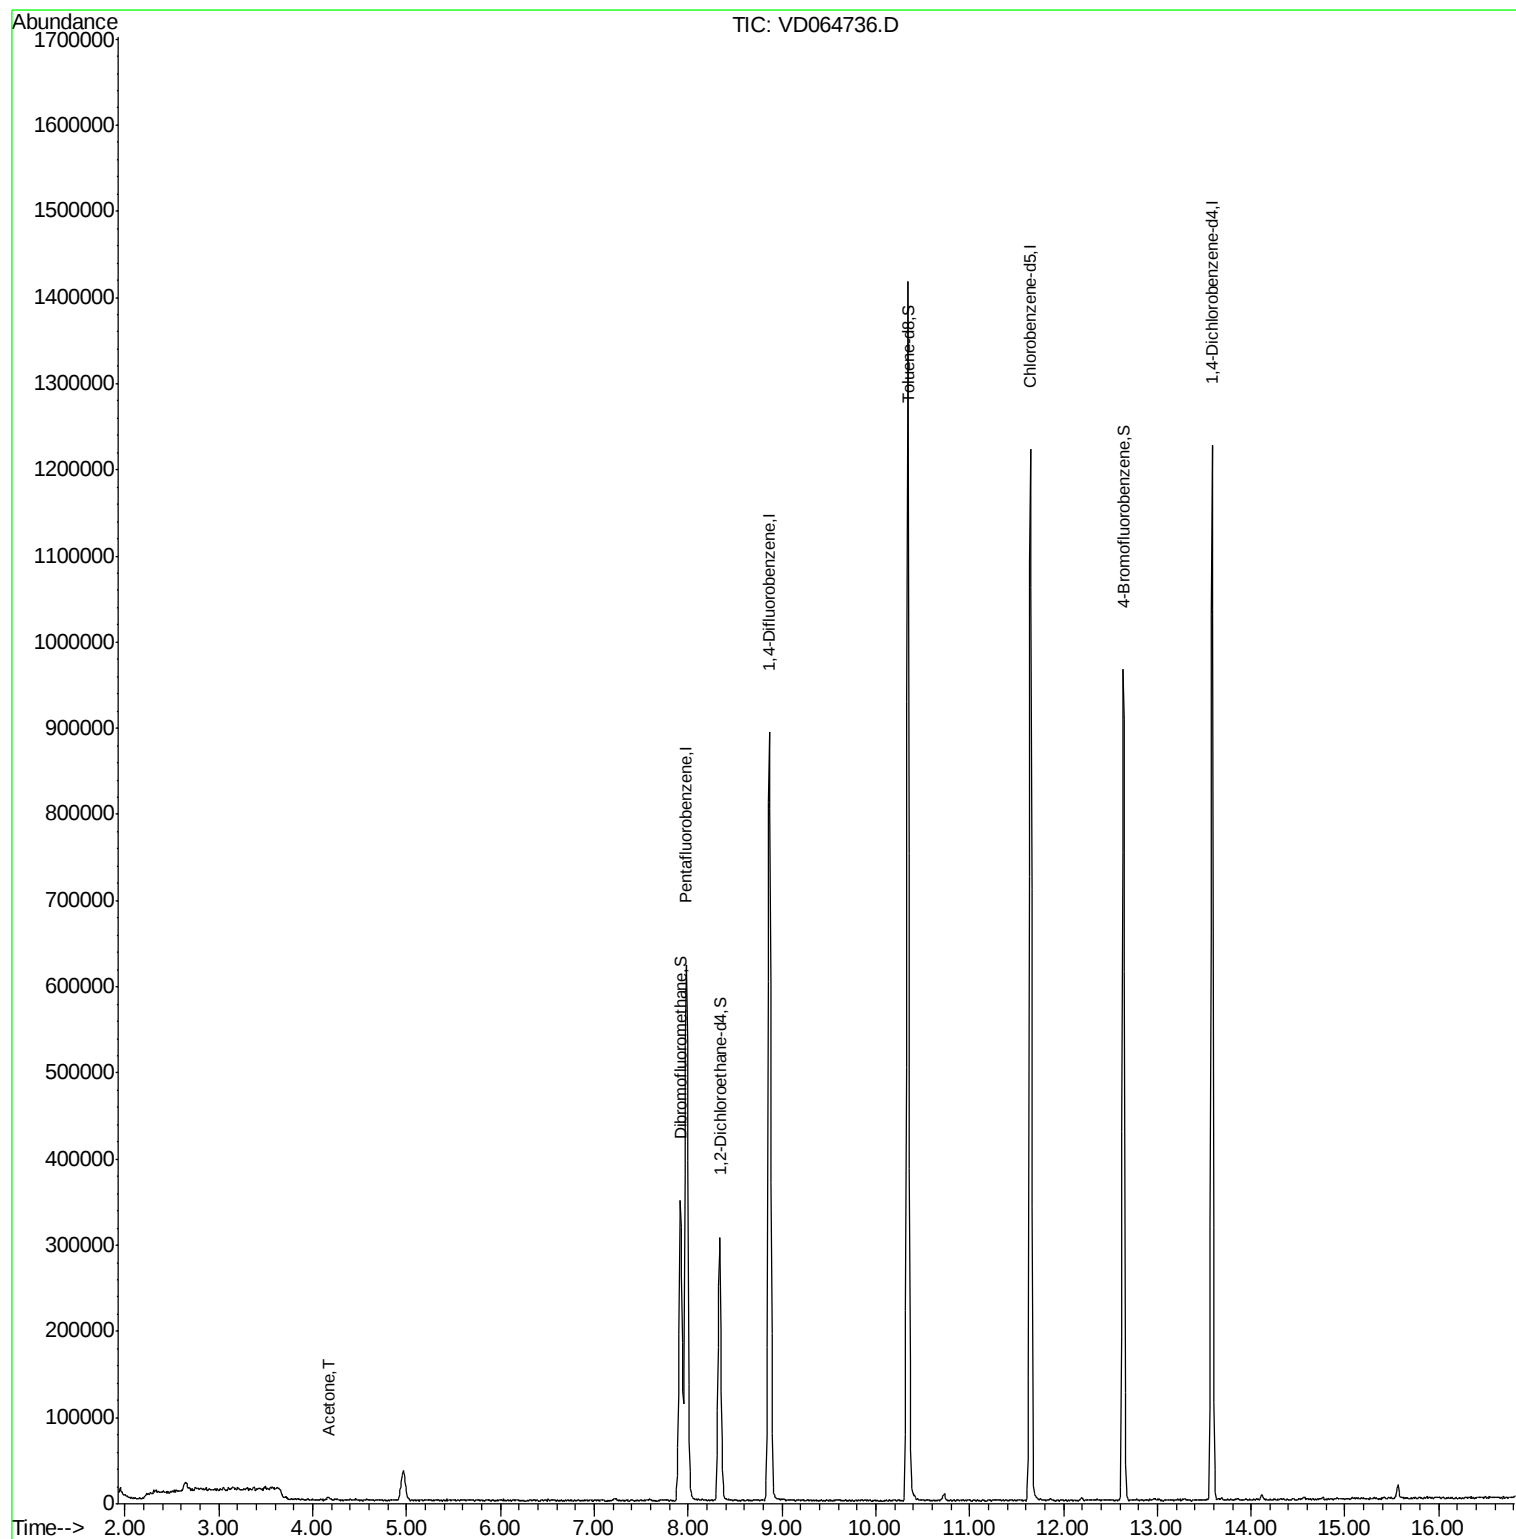



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.99 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD064736.D

Acq: 03 Jan 2020 16:05

Instrument :

MSVOA_D

ClientSampleId :


K309-SB-03

Tgt Ion:168 Resp: 487099

Ion Ratio Lower Upper




168 100

99 54.0 41.8 62.6

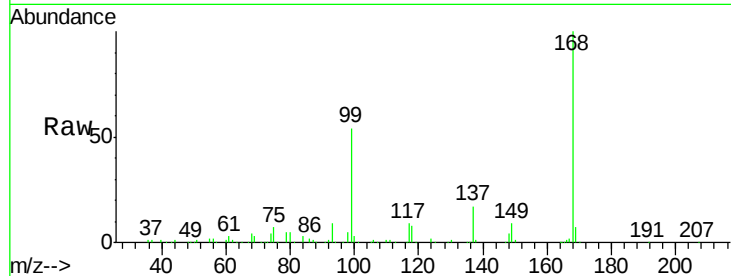

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

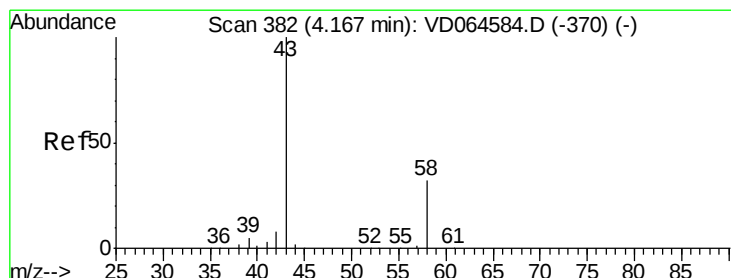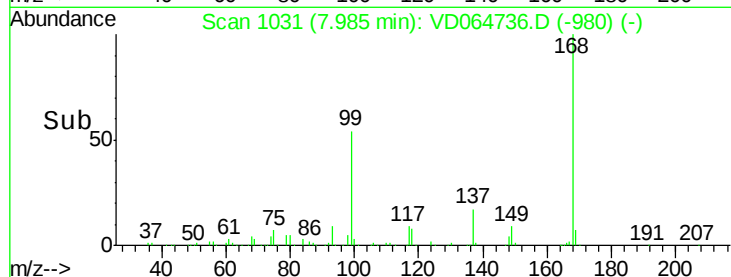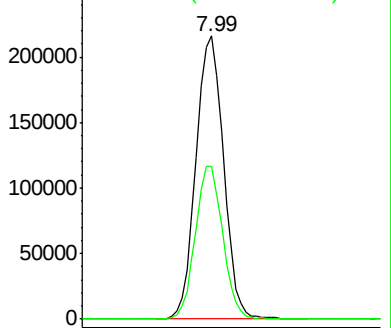

#16

Acetone

Concen: 9.322 ug/l

RT: 4.17 min Scan# 382

Delta R.T. 0.00 min

Lab File: VD064736.D


Acq: 03 Jan 2020 16:05

Tgt Ion: 43 Resp: 5274

Ion Ratio Lower Upper



43 100


58 31.0 25.8 38.6

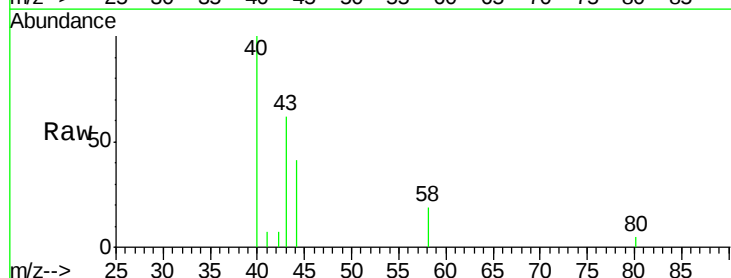

Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC



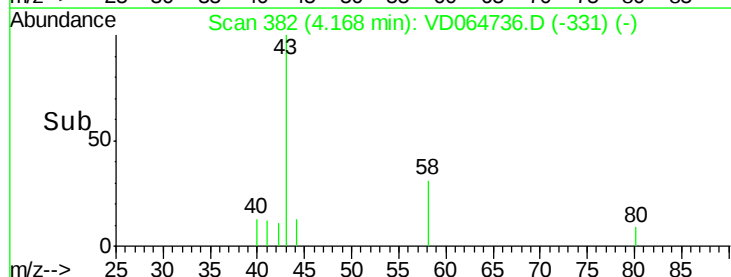
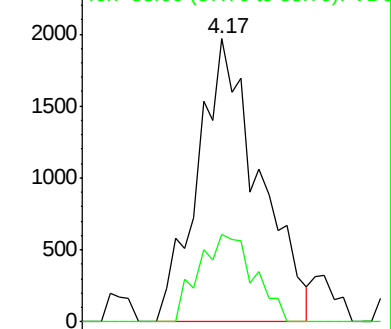


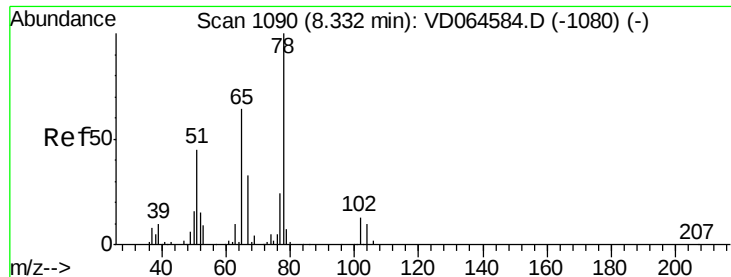

#33
 1,2-Dichloroethane-d4
 Concen: 56.206 ug/l
 RT: 8.34 min Scan# 1091
 Delta R.T. 0.01 min
 Lab File: VD064736.D
 Acq: 03 Jan 2020 16:05




Instrument :
 MSVOA_D
 ClientSampleId :
 K309-SB-03

Tgt Ion: 65 Resp: 241415
 Ion Ratio Lower Upper
 65 100
 67 52.1 0.0 106.2

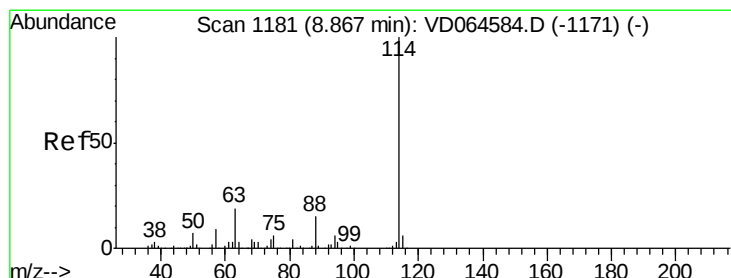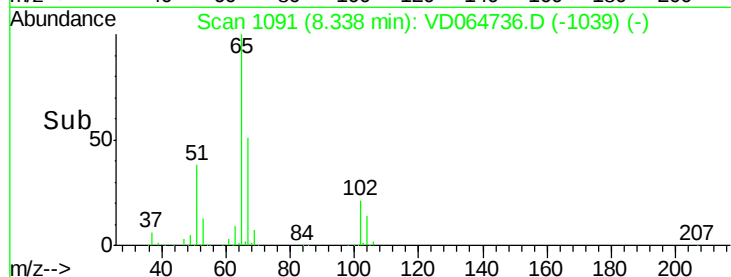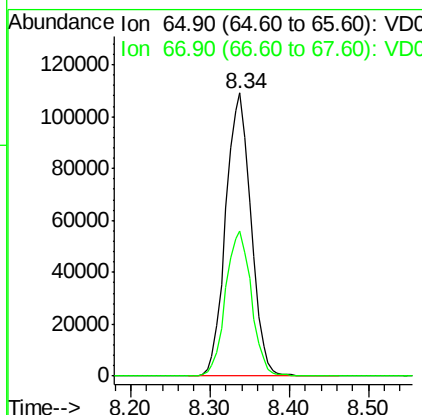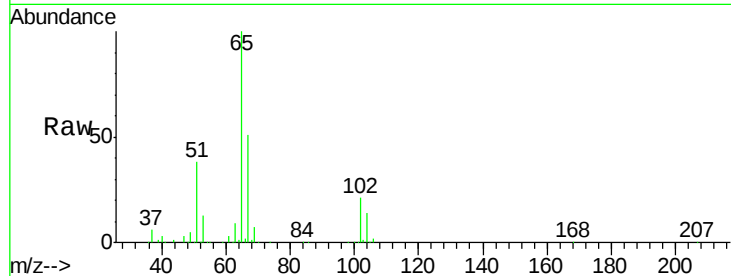

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.87 min Scan# 1181
 Delta R.T. 0.00 min
 Lab File: VD064736.D
 Acq: 03 Jan 2020 16:05

Tgt Ion: 114 Resp: 769894
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 38.0
 88 14.4 0.0 29.2


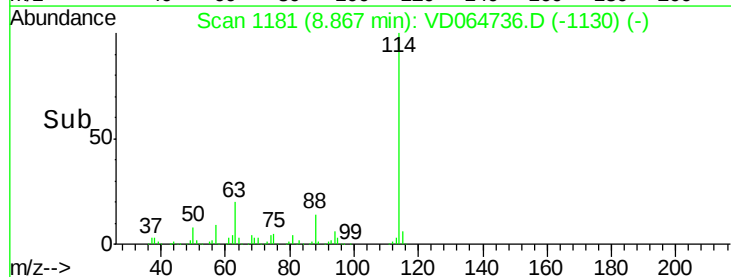
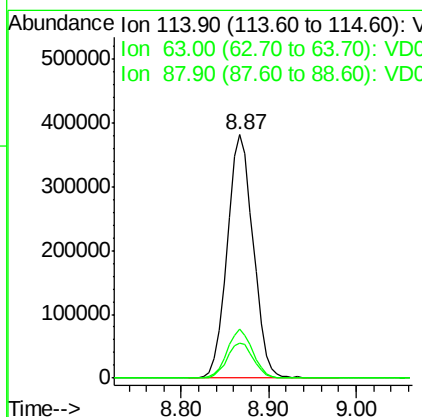
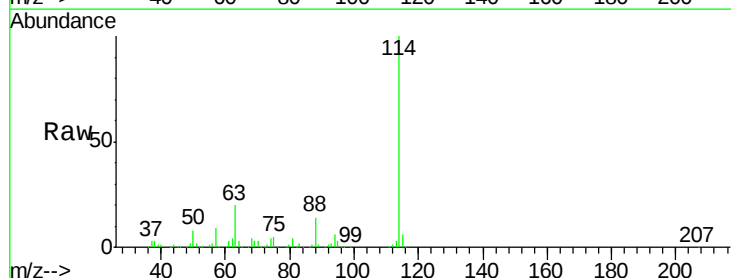




#35
 Dibromofluoromethane
 Concen: 50.682 ug/l
 RT: 7.92 min Scan# 1020
 Delta R.T. 0.00 min
 Lab File: VD064736.D
 Acq: 03 Jan 2020 16:05




Instrument :
 MSVOA_D
 ClientSampleId :
 K309-SB-03


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.9	80.6	121.0
192	22.9	17.9	26.9

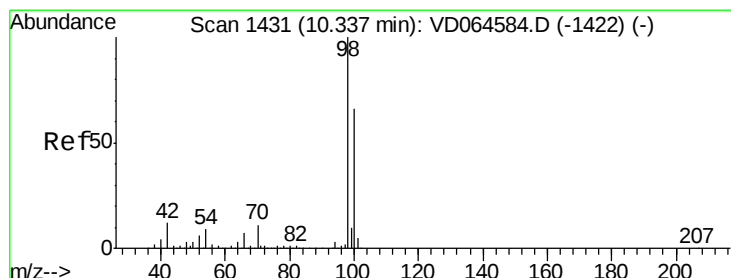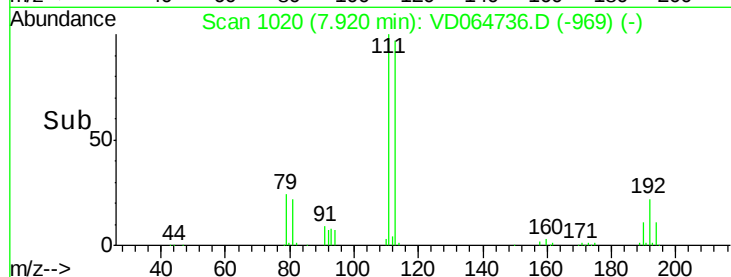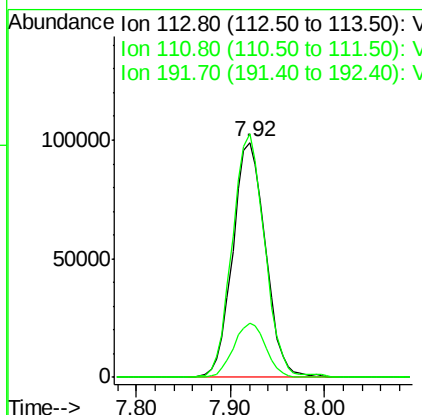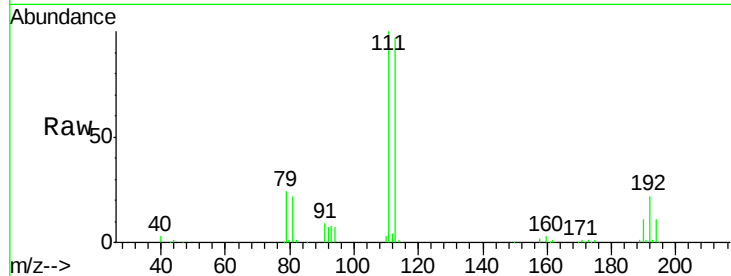

#50
 Toluene-d8
 Concen: 51.313 ug/l
 RT: 10.34 min Scan# 1432
 Delta R.T. 0.01 min
 Lab File: VD064736.D
 Acq: 03 Jan 2020 16:05

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.8	51.7	77.5

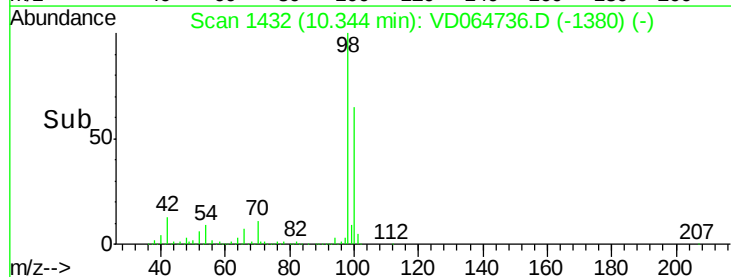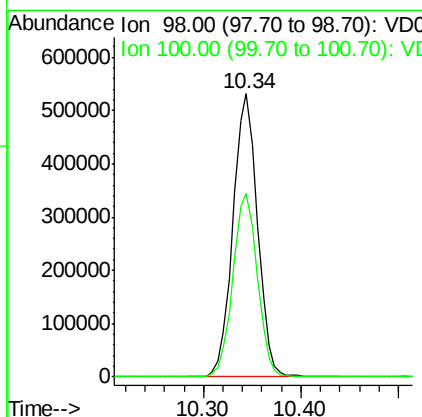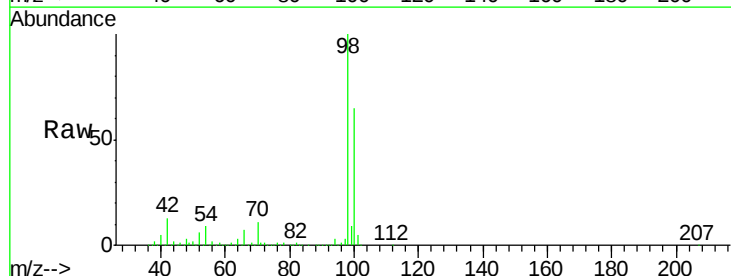

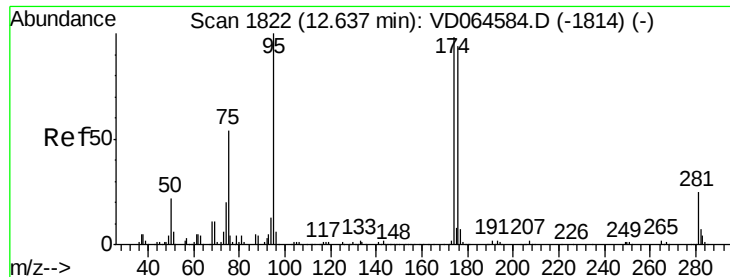

#62

4-Bromofluorobenzene

Concen: 49.391 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.00 min

Lab File: VD064736.D

Acq: 03 Jan 2020 16:05

Instrument :

MSVOA_D

ClientSampleId :

K309-SB-03


Tgt Ion: 95 Resp: 282530

Ion Ratio Lower Upper

95 100

174 96.4 0.0 193.2




176 91.4 0.0 184.2

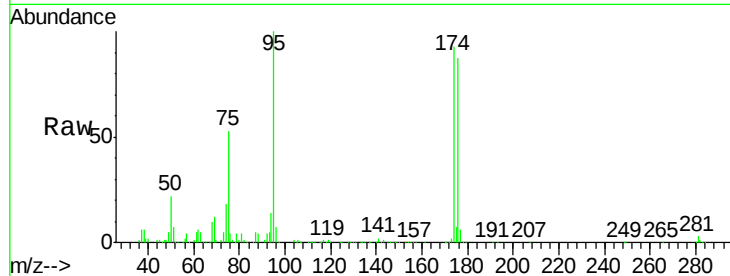

Abundance Ion 94.90 (94.60 to 95.60): V

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

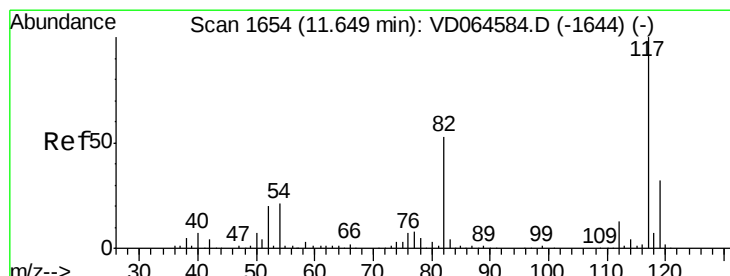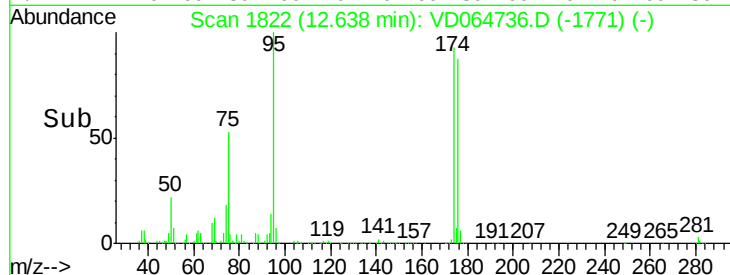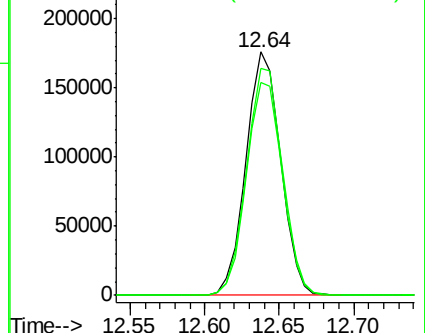

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.65 min Scan# 1654

Delta R.T. 0.00 min

Lab File: VD064736.D

Acq: 03 Jan 2020 16:05


Tgt Ion: 117 Resp: 687076

Ion Ratio Lower Upper

117 100

82 54.5 42.2 63.4



119 32.3 26.0 39.0

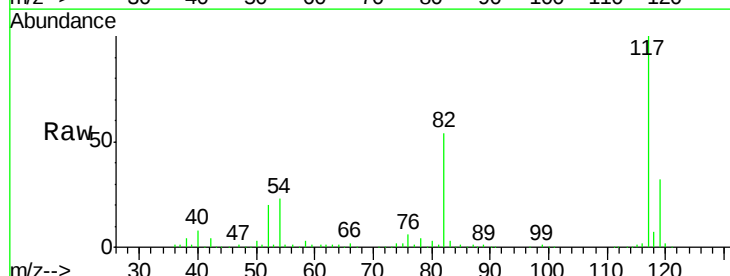


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

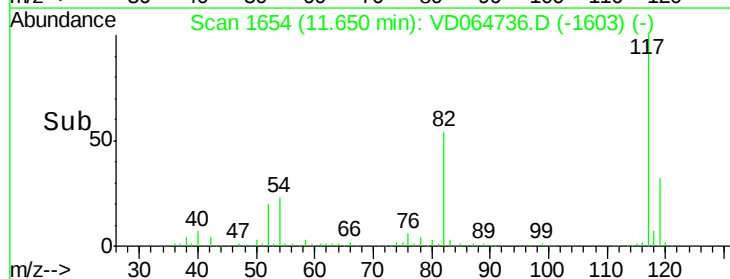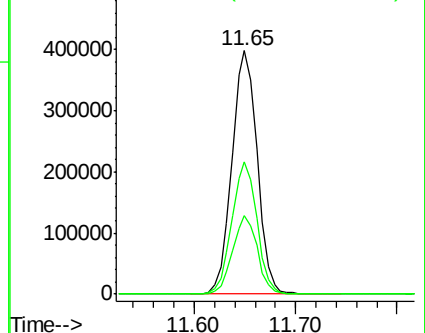

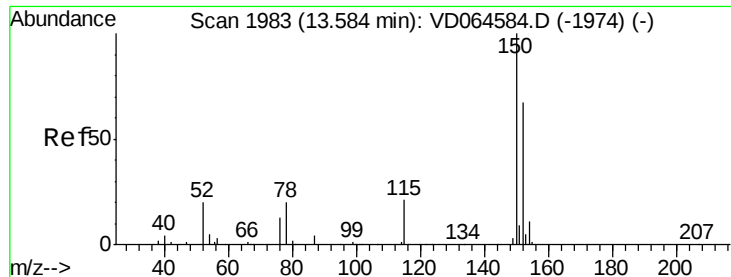

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.58 min Scan# 1983

Delta R.T. 0.00 min

Lab File: VD064736.D

Acq: 03 Jan 2020 16:05

Instrument :

MSVOA_D

ClientSampleId :

K309-SB-03


Tgt Ion:152 Resp: 321222

Ion Ratio Lower Upper

152 100

115 54.4 27.8 83.4

150 155.4 0.0 351.4

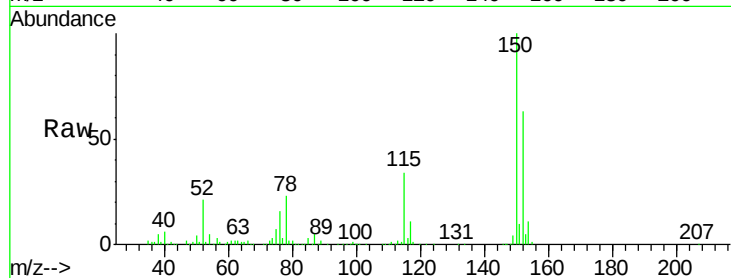

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

