


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010320\
 Data File : VD064748.D
 Acq On : 03 Jan 2020 22:17
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Title : SW846 8260
 Last Update : Tue Dec 24 13:19:06 2019

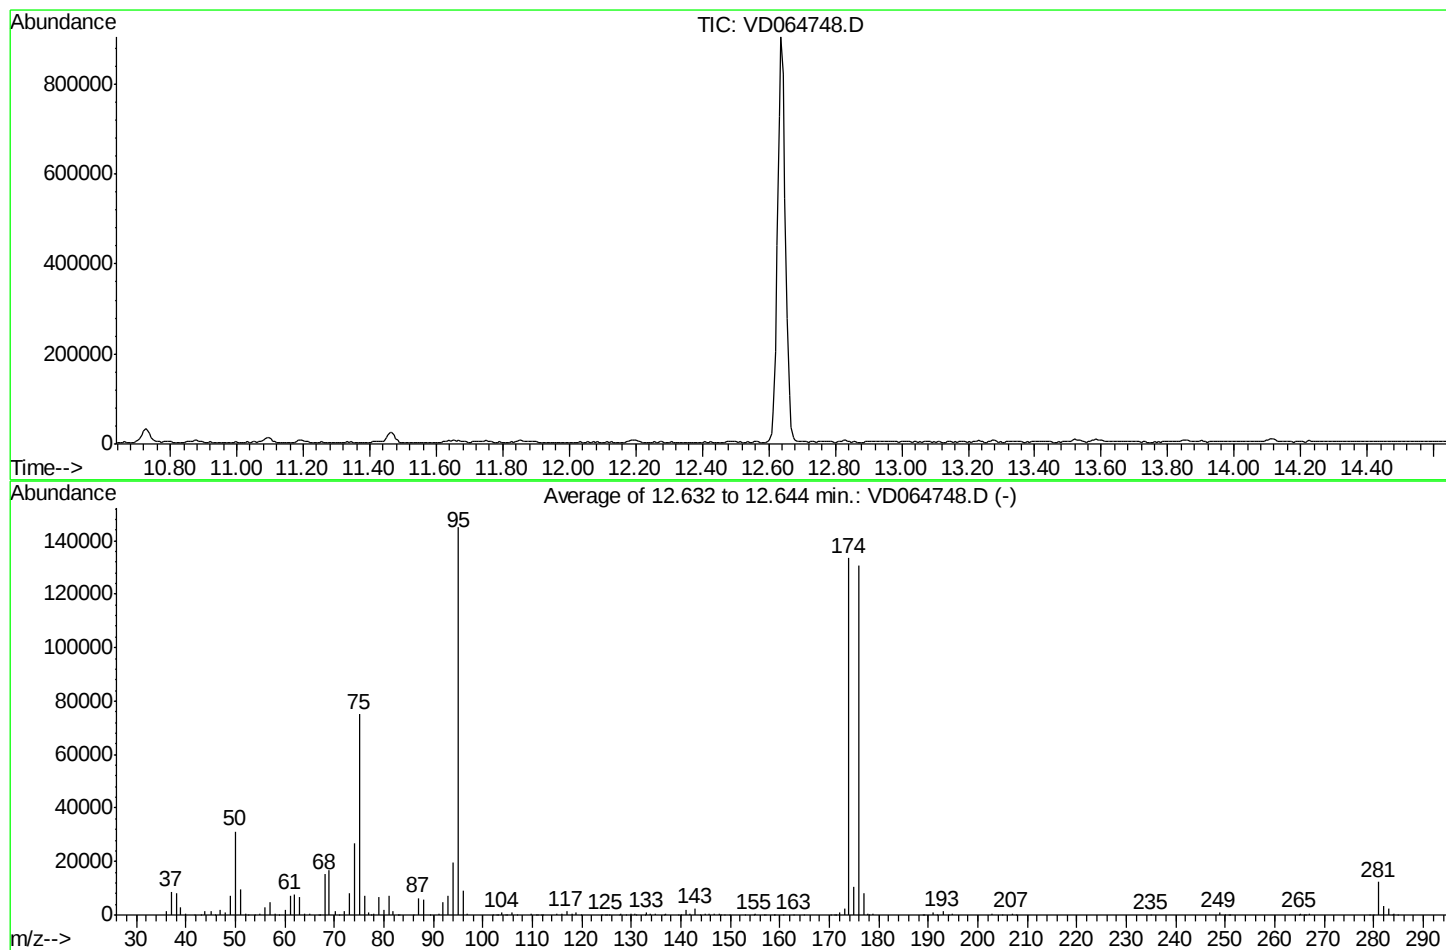

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	31237	PASS
75	95	30	60	51.8	75053	PASS
95	95	100	100	100.0	145000	PASS
96	95	5	9	6.2	9049	PASS
173	174	0.00	2	1.7	2210	PASS
174	95	50	100	92.1	133509	PASS
175	174	5	9	8.0	10712	PASS
176	174	95	101	98.1	130909	PASS
177	176	5	9	6.2	8097	PASS