
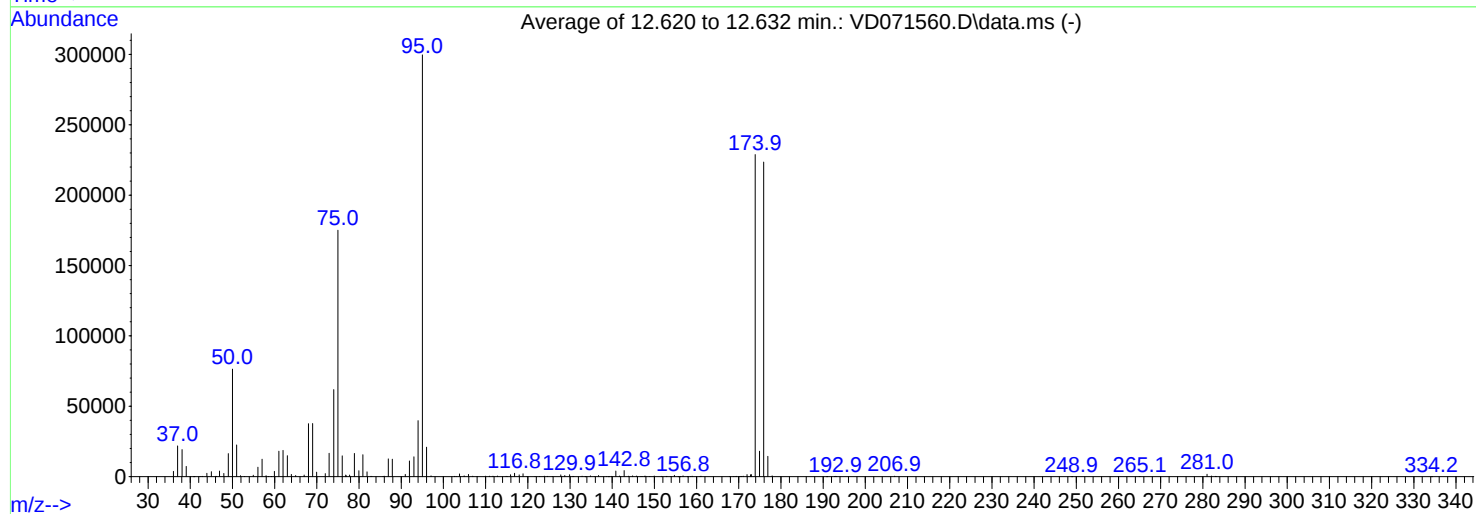


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010322\
 Data File : VD071560.D
 Acq On : 03 Jan 2022 09:39
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
 Title : SW846 8260
 Last Update : Thu Dec 23 08:20:24 2021

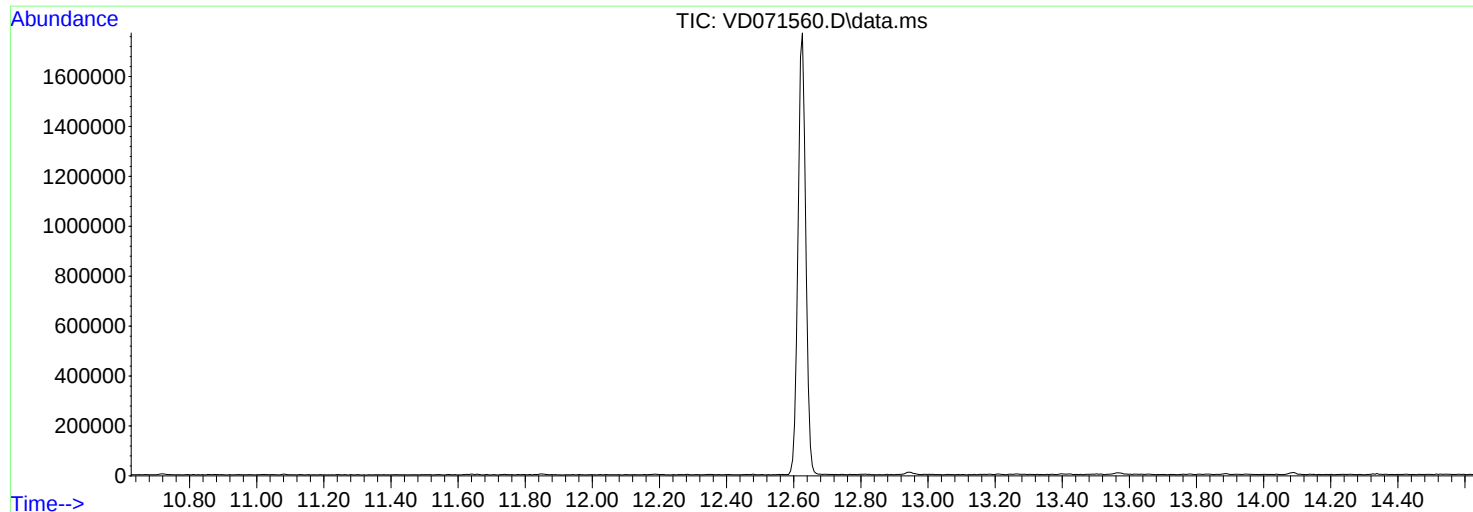

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	76459	PASS
75	95	30	60	58.4	175104	PASS
95	95	100	100	100.0	299691	PASS
96	95	5	9	7.0	20965	PASS
173	174	0.00	2	0.7	1536	PASS
174	95	50	100	76.4	228907	PASS
175	174	5	9	7.9	18040	PASS
176	174	95	101	97.6	223467	PASS
177	176	5	9	6.5	14471	PASS