


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010421\
 Data File : VD067985.D
 Acq On : 04 Jan 2021 09:35
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
 Title : SW846 8260
 Last Update : Wed Dec 23 07:34:16 2020

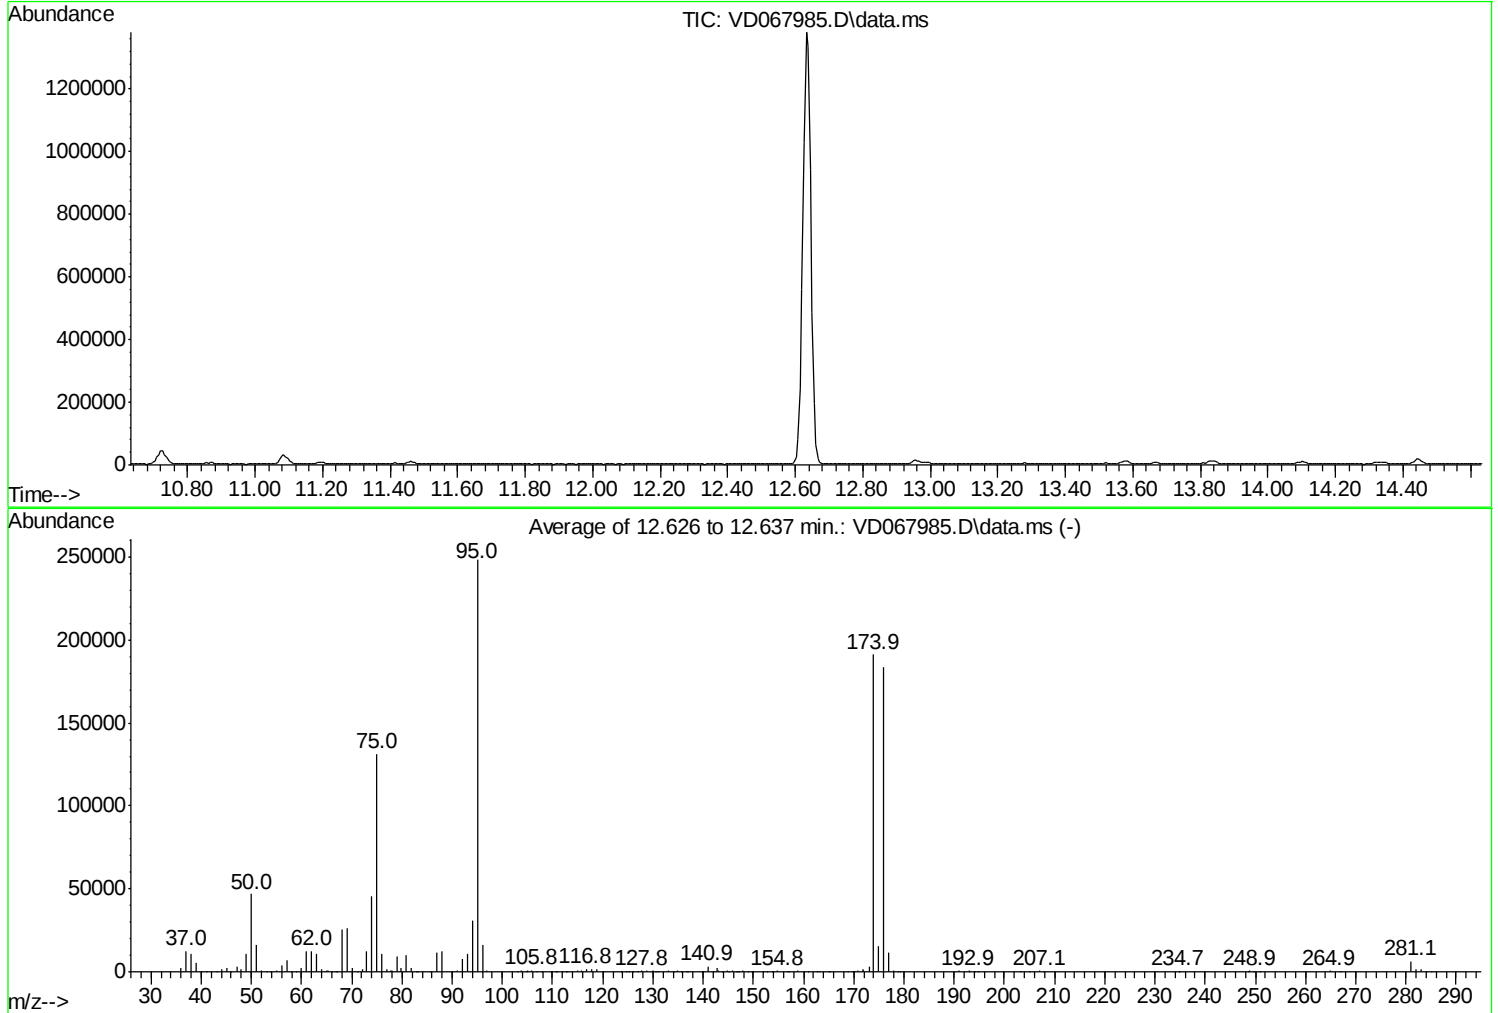

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	46763	PASS
75	95	30	60	52.9	131413	PASS
95	95	100	100	100.0	248363	PASS
96	95	5	9	6.5	16021	PASS
173	174	0.00	2	1.6	3072	PASS
174	95	50	100	77.0	191317	PASS
175	174	5	9	7.9	15146	PASS
176	174	95	101	96.2	183979	PASS
177	176	5	9	6.3	11600	PASS