

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010422\
 Data File : VD071588.D
 Acq On : 04 Jan 2022 12:57
 Operator : VA/SY
 Sample : M5196-11
 Misc : 6.89G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 B-4-(3-4)

Quant Time: Jan 04 15:41:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 23 08:20:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	411528	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	715075	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	653987	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	281417	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	272809	49.915	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.840%
35) Dibromofluoromethane	7.914	113	232091	48.293	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.580%
50) Toluene-d8	10.338	98	902535	49.695	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.400%
62) 4-Bromofluorobenzene	12.626	95	288536	44.709	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	89.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010422\
Data File : VD071588.D
Acq On : 04 Jan 2022 12:57
Operator : VA/SY
Sample : M5196-11
Misc : 6.89G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
B-4-(3-4)

Quant Time: Jan 04 15:41:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 23 08:20:24 2021
Response via : Initial Calibration




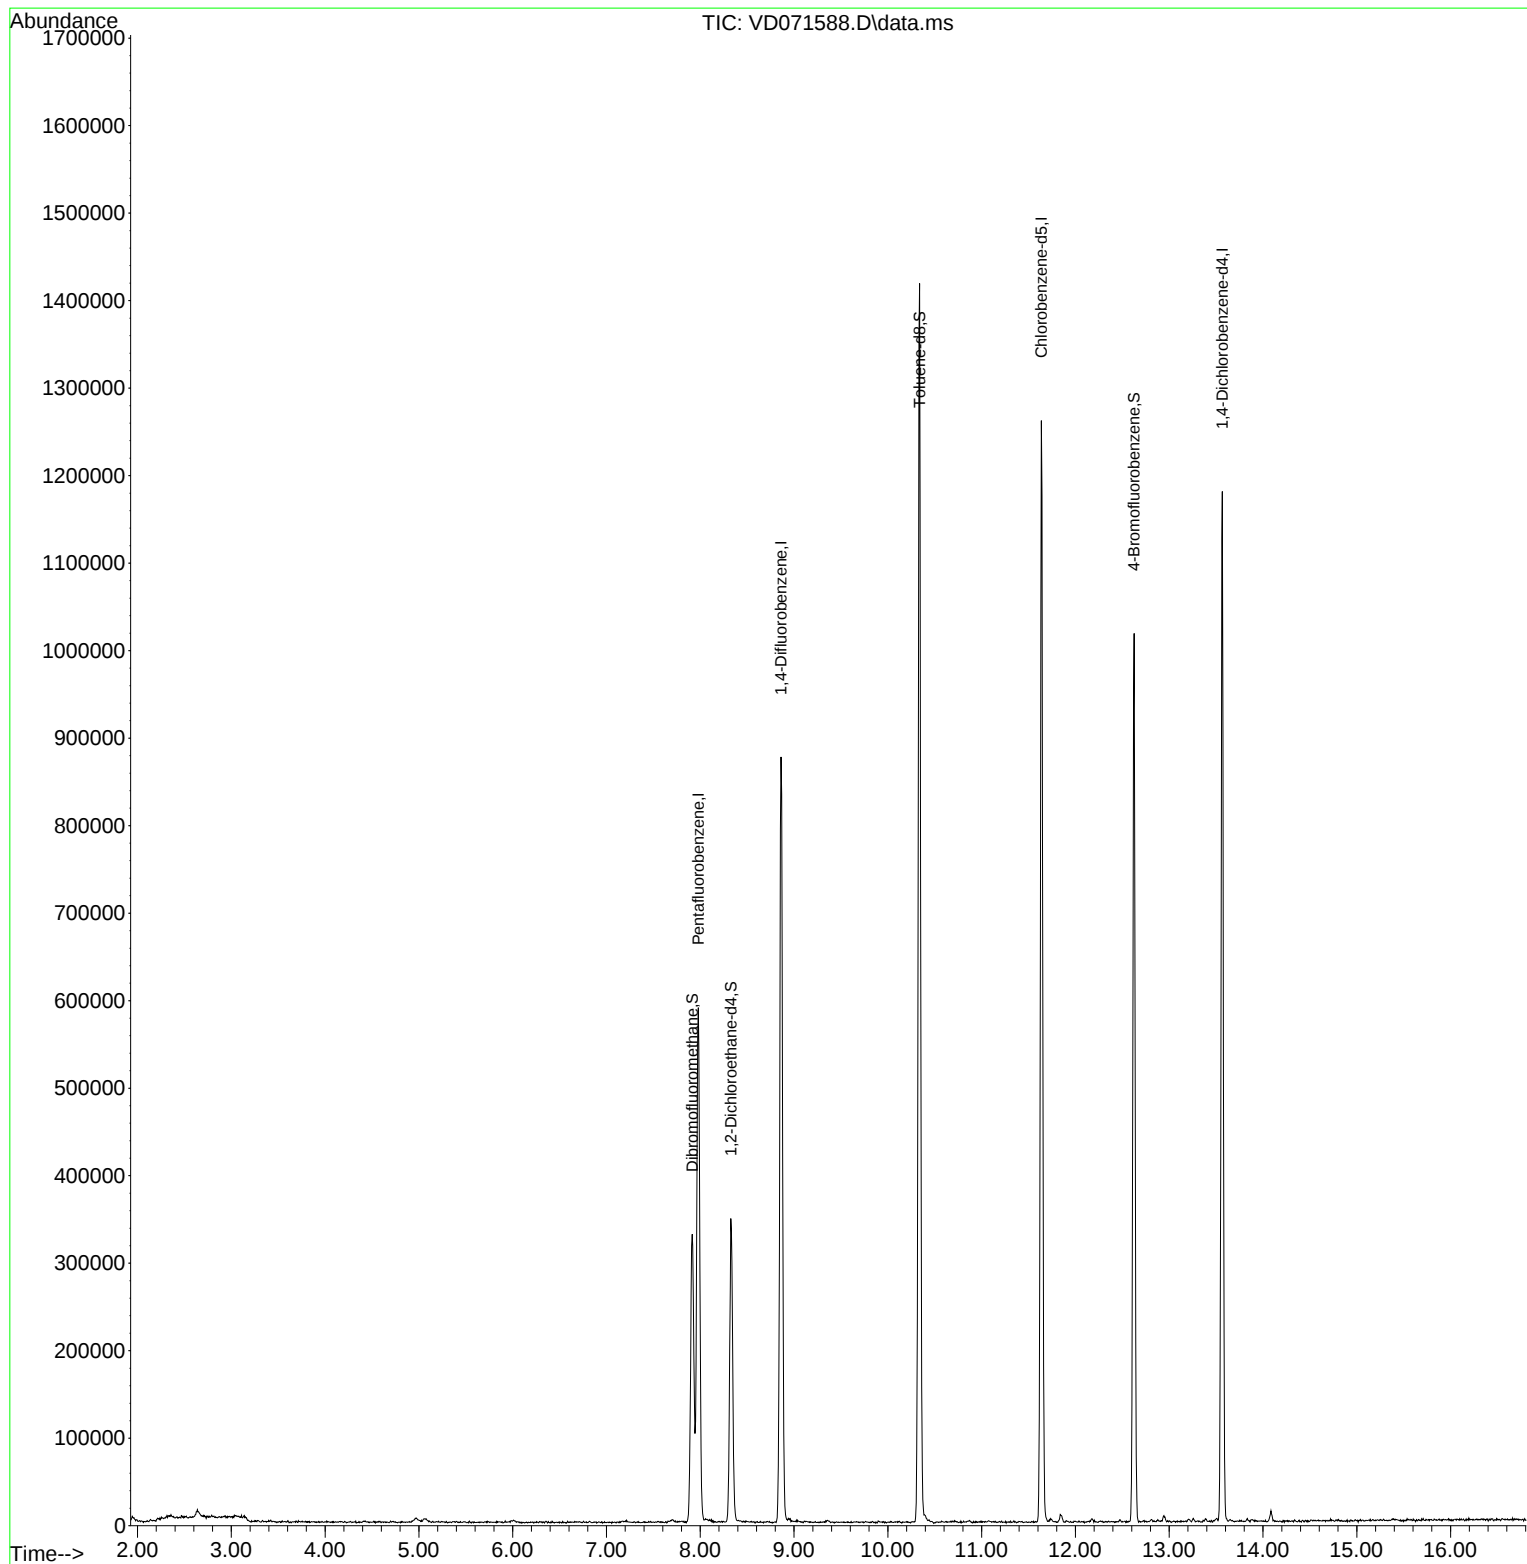


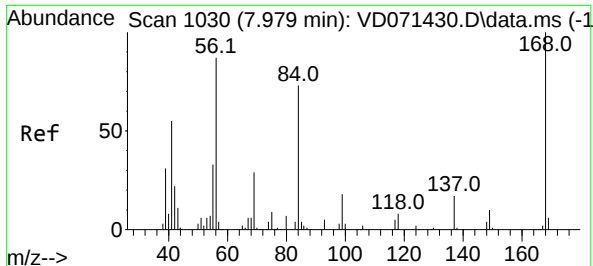

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.006 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57




Instrument :
MSVOA_D
ClientSampleId :
B-4-(3-4)

Tgt Ion:168 Resp: 411528
Ion Ratio Lower Upper
168 100
99 61.8 46.6 69.8

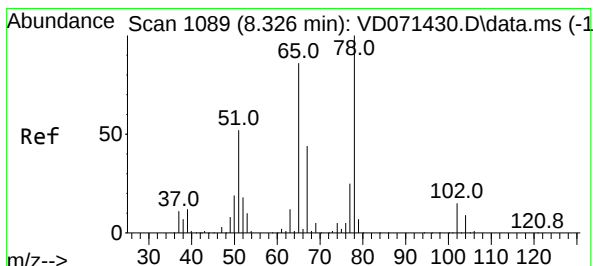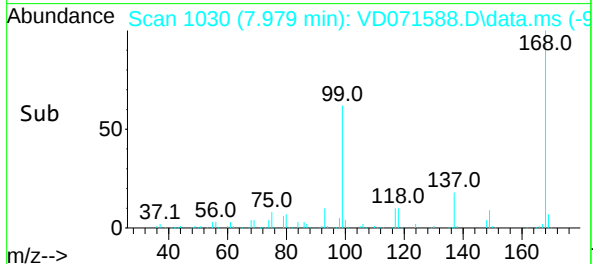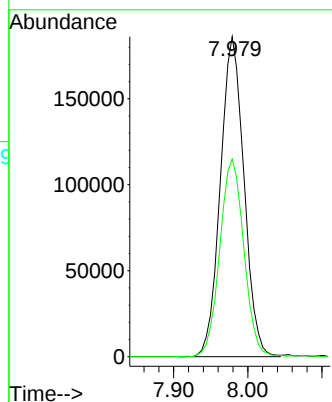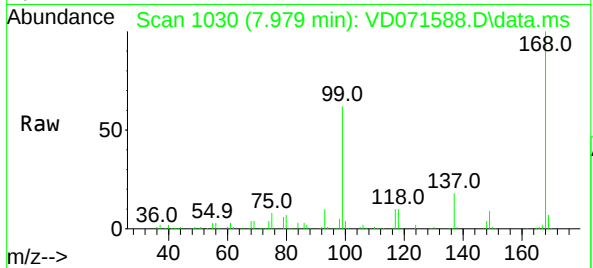

#33
1,2-Dichloroethane-d4
Concen: 49.915 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57

Tgt Ion: 65 Resp: 272809
Ion Ratio Lower Upper
65 100
67 50.8 0.0 112.2

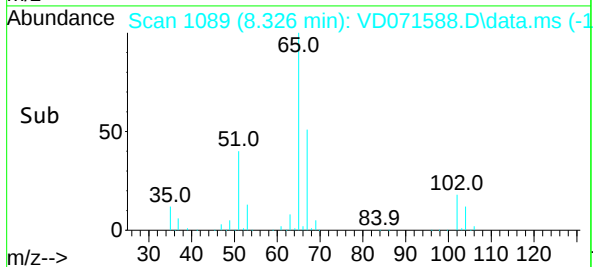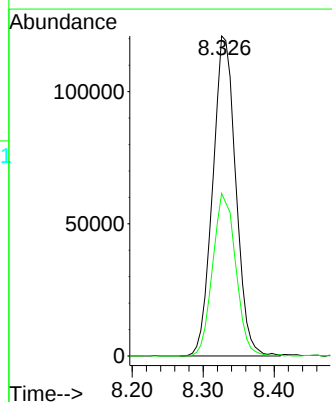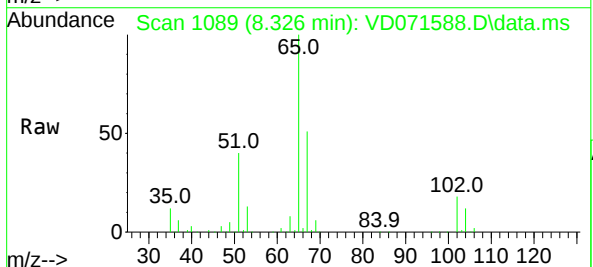



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD071588.D

Acq: 04 Jan 2022 12:57

Instrument :

MSVOA_D

ClientSampleId :

B-4-(3-4)





Tgt Ion:114 Resp: 715075

Ion Ratio Lower Upper

114 100

63 23.9 0.0 41.8

88 16.0 0.0 32.8

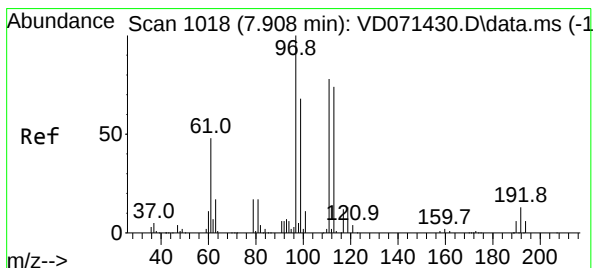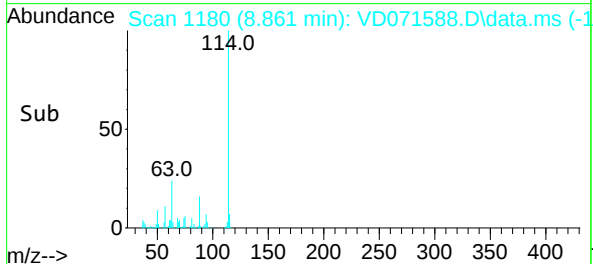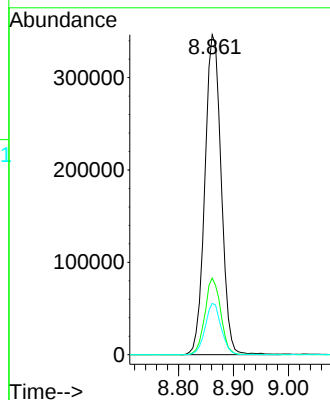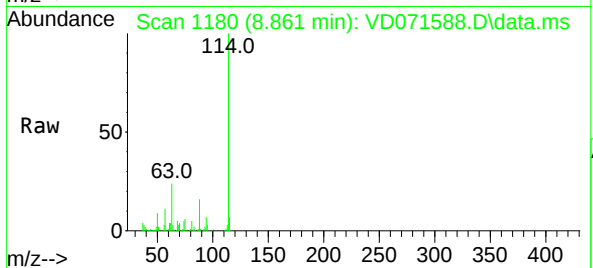

#35

Dibromofluoromethane

Concen: 48.293 ug/l

RT: 7.914 min Scan# 1019

Delta R.T. 0.006 min

Lab File: VD071588.D

Acq: 04 Jan 2022 12:57




Tgt Ion:113 Resp: 232091


Ion Ratio Lower Upper

113 100

111 103.1 82.0 123.0

192 17.7 15.2 22.8


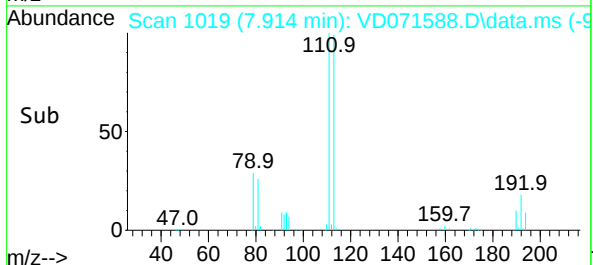
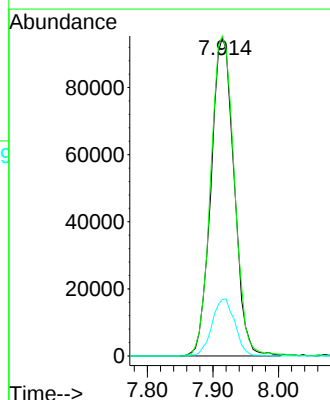
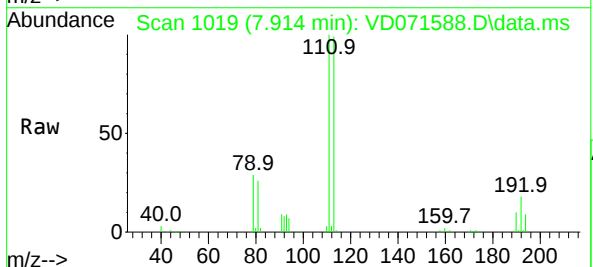


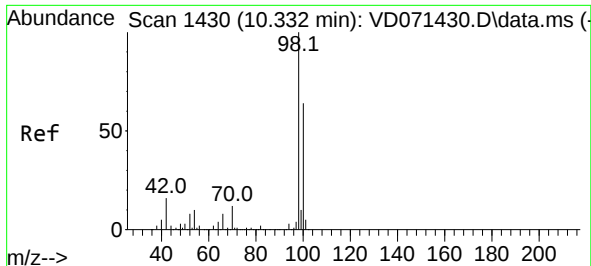

#50
Toluene-d8
Concen: 49.695 ug/l
RT: 10.338 min Scan# 1430
Delta R.T. 0.006 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57




Instrument :
MSVOA_D
ClientSampleId :
B-4-(3-4)


Tgt Ion: 98 Resp: 902535
Ion Ratio Lower Upper
98 100
100 64.4 51.8 77.6

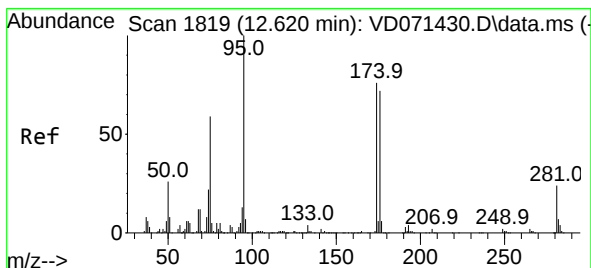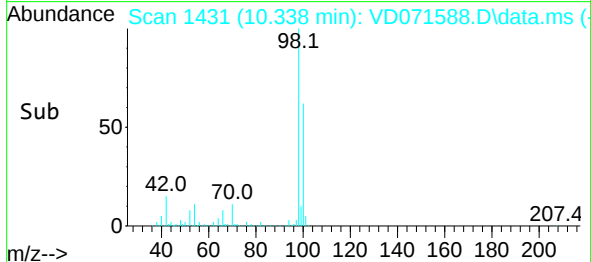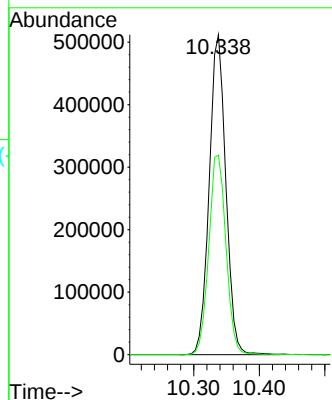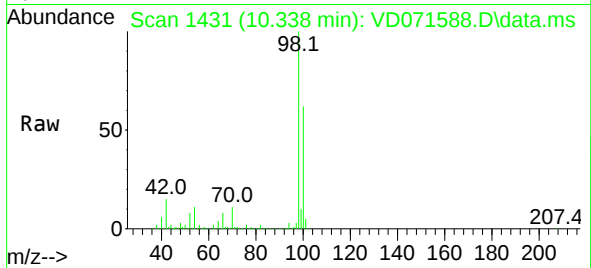

#62
4-Bromofluorobenzene
Concen: 44.709 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57

Tgt Ion: 95 Resp: 288536
Ion Ratio Lower Upper
95 100
174 76.8 0.0 159.4
176 73.7 0.0 154.0


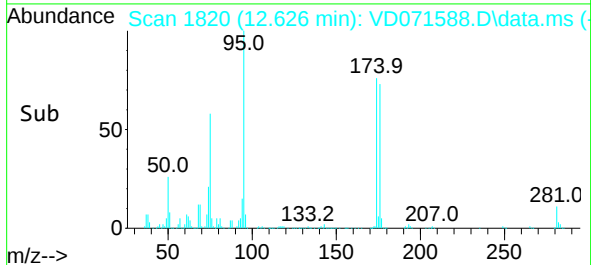
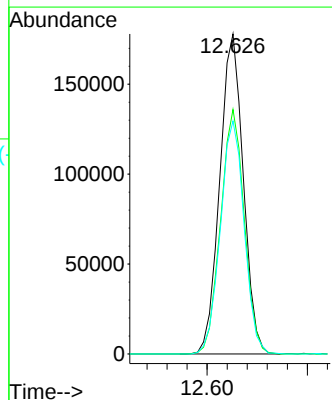
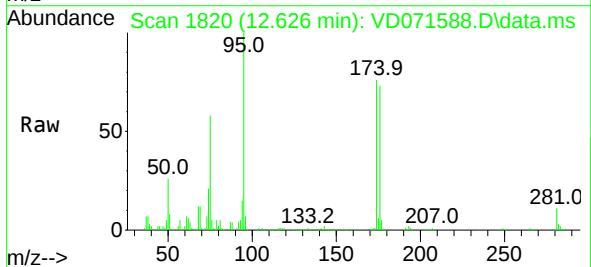


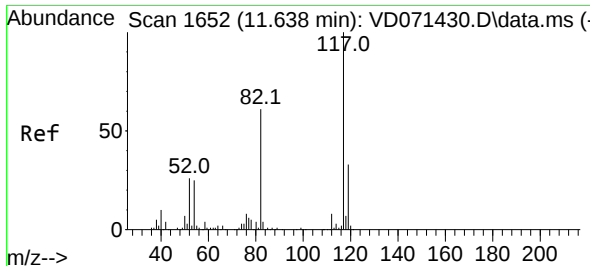

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57

Instrument :
MSVOA_D
ClientSampleId :
B-4-(3-4)

Tgt Ion:117 Resp: 653987
Ion Ratio Lower Upper
117 100
82 57.5 44.7 67.1
119 31.2 26.2 39.4

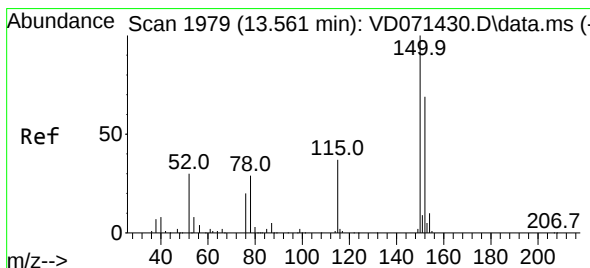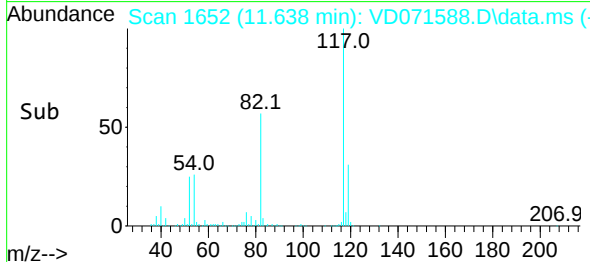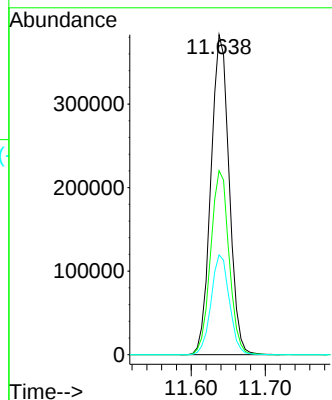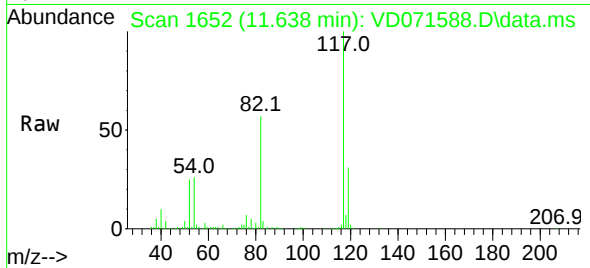

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. 0.006 min
Lab File: VD071588.D
Acq: 04 Jan 2022 12:57

Tgt Ion:152 Resp: 281417
Ion Ratio Lower Upper
152 100
115 61.6 29.8 89.3
150 157.1 0.0 349.2

