
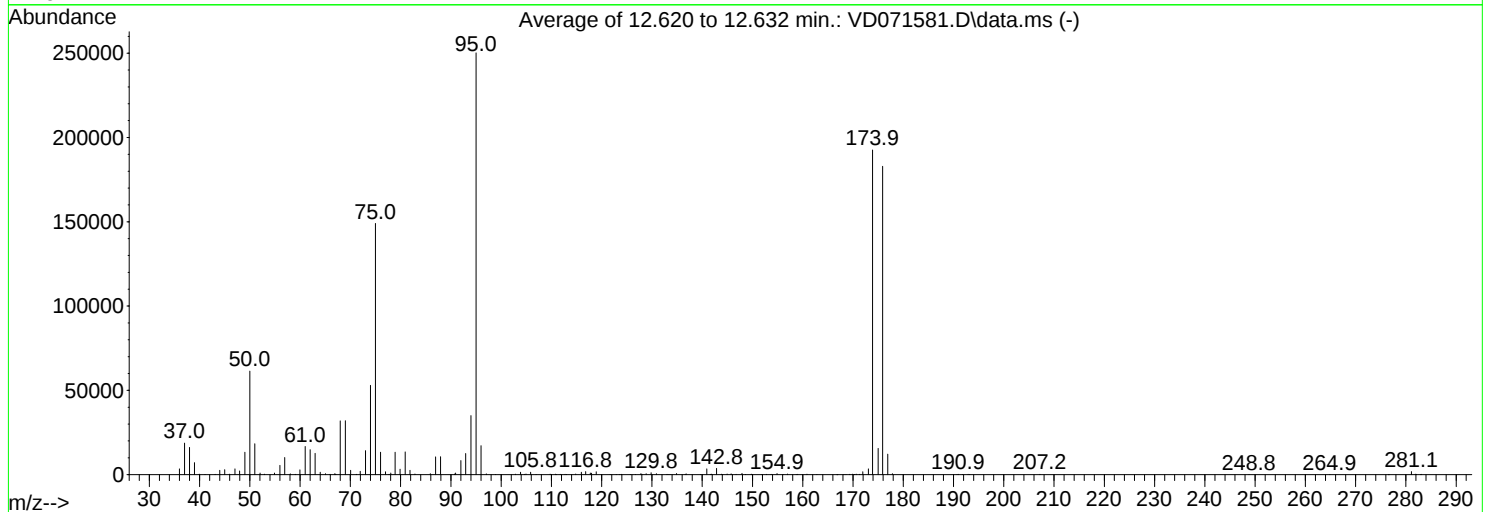


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010422\
 Data File : VD071581.D
 Acq On : 04 Jan 2022 08:51
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
 Title : SW846 8260
 Last Update : Thu Dec 23 08:20:24 2021

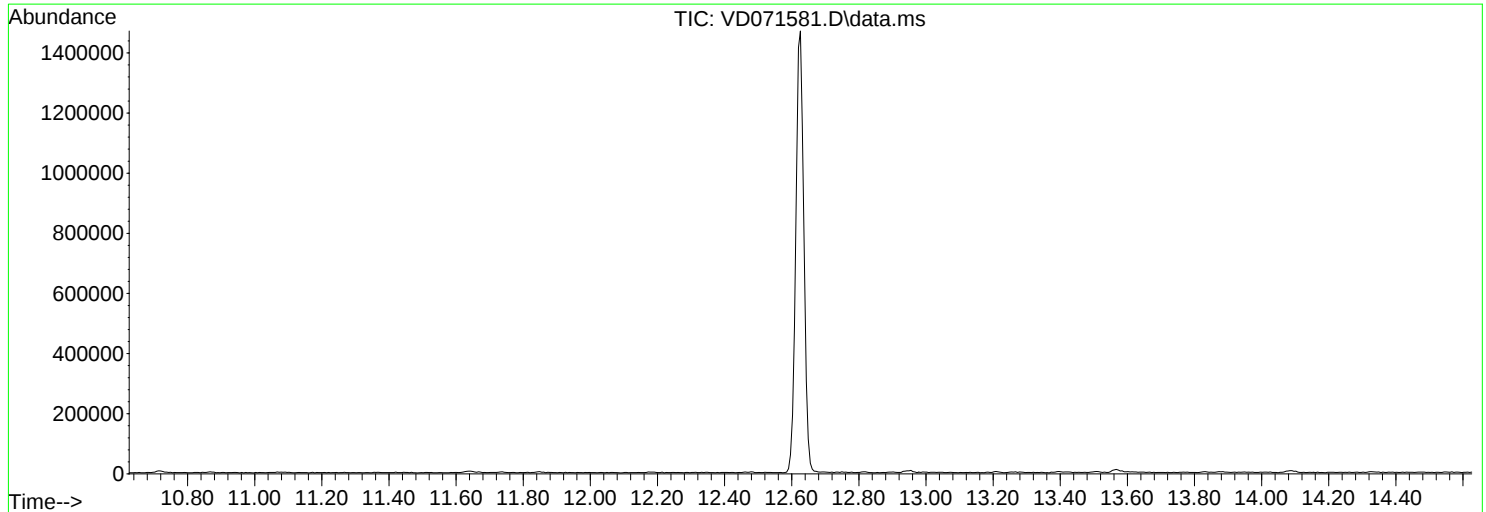

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1808

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	61403	PASS
75	95	30	60	59.5	148976	PASS
95	95	100	100	100.0	250219	PASS
96	95	5	9	6.9	17204	PASS
173	174	0.00	2	1.8	3398	PASS
174	95	50	100	77.0	192576	PASS
175	174	5	9	8.1	15622	PASS
176	174	95	101	95.0	182955	PASS
177	176	5	9	6.7	12198	PASS