


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010521\
 Data File : VD067997.D
 Acq On : 05 Jan 2021 09:12
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
 Title : SW846 8260
 Last Update : Wed Dec 23 07:34:16 2020

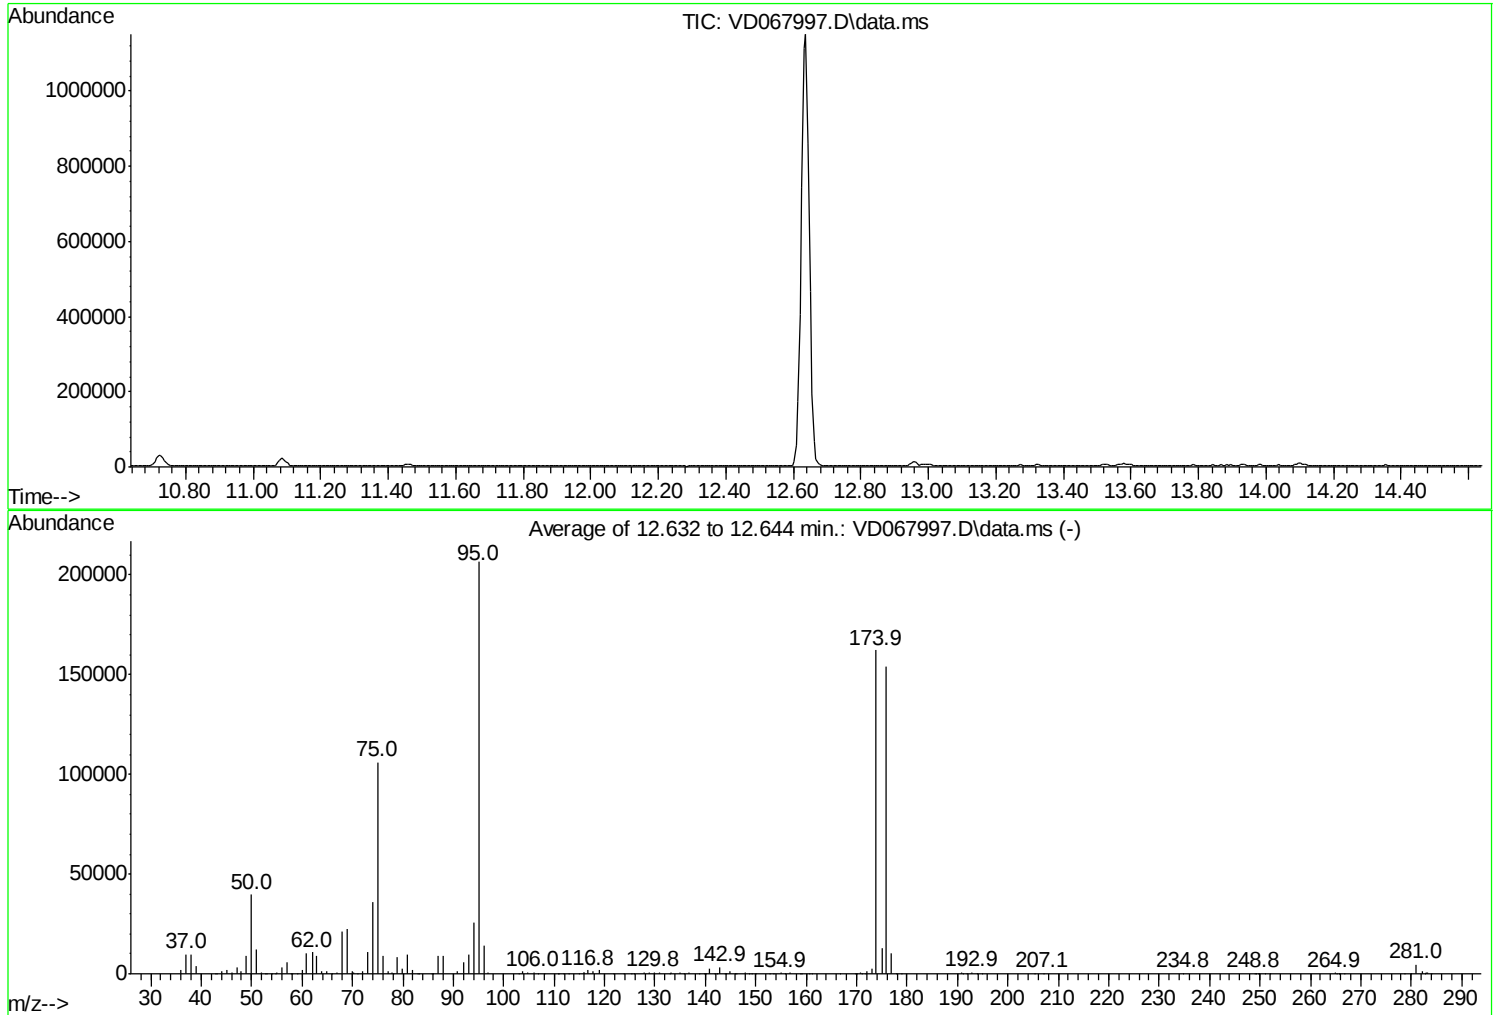

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	39627	PASS
75	95	30	60	51.3	106043	PASS
95	95	100	100	100.0	206656	PASS
96	95	5	9	6.7	13873	PASS
173	174	0.00	2	1.8	2855	PASS
174	95	50	100	78.5	162219	PASS
175	174	5	9	7.9	12740	PASS
176	174	95	101	94.9	154005	PASS
177	176	5	9	6.7	10302	PASS