
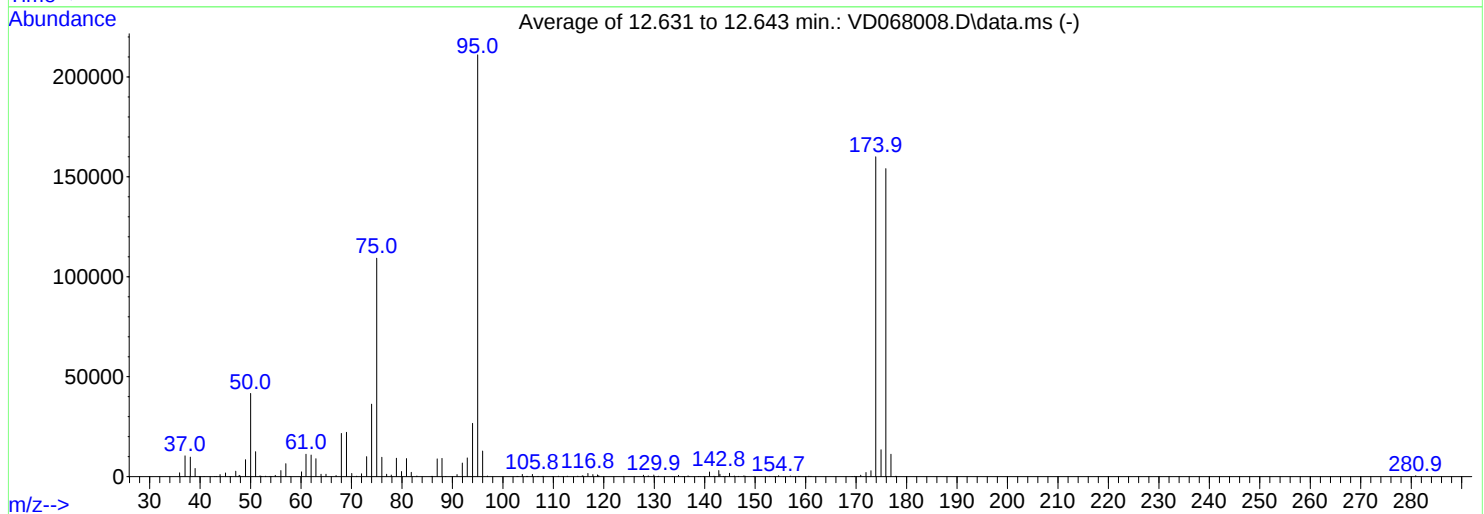


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010621\
 Data File : VD068008.D
 Acq On : 06 Jan 2021 10:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
 Title : SW846 8260
 Last Update : Wed Dec 23 07:34:16 2020

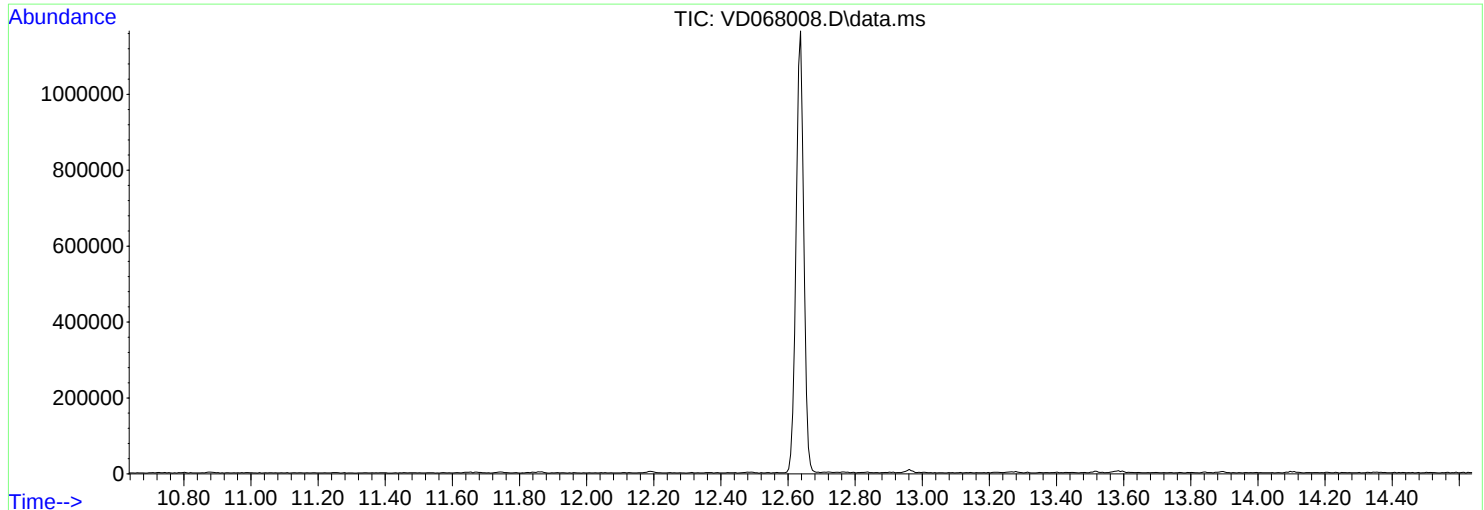

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	41621	PASS
75	95	30	60	51.8	109272	PASS
95	95	100	100	100.0	211051	PASS
96	95	5	9	6.1	12838	PASS
173	174	0.00	2	1.9	3001	PASS
174	95	50	100	75.8	160021	PASS
175	174	5	9	8.4	13457	PASS
176	174	95	101	96.3	154155	PASS
177	176	5	9	7.3	11194	PASS