


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010720\
 Data File : VD064787.D
 Acq On : 07 Jan 2020 09:43
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Title : SW846 8260
 Last Update : Tue Dec 24 13:19:06 2019

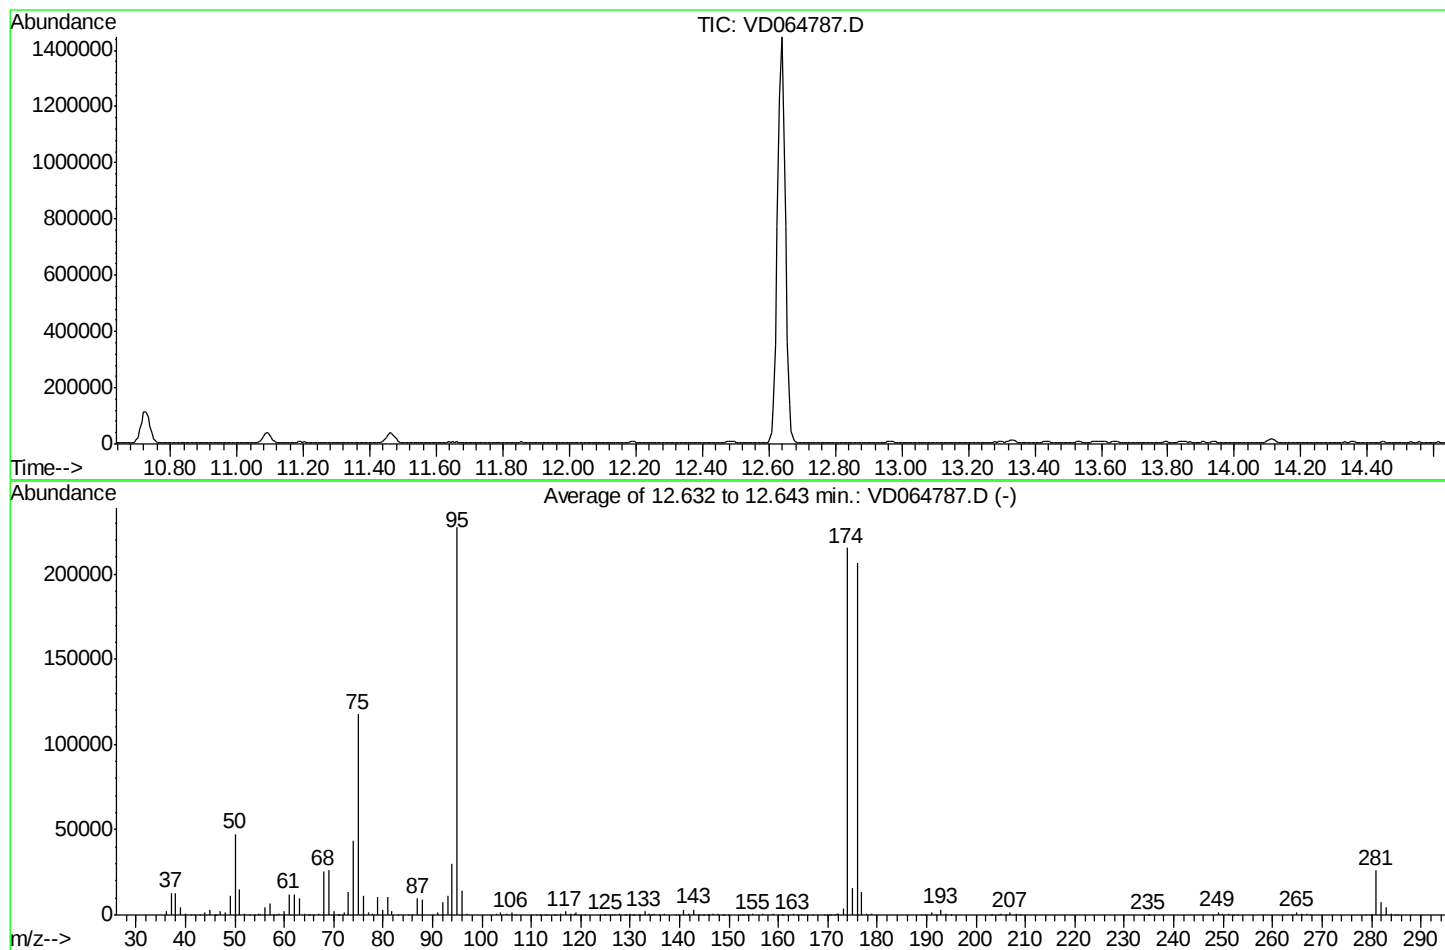

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	47405	PASS
75	95	30	60	51.7	117616	PASS
95	95	100	100	100.0	227328	PASS
96	95	5	9	6.4	14617	PASS
173	174	0.00	2	1.7	3588	PASS
174	95	50	100	94.7	215210	PASS
175	174	5	9	7.3	15791	PASS
176	174	95	101	95.9	206336	PASS
177	176	5	9	6.7	13813	PASS