
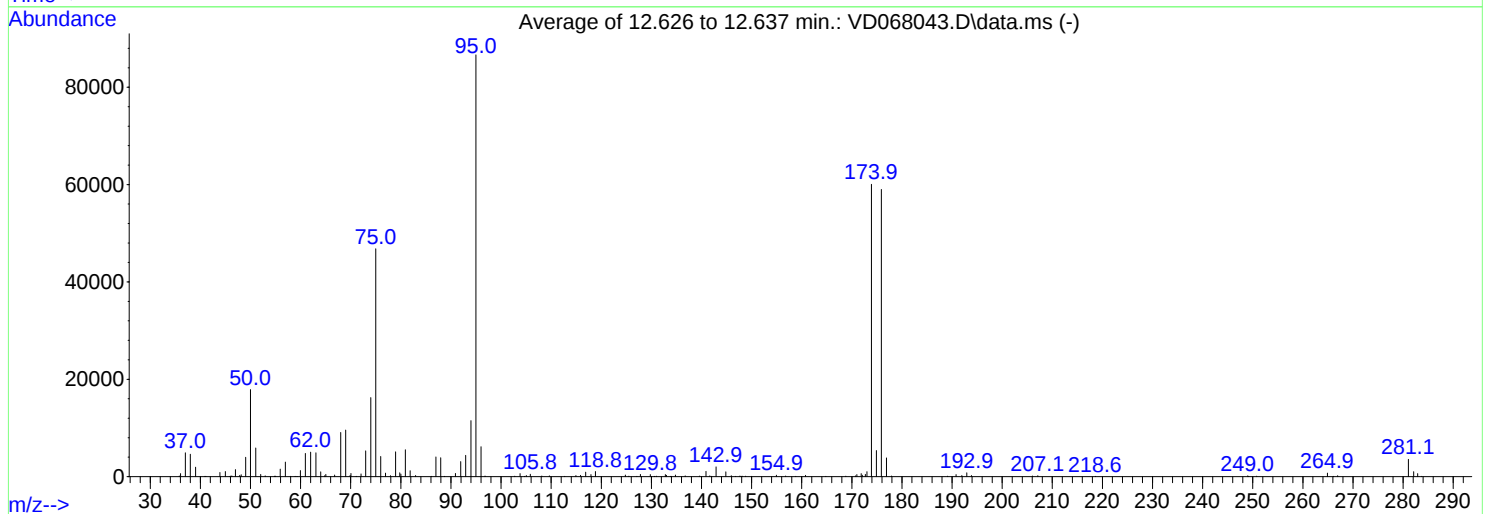


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD010821\
Data File : VD068043.D
Acq On : 08 Jan 2021 12:14
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
Title : SW846 8260
Last Update : Wed Dec 23 07:34:16 2020

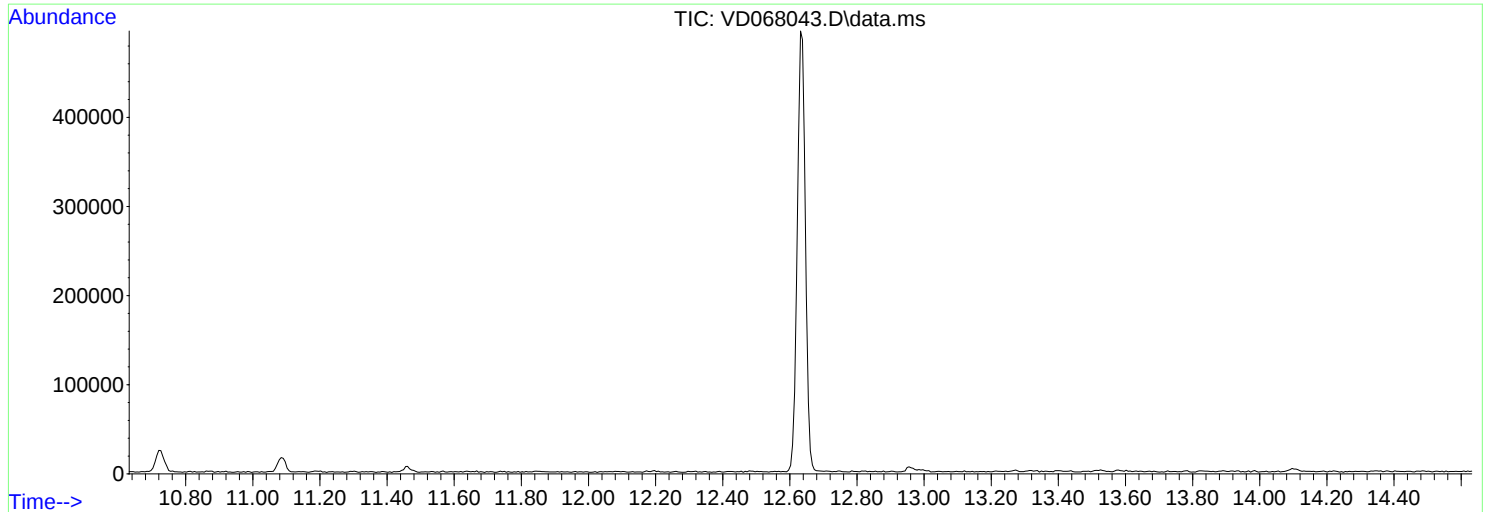

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	17885	PASS
75	95	30	60	54.0	46816	PASS
95	95	100	100	100.0	86653	PASS
96	95	5	9	7.1	6148	PASS
173	174	0.00	2	1.7	1006	PASS
174	95	50	100	69.3	60067	PASS
175	174	5	9	8.9	5367	PASS
176	174	95	101	98.2	58992	PASS
177	176	5	9	6.5	3845	PASS