

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD010920\
 Data File : VD064825.D
 Acq On : 09 Jan 2020 19:22
 Operator : VA/SY
 Sample : L1064-01
 Misc : 7.54G/5.00ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Jan 10 05:43:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 24 13:19:06 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	507362	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	774061	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	685399	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	318028	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	209169	46.75	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.50%	
35) Dibromofluoromethane	7.91	113	230545	48.55	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.10%	
50) Toluene-d8	10.34	98	937062	51.52	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.04%	
62) 4-Bromofluorobenzene	12.64	95	280407	48.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.52%	
Target Compounds						
16) Acetone	4.16	43	1452	5.548	ug/l #	88
20) Methylene Chloride	4.95	84	21148	Below Cal		89
31) Cyclohexane	7.98	56	14592	1.749	ug/l #	46
76) 1,2,3-Trichloropropane	12.64	75	147623	58.782	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.64	75	147623	122.942	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD010920\
Data File : VD064825.D
Acq On : 09 Jan 2020 19:22
Operator : VA/SY
Sample : L1064-01
Misc : 7.54G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Jan 10 05:43:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 24 13:19:06 2019
Response via : Initial Calibration

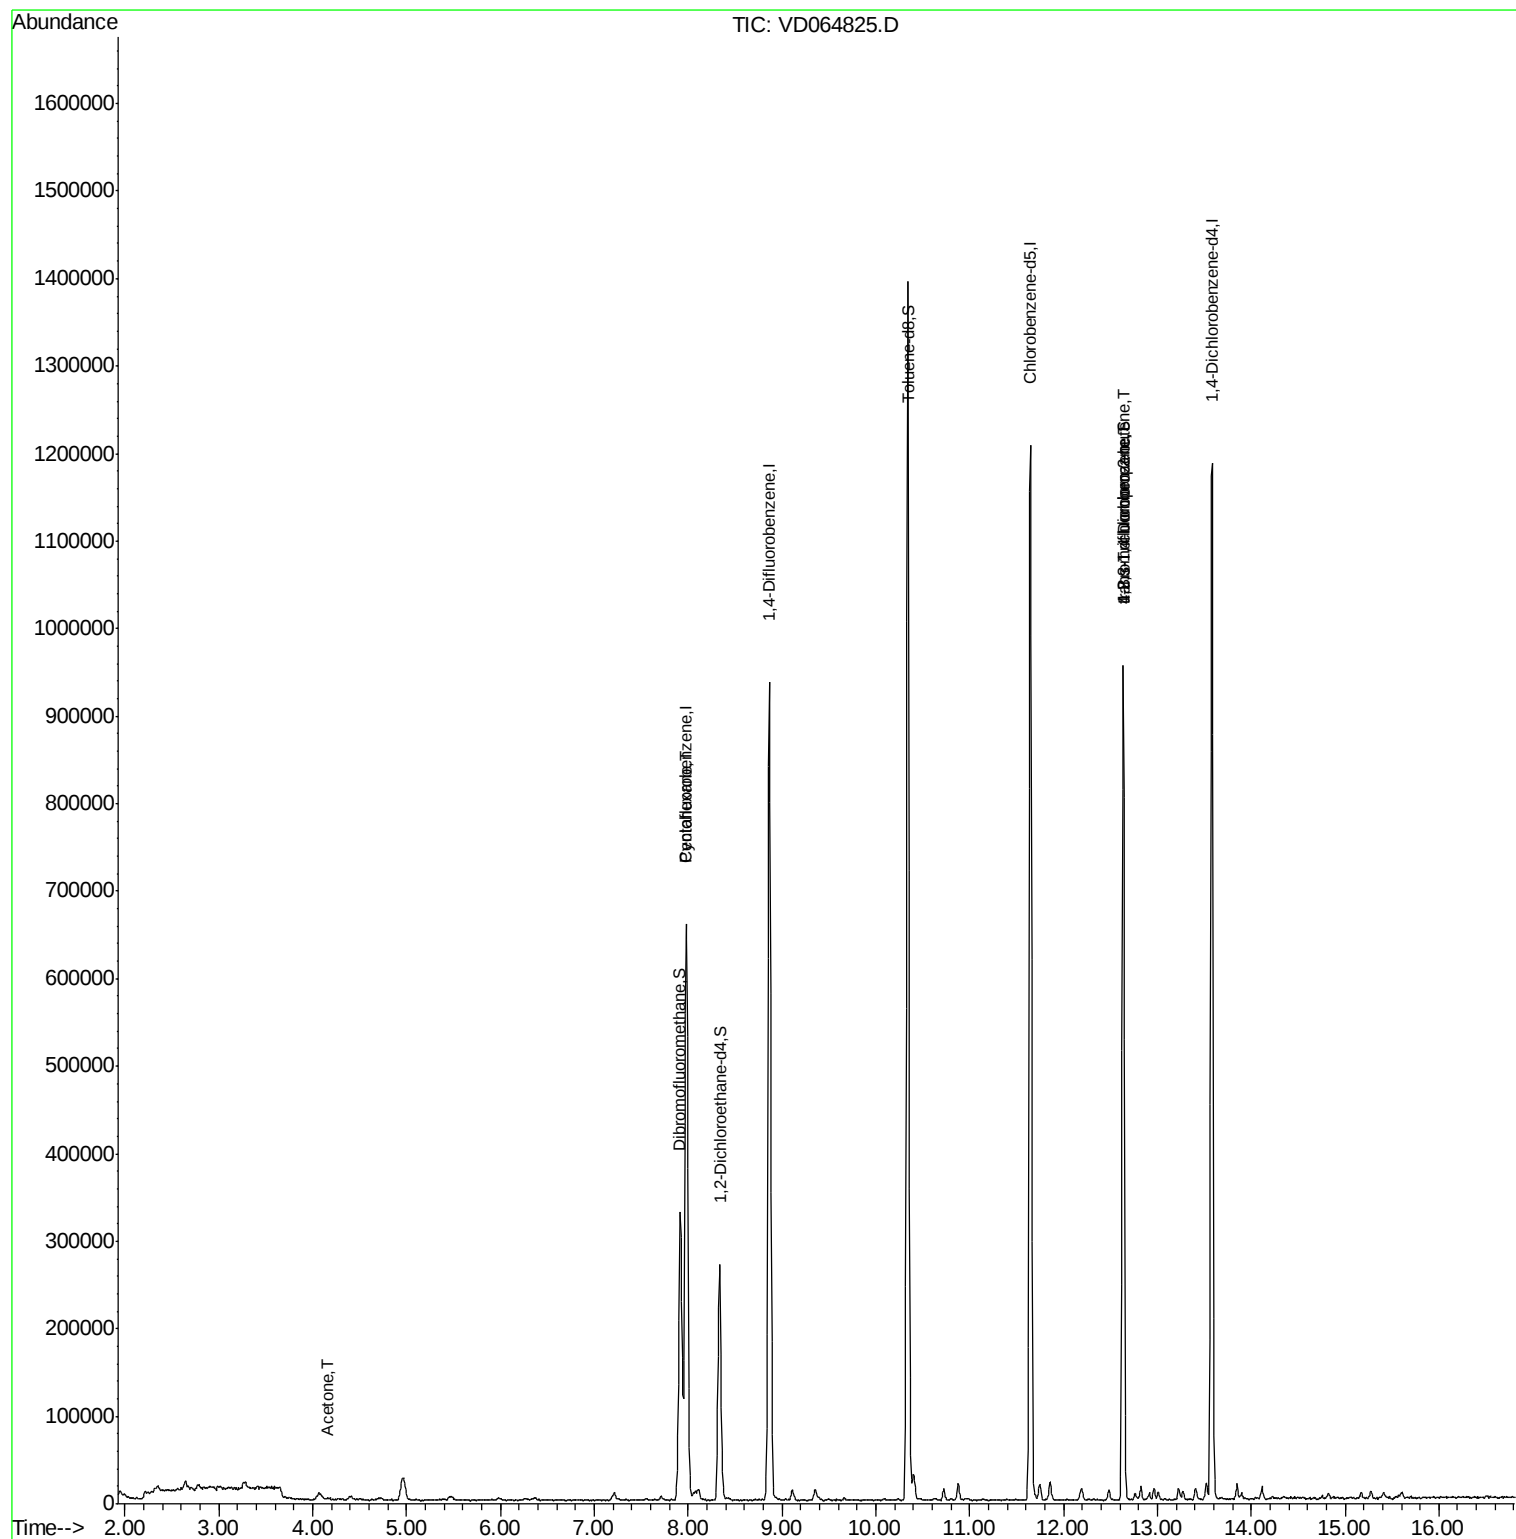



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1031

Delta R.T. 0.00 min

Lab File: VD064825.D

Acq: 09 Jan 2020 19:22


Instrument :
MSVOA_D
ClientSampleId :

Tot Ion:168 Resp: 507362

Ion Ratio Lower Upper

168 100

99 51.0 41.8 62.6

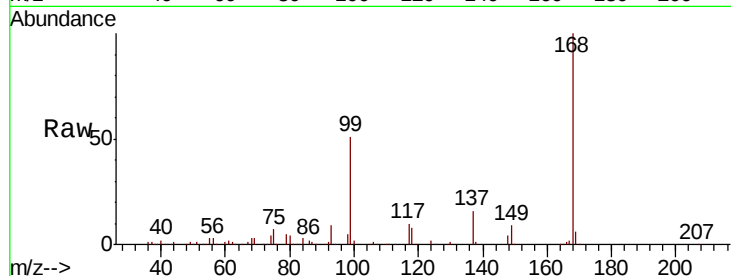

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

250000

200000



150000

100000

50000

0

Time-->



#16

Acetone

Concen: 5.548 ug/l

RT: 4.16 min Scan# 380

Delta R.T. -0.01 min

Lab File: VD064825.D


Acq: 09 Jan 2020 19:22

Tgt Ion: 43 Resp: 1452

Ion Ratio Lower Upper

43 100

58 39.0 25.8 38.6#



Abundance Ion 43.00 (42.70 to 43.70): VDC

Ion 58.00 (57.70 to 58.70): VDC

4.16

1200

1000

800


600


400

200

0

Time-->









#31
Cyclohexane
Concen: 1.749 ug/l
RT: 7.98 min Scan# 1030
Delta R.T. -0.01 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22

Instrument :
MSVOA_D
ClientSampleId :

Tot Ion: 56 Resp: 14592
Ion Ratio Lower Upper
56 100
69 118.1 24.7 37.1#
84 102.5 69.4 104.2

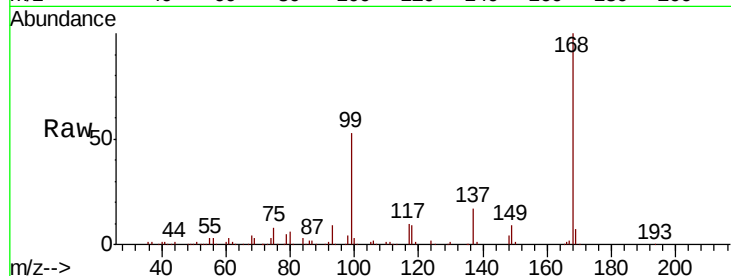


Abundance Ion 56.00 (55.70 to 56.70): VDC
Ion 69.00 (68.70 to 69.70): VDC
Ion 84.00 (83.70 to 84.70): VDC


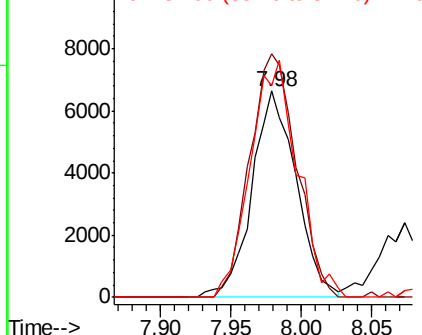



#33
1,2-Dichloroethane-d4
Concen: 46.754 ug/l
RT: 8.33 min Scan# 1090
Delta R.T. 0.00 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22

Tgt Ion: 65 Resp: 209169
Ion Ratio Lower Upper
65 100
67 51.9 0.0 106.2



Abundance Ion 64.90 (64.60 to 65.60): VDC
Ion 66.90 (66.60 to 67.60): VDC

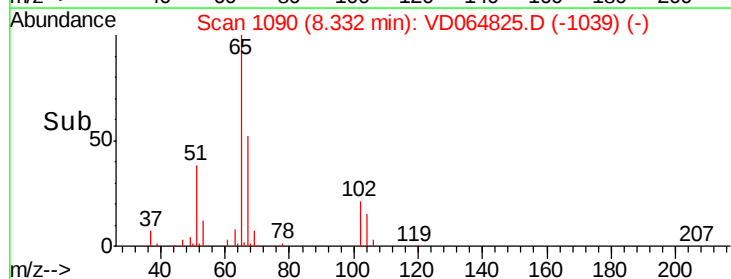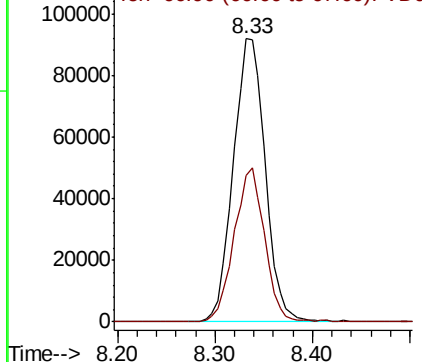

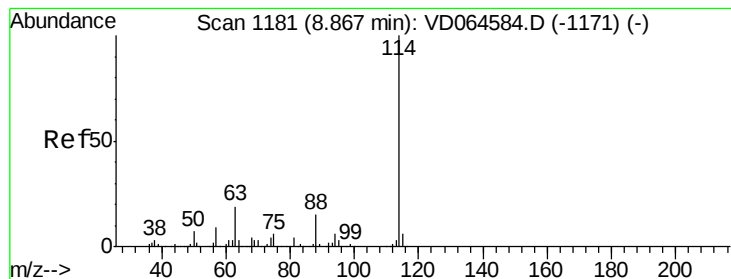

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD064825.D

Acq: 09 Jan 2020 19:22

Instrument :

MSVOA_D

ClientSampleId :


Tot Ion:114 Resp: 774061

Ion Ratio Lower Upper

114 100

63 20.0 0.0 38.0




88 14.4 0.0 29.2



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

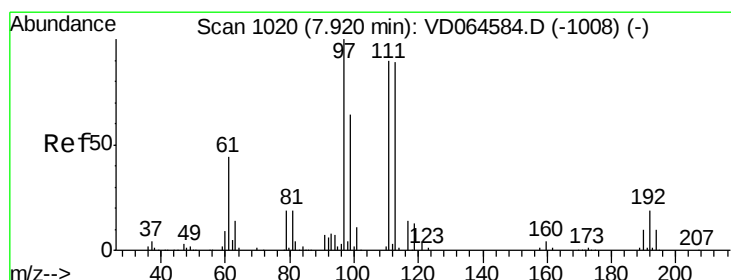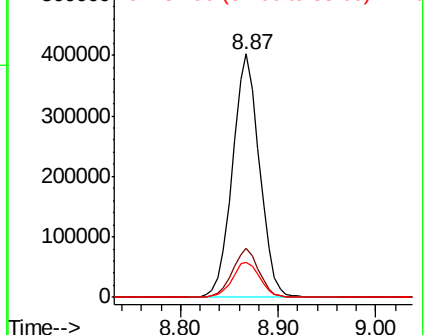

#35

Dibromofluoromethane

Concen: 48.546 ug/l

RT: 7.91 min Scan# 1019

Delta R.T. -0.01 min

Lab File: VD064825.D

Acq: 09 Jan 2020 19:22


Tgt Ion:113 Resp: 230545

Ion Ratio Lower Upper

113 100

111 102.8 80.6 121.0



192 22.0 17.9 26.9




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




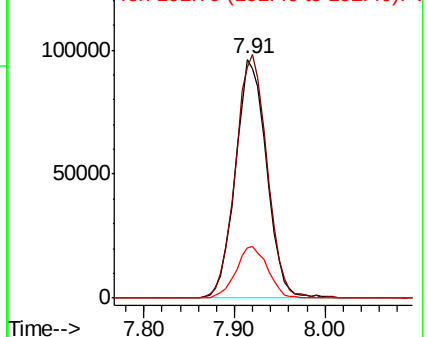


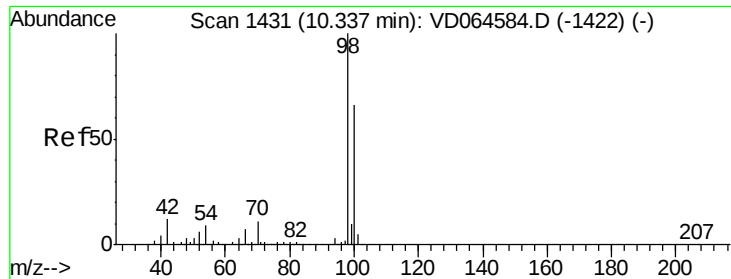

#50
Toluene-d8
Concen: 51.520 ug/l
RT: 10.34 min Scan# 1432
Delta R.T. 0.01 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22




Instrument :
MSVOA_D
ClientSampleId :


Tot Ion: 98 Resp: 937062
Ion Ratio Lower Upper
98 100
100 65.3 51.7 77.5

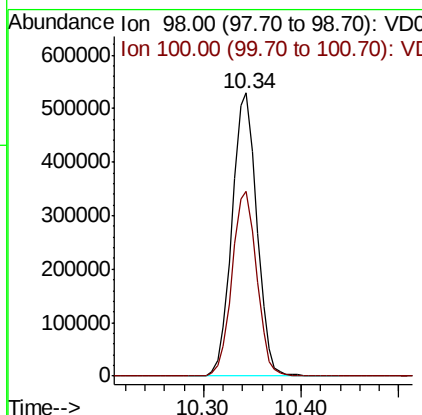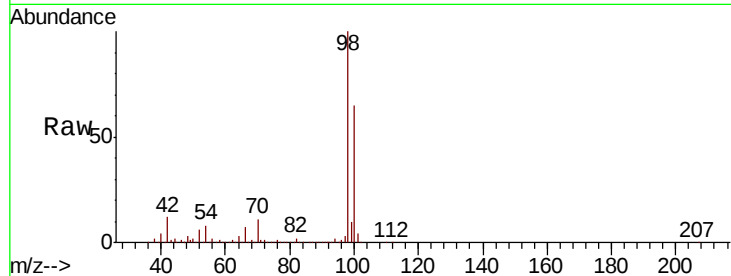

#62
4-Bromofluorobenzene
Concen: 48.756 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22

Tgt Ion: 95 Resp: 280407
Ion Ratio Lower Upper
95 100
174 91.1 0.0 193.2
176 90.4 0.0 184.2


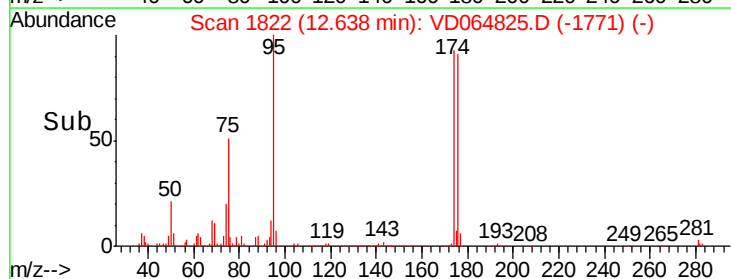
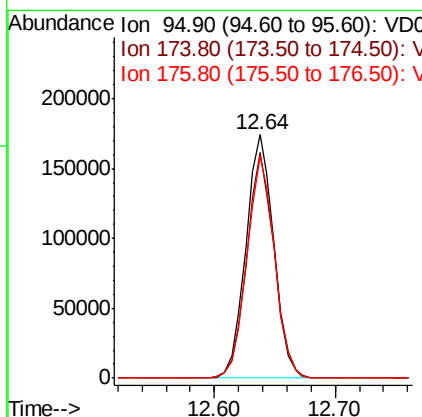



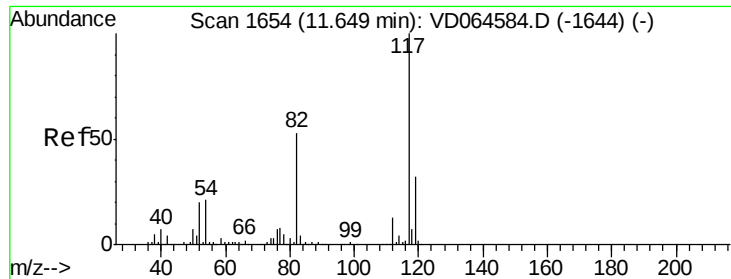

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.65 min Scan# 1654
Delta R.T. 0.00 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22




Instrument :
MSVOA_D
ClientSampleId :


Tot Ion:117 Resp: 685399
Ion Ratio Lower Upper
117 100
82 51.2 42.2 63.4
119 32.2 26.0 39.0

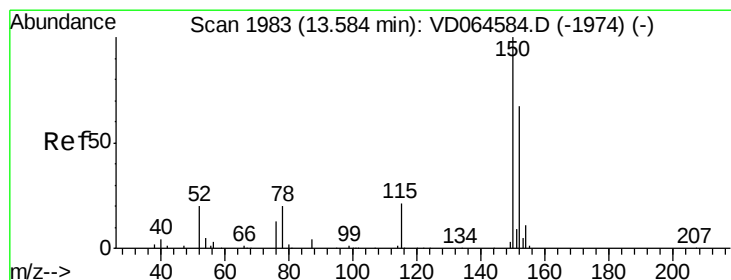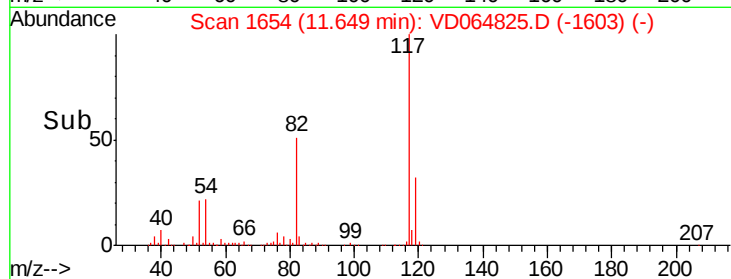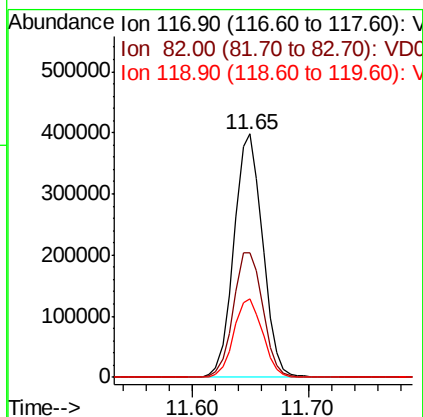

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD064825.D
Acq: 09 Jan 2020 19:22

Tgt Ion:152 Resp: 318028
Ion Ratio Lower Upper
152 100
115 54.5 27.8 83.4
150 158.1 0.0 351.4

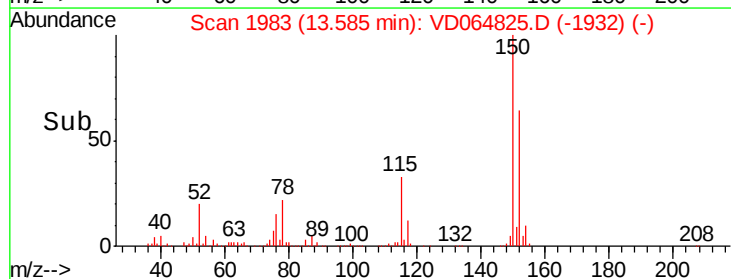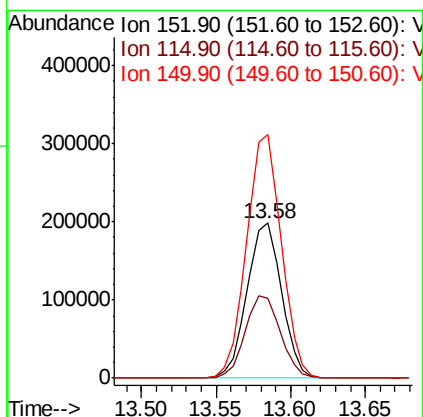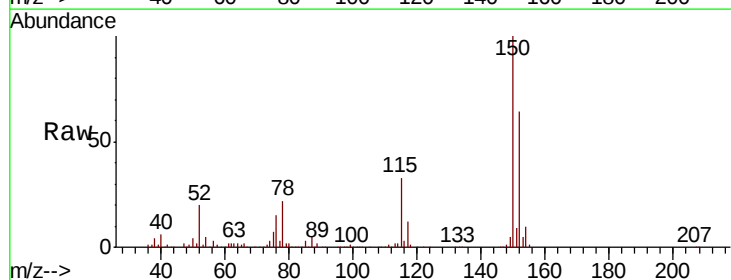



#76

1,2,3-Trichloropropane

Concen: 58.782 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. -0.15 min

Lab File: VD064825.D

Acq: 09 Jan 2020 19:22

Instrument :

MSVOA_D


ClientSampleId :

Tot Ion: 75 Resp: 147623

Ion Ratio Lower Upper




75 100

77 1.4 0.0 0.0#

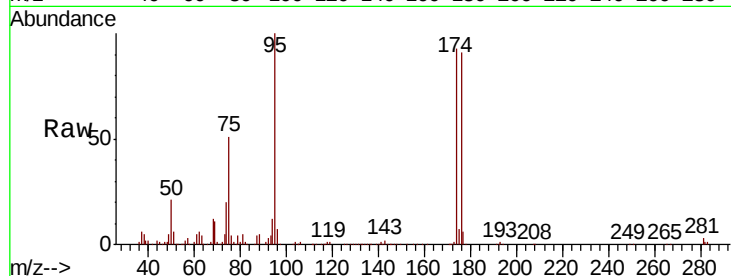

Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 77.00 (76.70 to 77.70): VDC

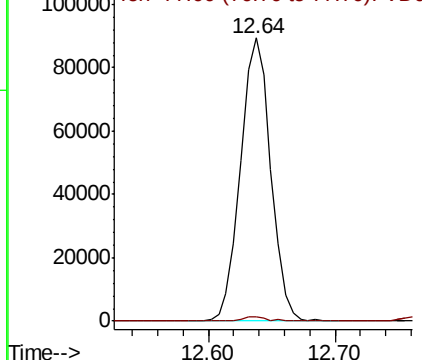

#81

trans-1,4-Dichloro-2-butene

Concen: 122.942 ug/l

RT: 12.64 min Scan# 1822

Delta R.T. 0.11 min

Lab File: VD064825.D

Acq: 09 Jan 2020 19:22


Tgt Ion: 75 Resp: 147623

Ion Ratio Lower Upper

75 100

53 0.1 78.8 118.2#

89 0.0 38.3 57.5#



Abundance Ion 74.90 (74.60 to 75.60): VDC

Ion 53.00 (52.70 to 53.70): VDC

