

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD011020\
 Data File : VD064837.D
 Acq On : 10 Jan 2020 17:06
 Operator : VA/SY
 Sample : L1063-04RE
 Misc : 7.52G/5.00ml/MSVOA D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 WP022SB452_200108_25-27RE

Quant Time: Jan 10 22:27:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 24 13:19:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.98
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.87
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.65
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.58

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD011020\
Data File : VD064837.D
Acq On : 10 Jan 2020 17:06
Operator : VA/SY
Sample : L1063-04RE
Misc : 7.52G/5.00ml/MSVOA D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
WP022SB452_200108_25-27RE

Quant Time: Jan 10 22:27:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 24 13:19:06 2019
Response via : Initial Calibration

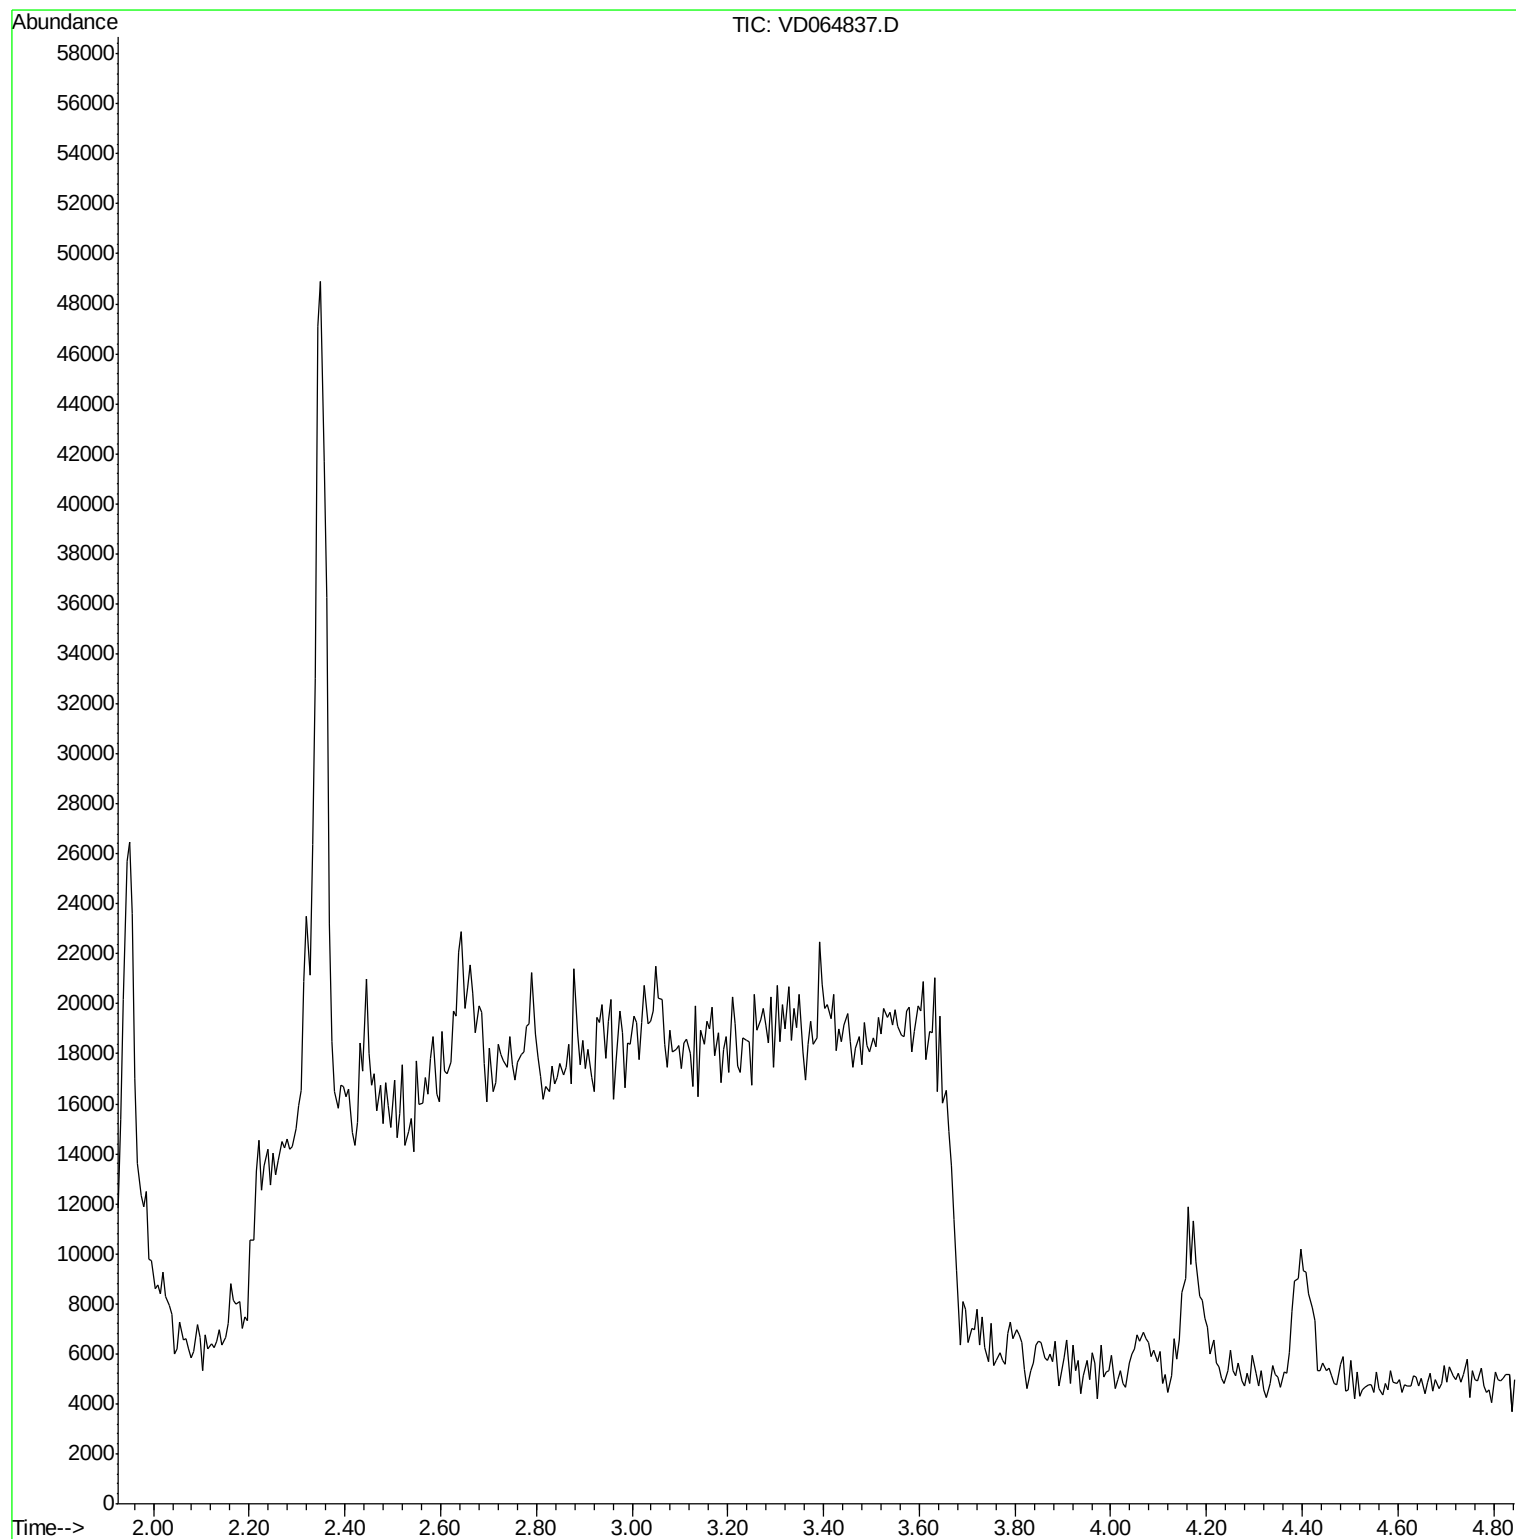


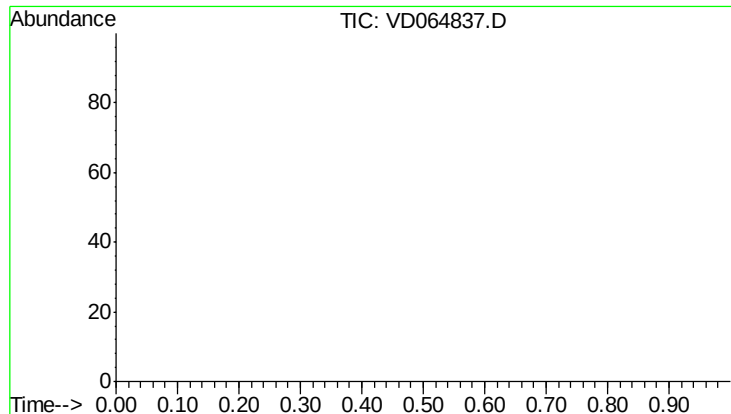


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.98 min

Lab File: VD064837.D
Acq: 10 Jan 2020 17:06

Instrument :
MSVOA_D
ClientSampleId :
WP022SB452_200108_25-27RE


Tot Ion	168
Sig	Exp Ratio
168	100
99	52.2

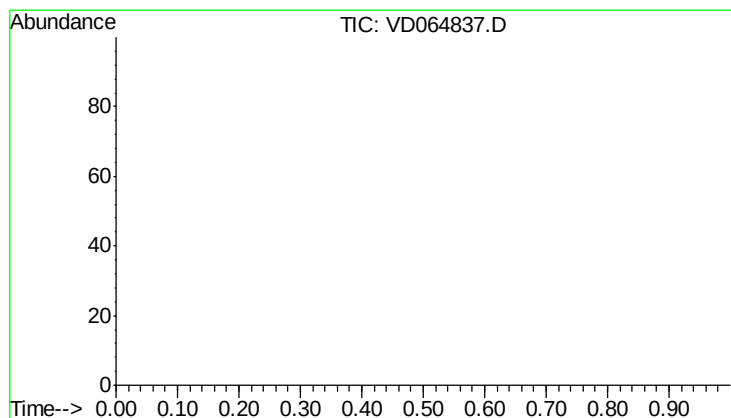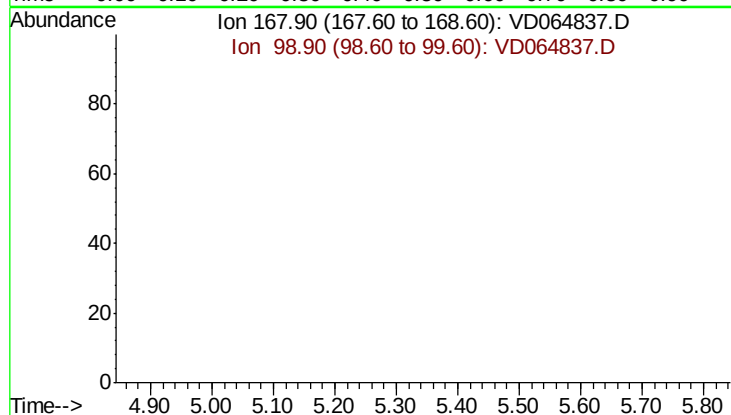


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.33 min

Lab File: VD064837.D
Acq: 10 Jan 2020 17:06

Tgt Ion	65
Sig	Exp Ratio
65	100
67	53.1


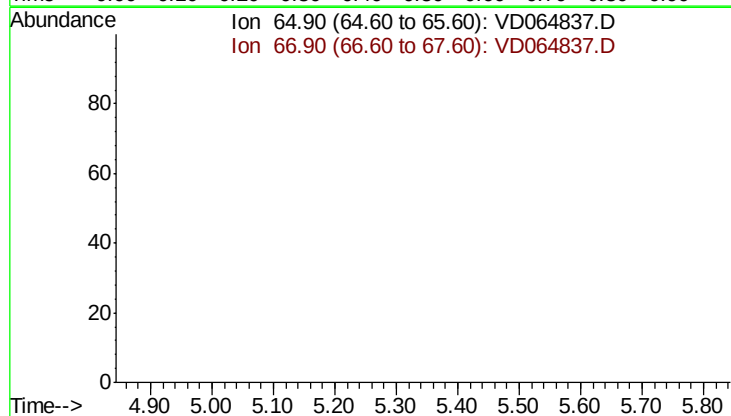


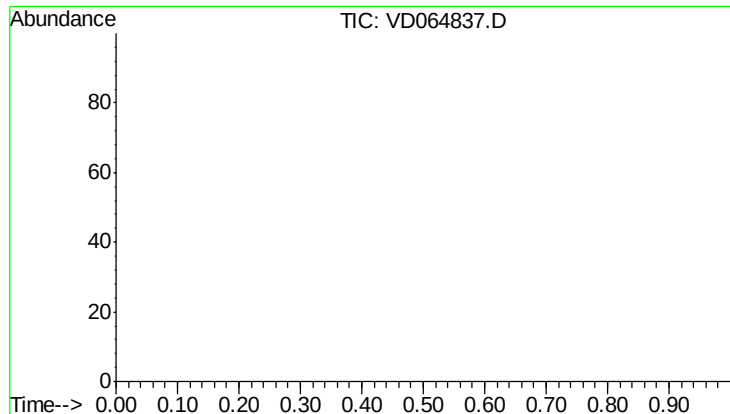

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.87 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06


Instrument :
 MSVOA_D
 ClientSampleId :
 WP022SB452_200108_25-27RE


Tot Ion	Exp Ratio
114	100
63	19.0
88	14.6

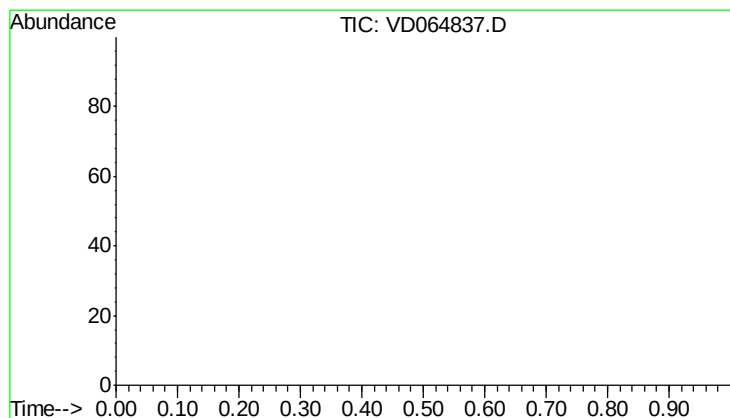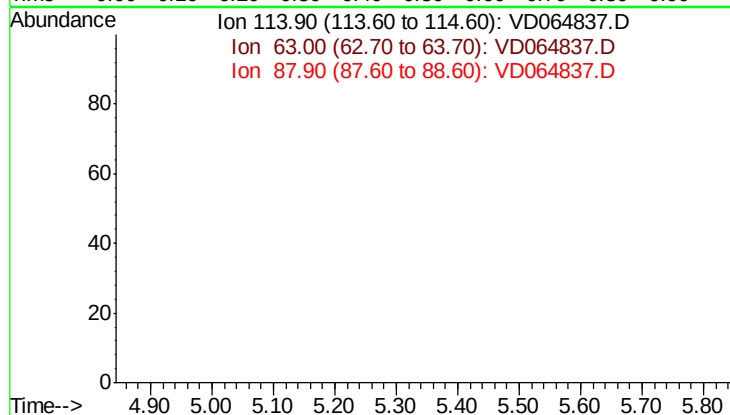

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.92 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06

Tgt Ion	Exp Ratio
113	100
111	100.8
192	22.4


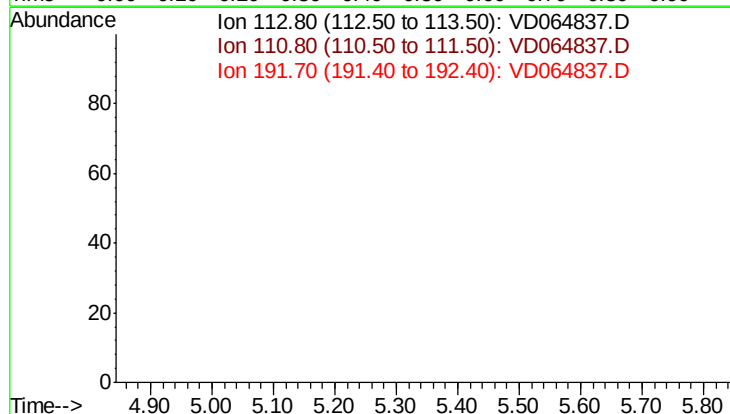


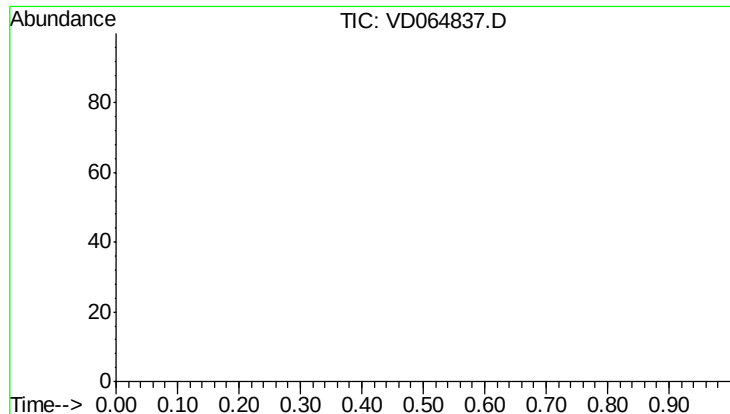

#50
 Toluene-d8
 Concen: 0.000 ug/l
 Expected RT: 10.34 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06


Instrument :
 MSVOA_D
 ClientSampleId :
 WP022SB452_200108_25-27RE


Tot Ion	Sig	Exp Ratio
98	100	
100	64.6	

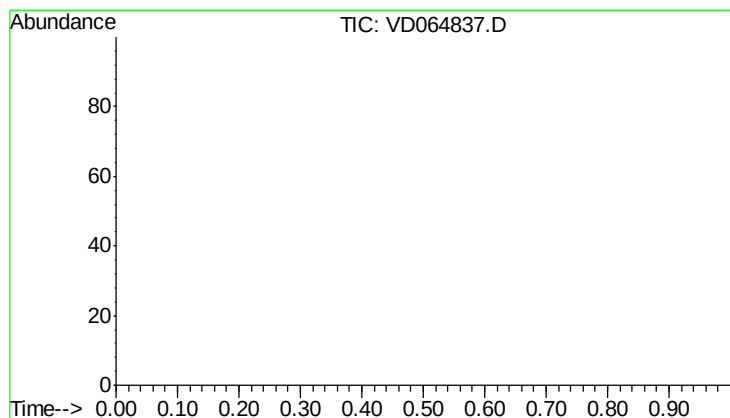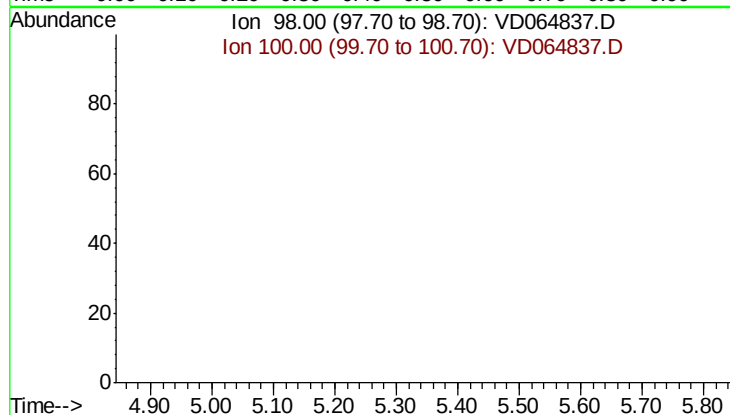

#62
 4-Bromofluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 12.64 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06

Tgt Ion	Sig	Exp Ratio
95	100	
174	96.6	
176	92.1	


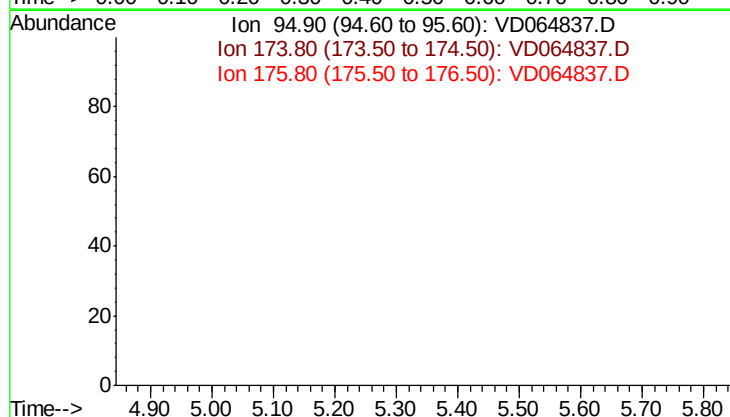


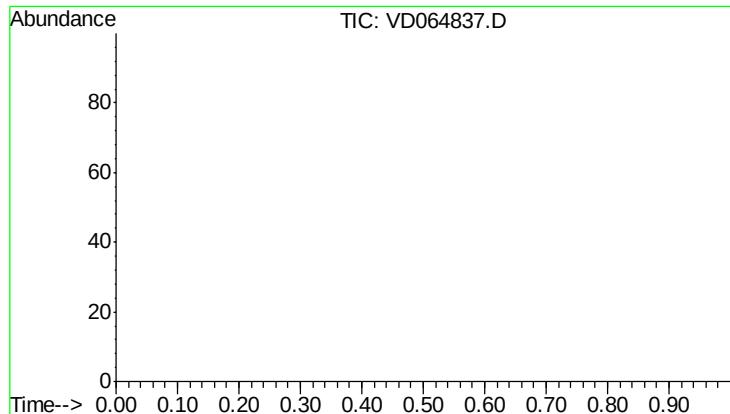

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.65 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06

Instrument :
 MSVOA_D
 ClientSampleId :
 WP022SB452_200108_25-27RE

Tot Ion	Sig	Exp Ratio
117	100	
82	52.8	
119	32.5	

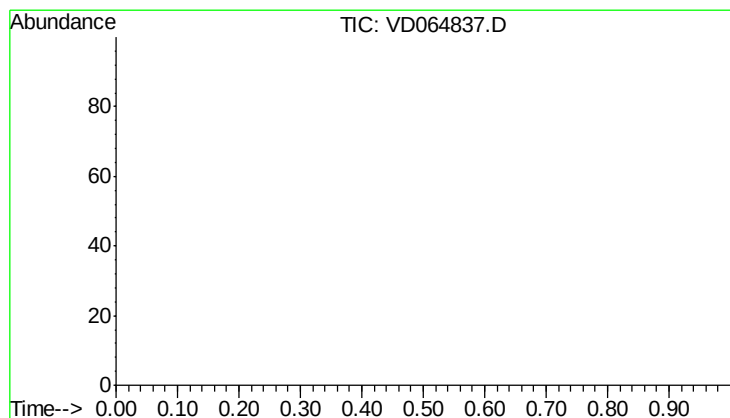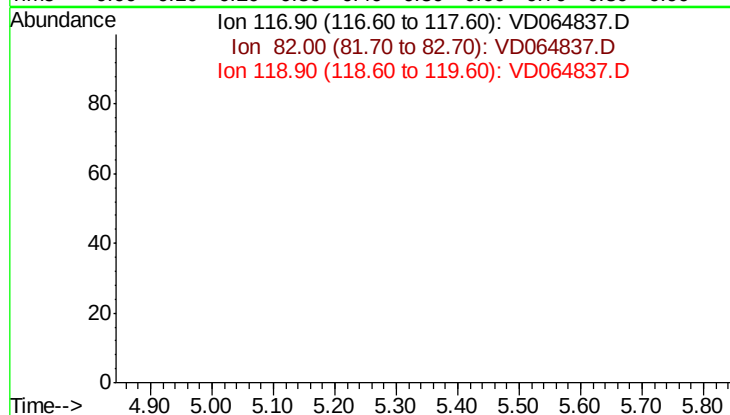

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.58 min
 Lab File: VD064837.D
 Acq: 10 Jan 2020 17:06

Tgt Ion	Sig	Exp Ratio
152	100	
115	55.6	
150	175.7	

