


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD011020\
Data File : VD064830.D
Acq On : 10 Jan 2020 12:46
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Title : SW846 8260
Last Update : Tue Dec 24 13:19:06 2019

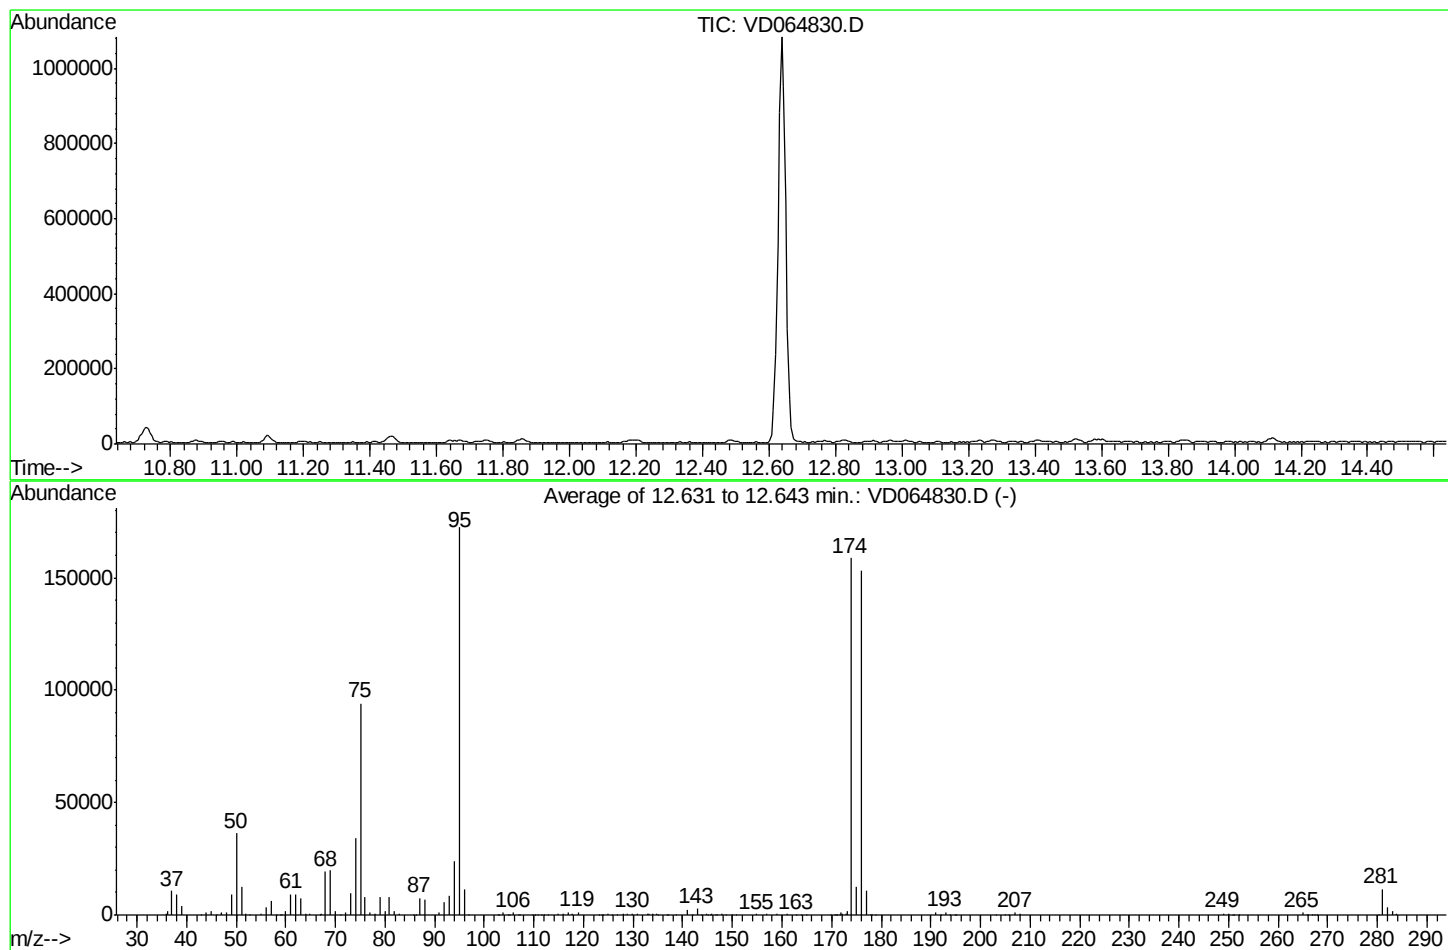

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	36266	PASS
75	95	30	60	54.5	93976	PASS
95	95	100	100	100.0	172437	PASS
96	95	5	9	6.6	11339	PASS
173	174	0.00	2	1.2	1868	PASS
174	95	50	100	92.0	158677	PASS
175	174	5	9	7.8	12340	PASS
176	174	95	101	96.5	153194	PASS
177	176	5	9	7.2	11035	PASS