

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011524\
 Data File : VD078160.D
 Acq On : 15 Jan 2024 13:29
 Operator : RP/MD
 Sample : P1139-01
 Misc : 5.42G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 MR-314-0-2

Quant Time: Jan 16 00:35:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D010824S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 09 01:29:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	125995	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.781	114	253972	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.580	117	233748	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.521	152	75277	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.233	65	60245	45.418	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	90.840%
35) Dibromofluoromethane	7.810	113	79205	43.273	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	86.540%
50) Toluene-d8	10.269	98	321427	52.362	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	104.720%
62) 4-Bromofluorobenzene	12.574	95	78971	36.956	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	73.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011524\
Data File : VD078160.D
Acq On : 15 Jan 2024 13:29
Operator : RP/MD
Sample : P1139-01
Misc : 5.42G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
MR-314-0-2

Quant Time: Jan 16 00:35:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D010824S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 09 01:29:14 2024
Response via : Initial Calibration




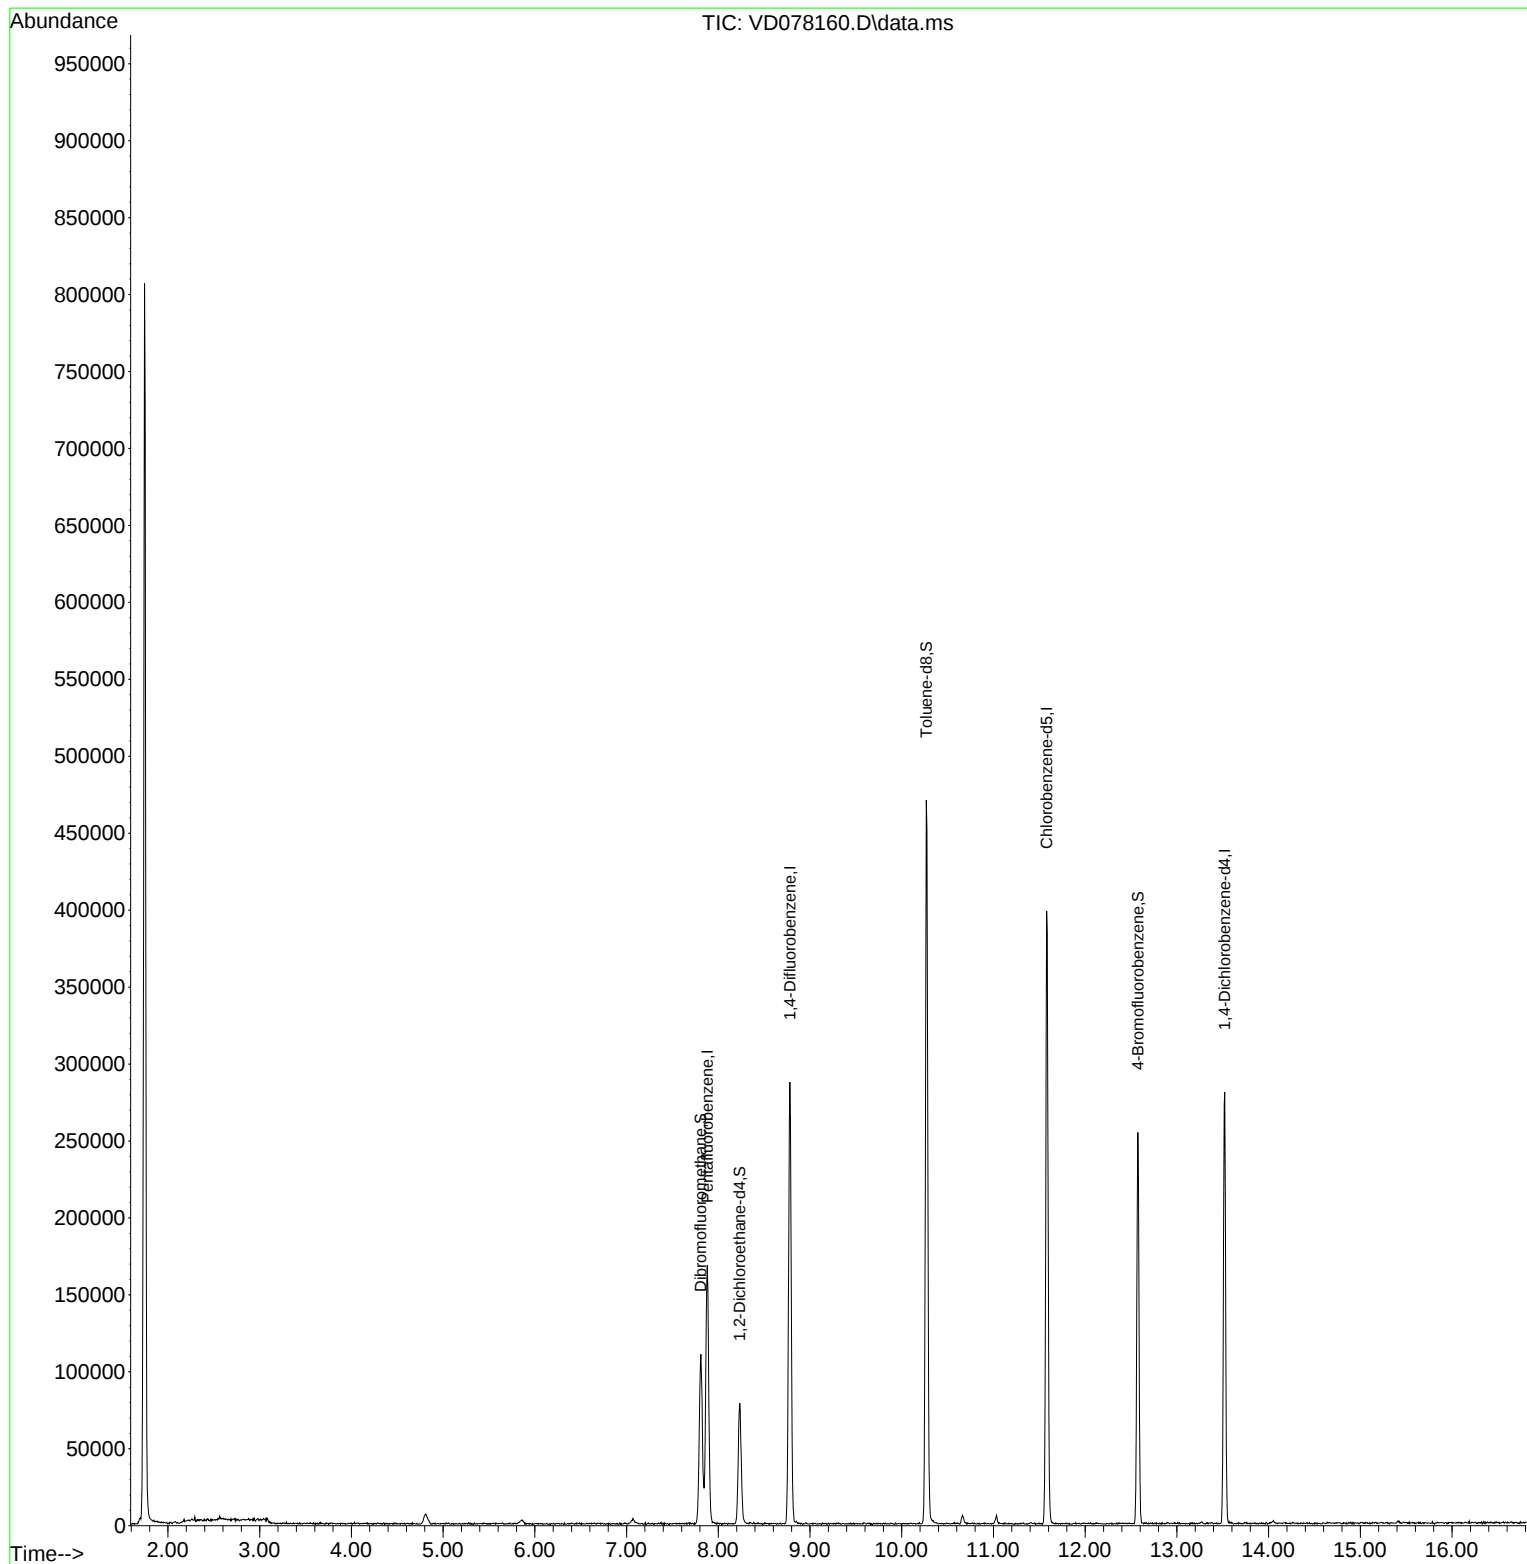


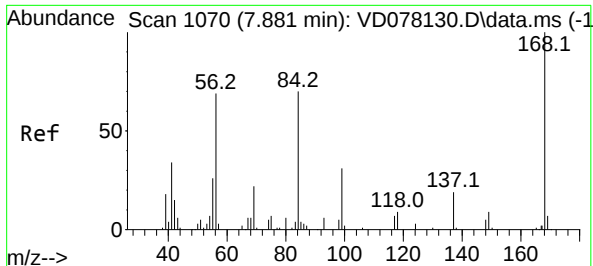

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29




Instrument :
MSVOA_D
ClientSampleId :
MR-314-0-2


Tgt Ion:168 Resp: 125995
Ion Ratio Lower Upper
168 100
99 56.3 36.7 55.1#

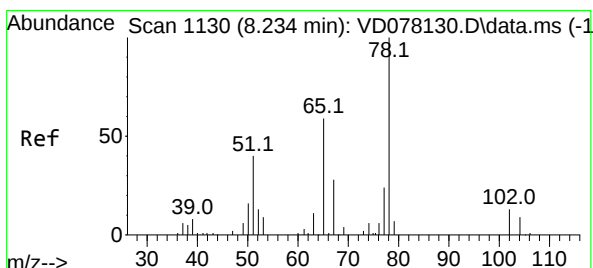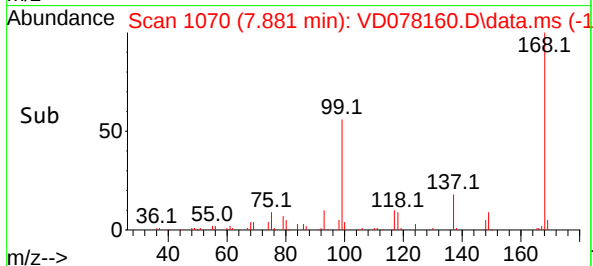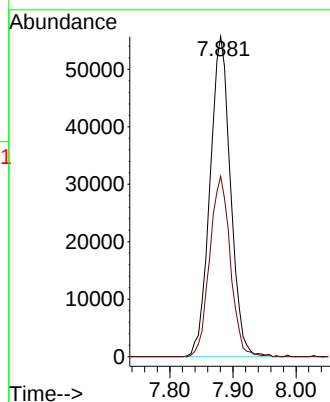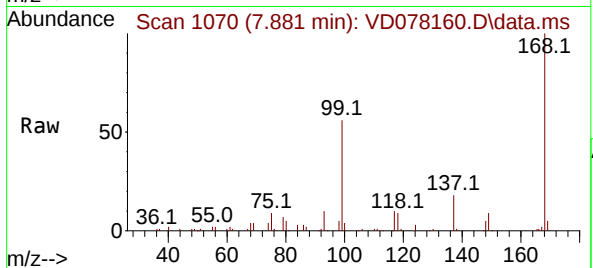

#33
1,2-Dichloroethane-d4
Concen: 45.418 ug/l
RT: 8.233 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29

Tgt Ion: 65 Resp: 60245
Ion Ratio Lower Upper
65 100
67 54.9 0.0 115.0

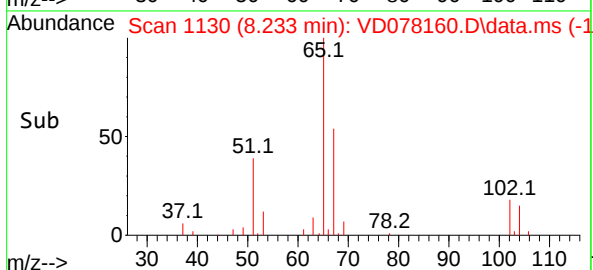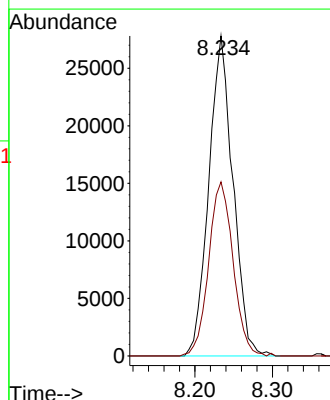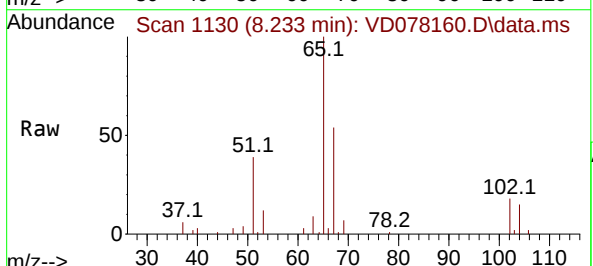

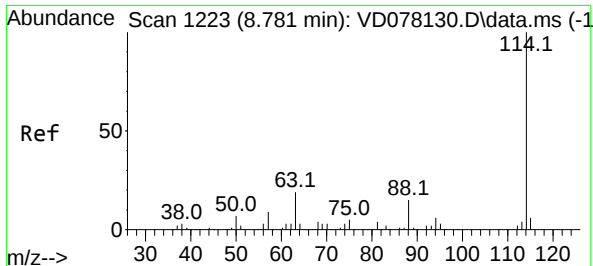

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD078160.D

Acq: 15 Jan 2024 13:29

Instrument :

MSVOA_D

ClientSampleId :

MR-314-0-2





Tgt Ion:114 Resp: 253972

Ion Ratio Lower Upper

114 100

63 18.5 0.0 33.4

88 13.8 0.0 26.2

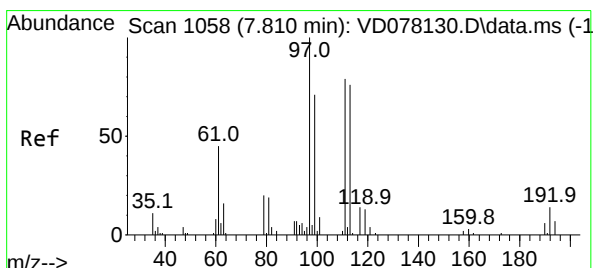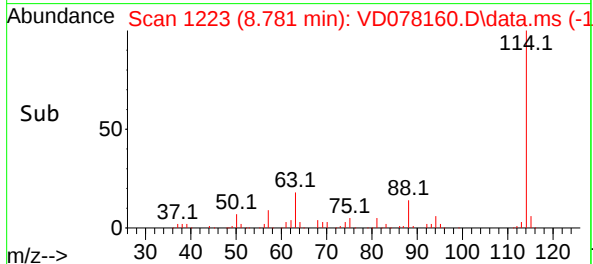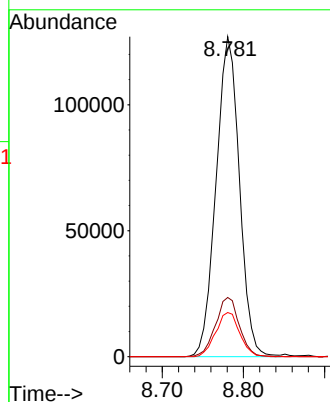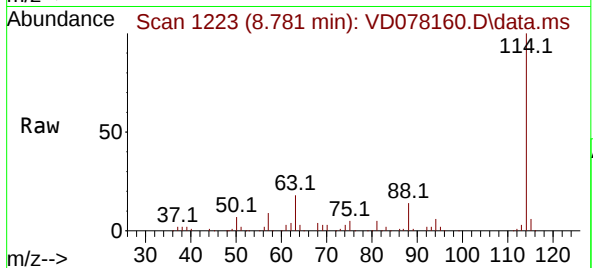

#35

Dibromofluoromethane

Concen: 43.273 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VD078160.D

Acq: 15 Jan 2024 13:29




Tgt Ion:113 Resp: 79205


Ion Ratio Lower Upper

113 100

111 103.2 84.7 127.1

192 17.5 16.8 25.2


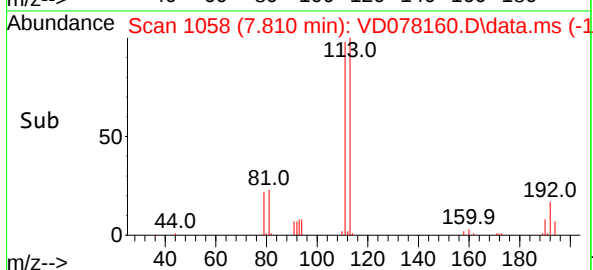
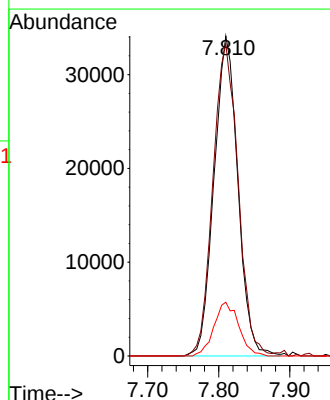
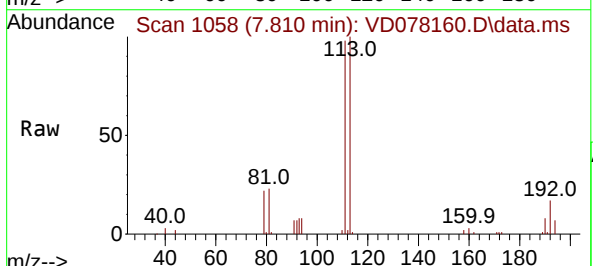


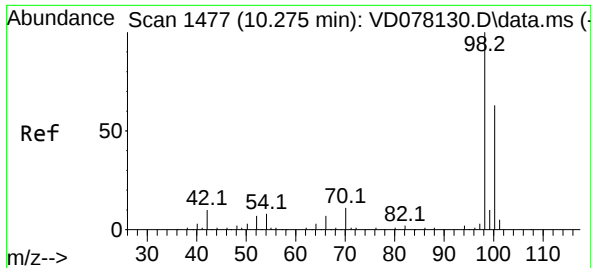

#50
Toluene-d8
Concen: 52.362 ug/l
RT: 10.269 min Scan# 1477
Delta R.T. -0.006 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29




Instrument :
MSVOA_D
ClientSampleId :
MR-314-0-2


Tgt Ion: 98 Resp: 321427
Ion Ratio Lower Upper
98 100
100 65.5 50.3 75.5

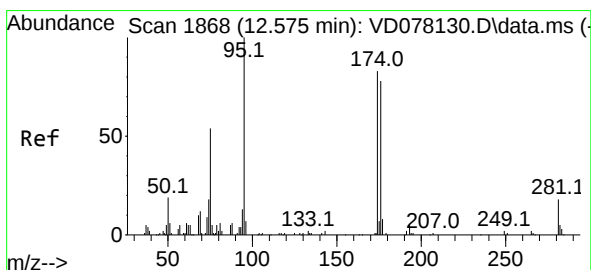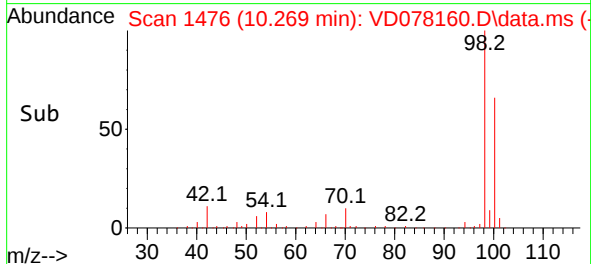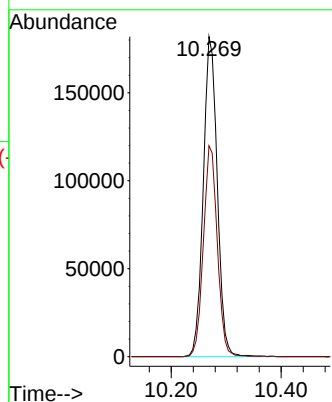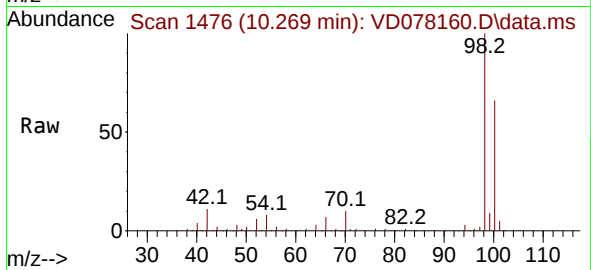

#62
4-Bromofluorobenzene
Concen: 36.956 ug/l
RT: 12.574 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29

Tgt Ion: 95 Resp: 78971
Ion Ratio Lower Upper
95 100
174 84.0 0.0 201.8
176 79.9 0.0 191.8


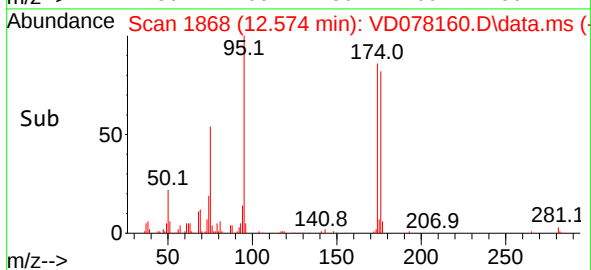
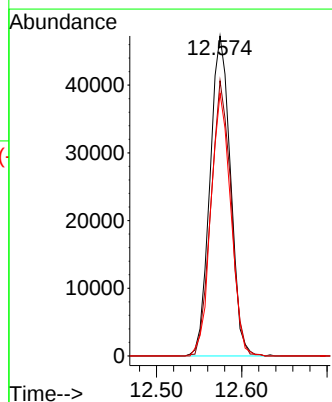
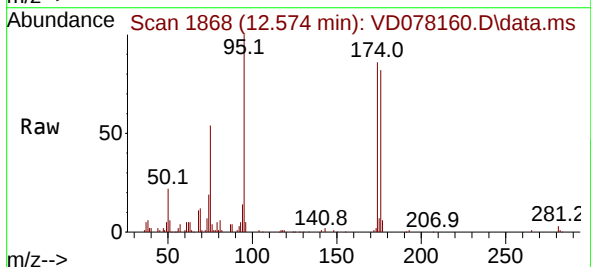


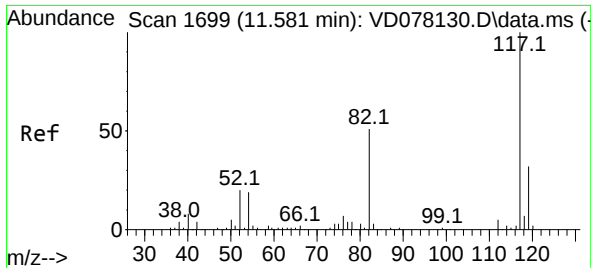

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.580 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29

Instrument :
MSVOA_D
ClientSampleId :
MR-314-0-2

Tgt Ion:117 Resp: 233748
Ion Ratio Lower Upper
117 100
82 54.0 38.3 57.5
119 31.5 25.0 37.4

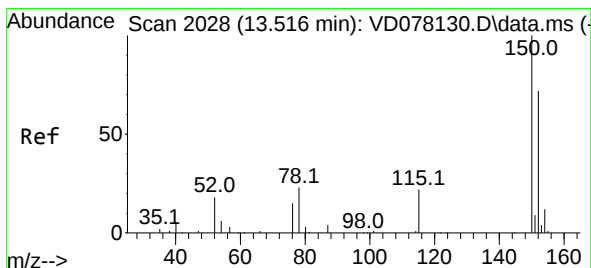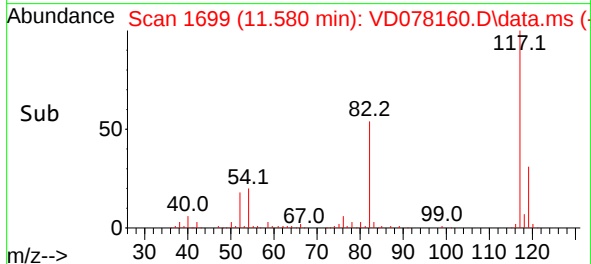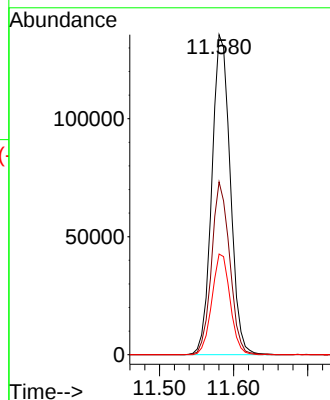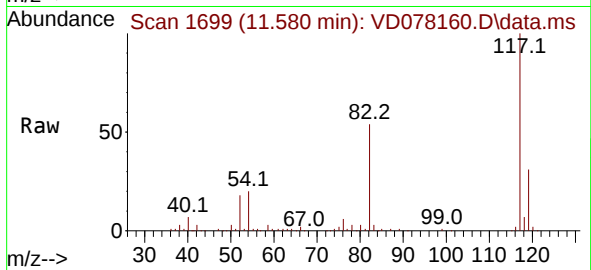

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.521 min Scan# 2029
Delta R.T. 0.005 min
Lab File: VD078160.D
Acq: 15 Jan 2024 13:29

Tgt Ion:152 Resp: 75277
Ion Ratio Lower Upper
152 100
115 55.8 27.1 81.3
150 158.6 0.0 353.6

