
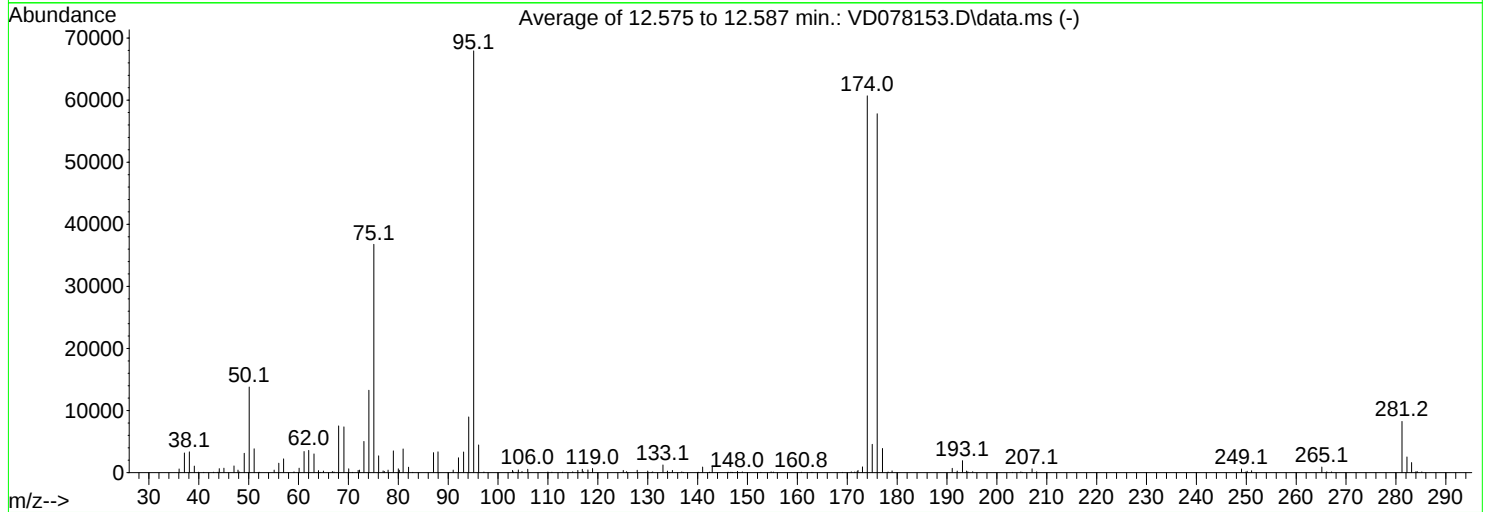


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011524\
Data File : VD078153.D
Acq On : 15 Jan 2024 08:47
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D0108245.M
Title : SW846 8260
Last Update : Tue Jan 09 01:29:14 2024

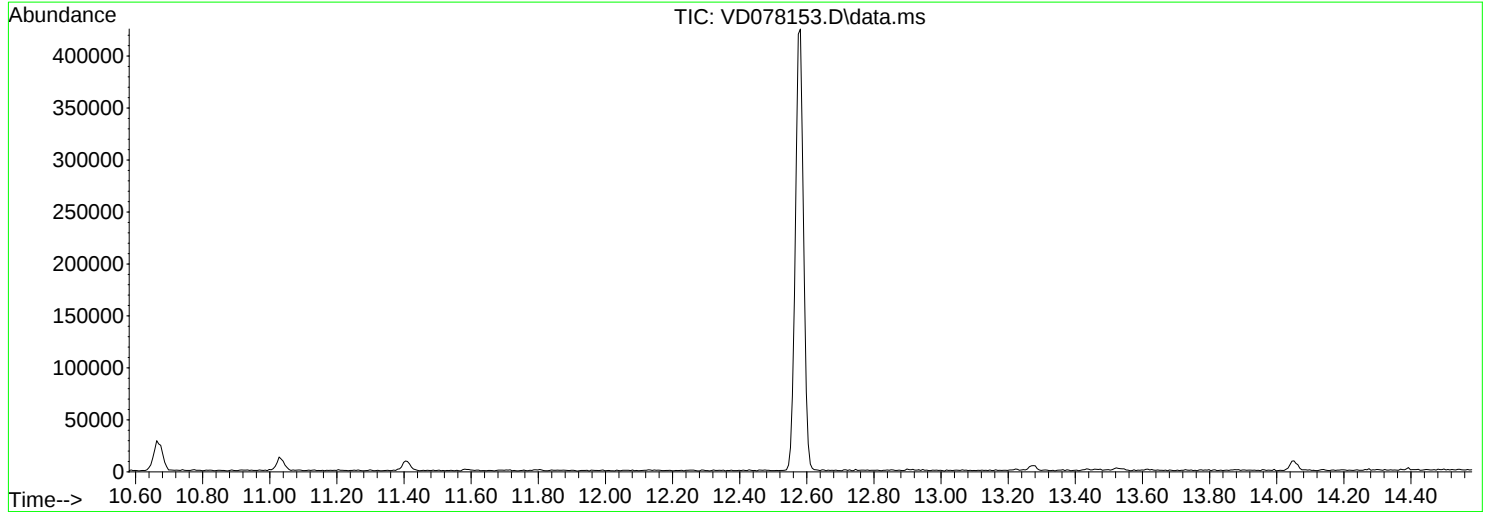

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	13780	PASS
75	95	30	60	54.1	36773	PASS
95	95	100	100	100.0	67941	PASS
96	95	5	9	6.6	4472	PASS
173	174	0.00	2	1.5	935	PASS
174	95	50	100	89.4	60707	PASS
175	174	5	9	7.5	4575	PASS
176	174	95	101	95.2	57819	PASS
177	176	5	9	6.7	3882	PASS