


Methylene Chloride

Response Ratio

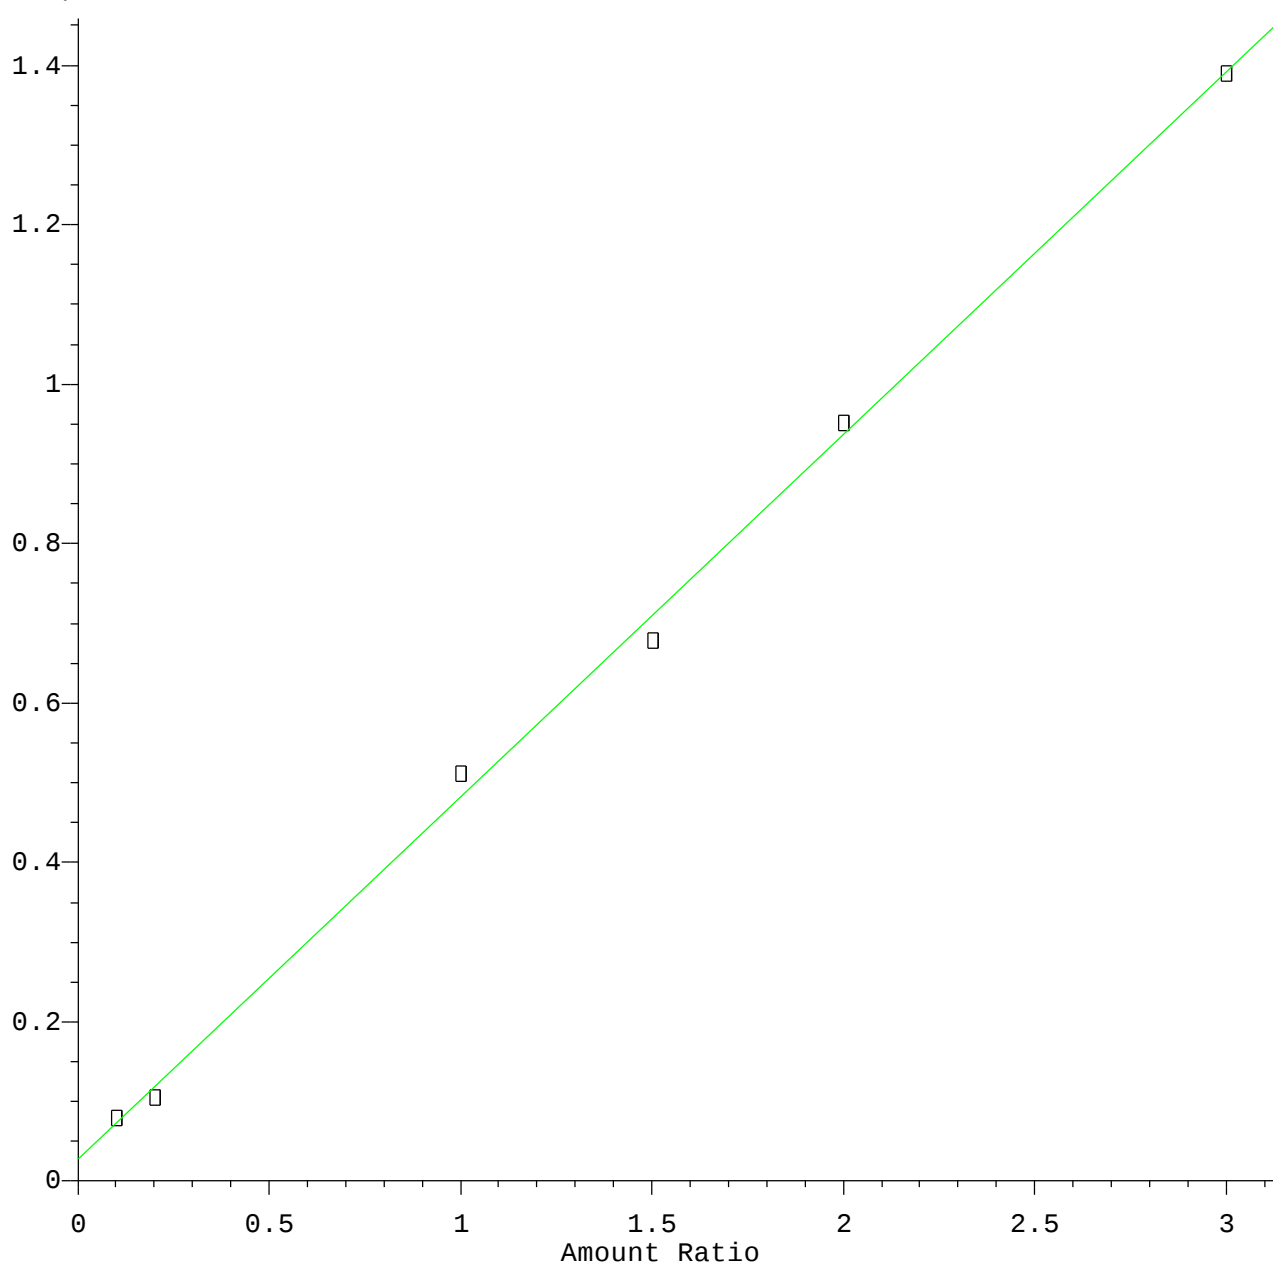


Resp Ratio = 4.54e-001 * Amt + 2.81e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D011819S.M
Calibration Table Last Updated: Sat Jan 19 03:10:52 2019

2-Chloroethyl Vinyl ether

Response Ratio

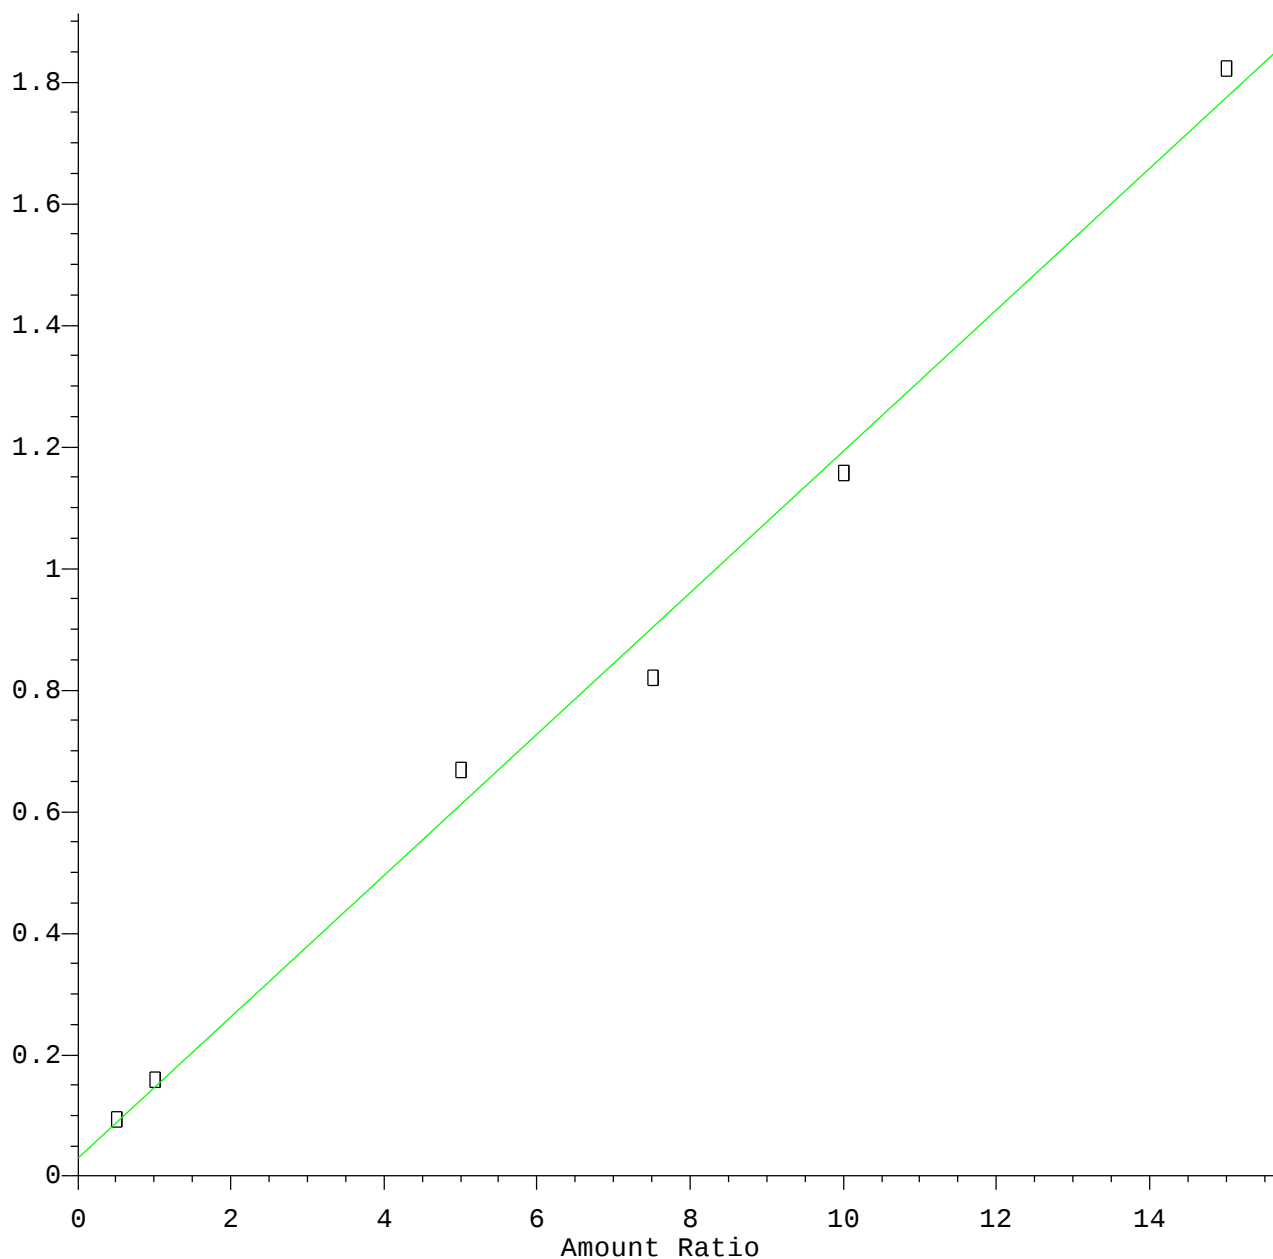


Resp Ratio = $1.16 \times 10^{-1} \times \text{Amt} + 2.97 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D011819S.M
Calibration Table Last Updated: Sat Jan 19 03:10:52 2019

4-Chlorotoluene

Response Ratio

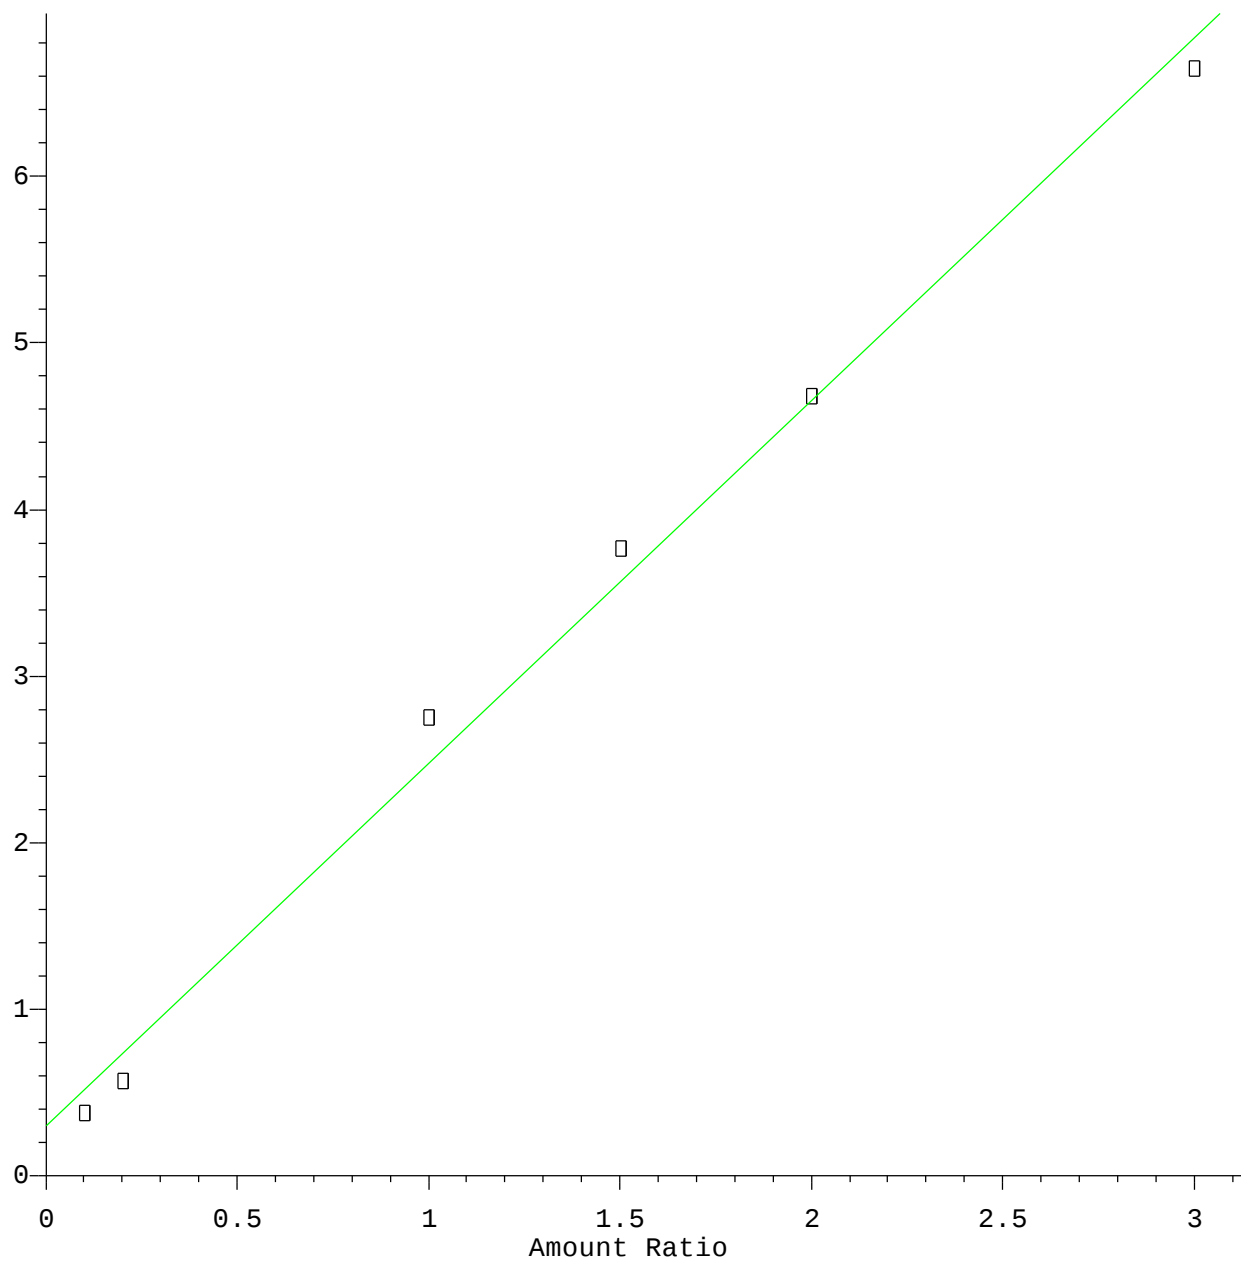

Resp Ratio = 2.18e+000 * Amt + 2.99e-001
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D011819S.M
Calibration Table Last Updated: Sat Jan 19 03:10:52 2019