


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD011819\
 Data File : VD060753.D
 Acq On : 18 Jan 2019 10:09
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D011819S.M
 Title : SW846 8260
 Last Update : Sat Jan 19 03:10:52 2019

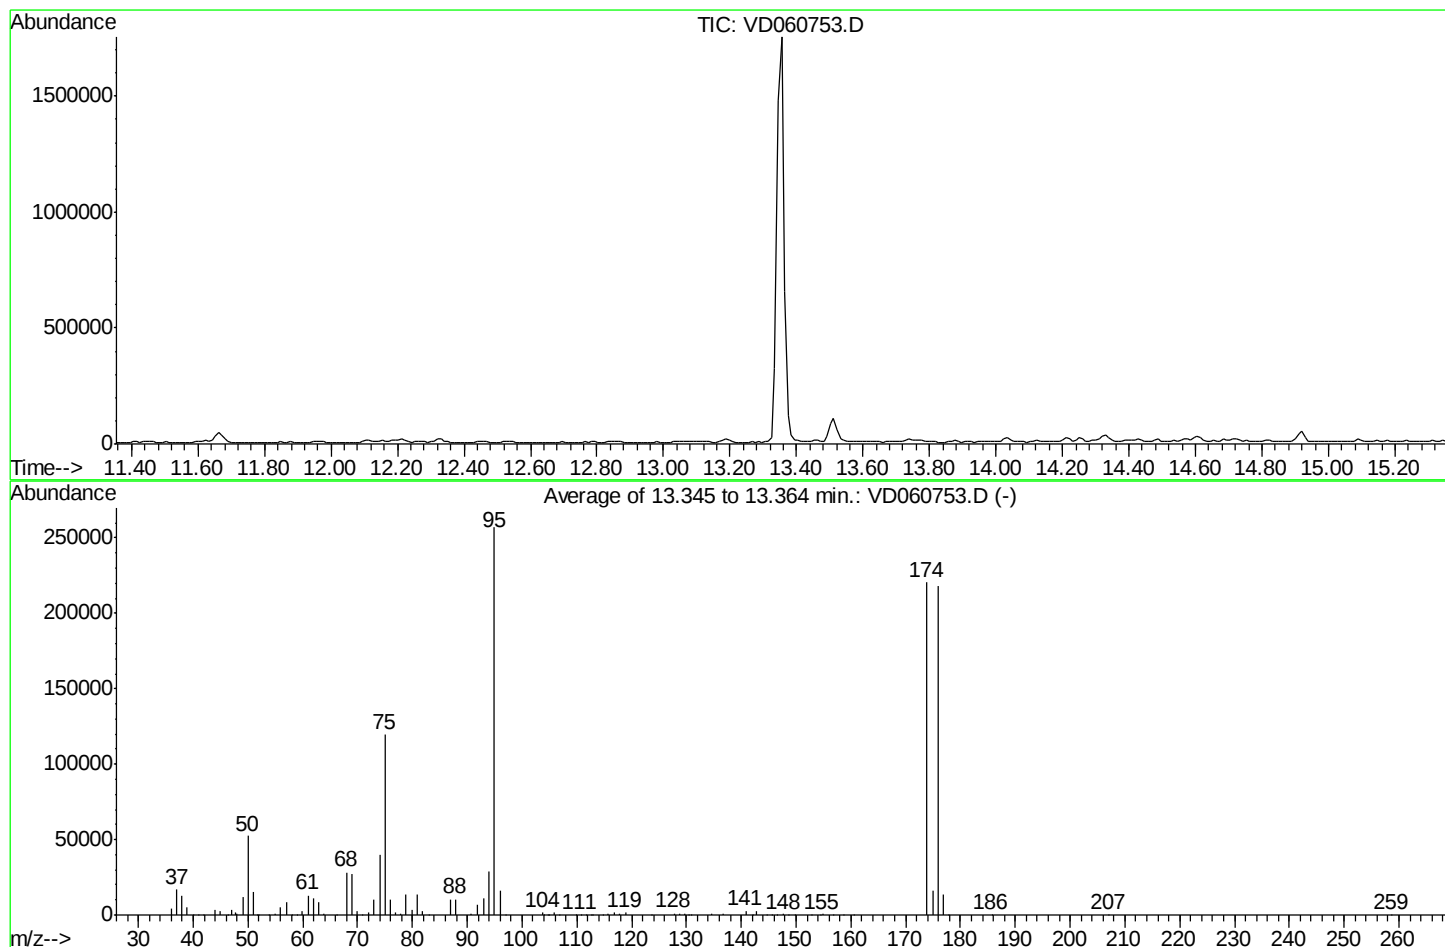

AutoFind: Scans 1251, 1252, 1253; Background Corrected with Scan 1246

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	52386	PASS
75	95	30	60	46.5	119554	PASS
95	95	100	100	100.0	257042	PASS
96	95	5	9	6.3	16279	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.8	220416	PASS
175	174	5	9	7.2	15940	PASS
176	174	95	101	99.1	218538	PASS
177	176	5	9	6.2	13461	PASS