


## Methyl Iodide

Response Ratio

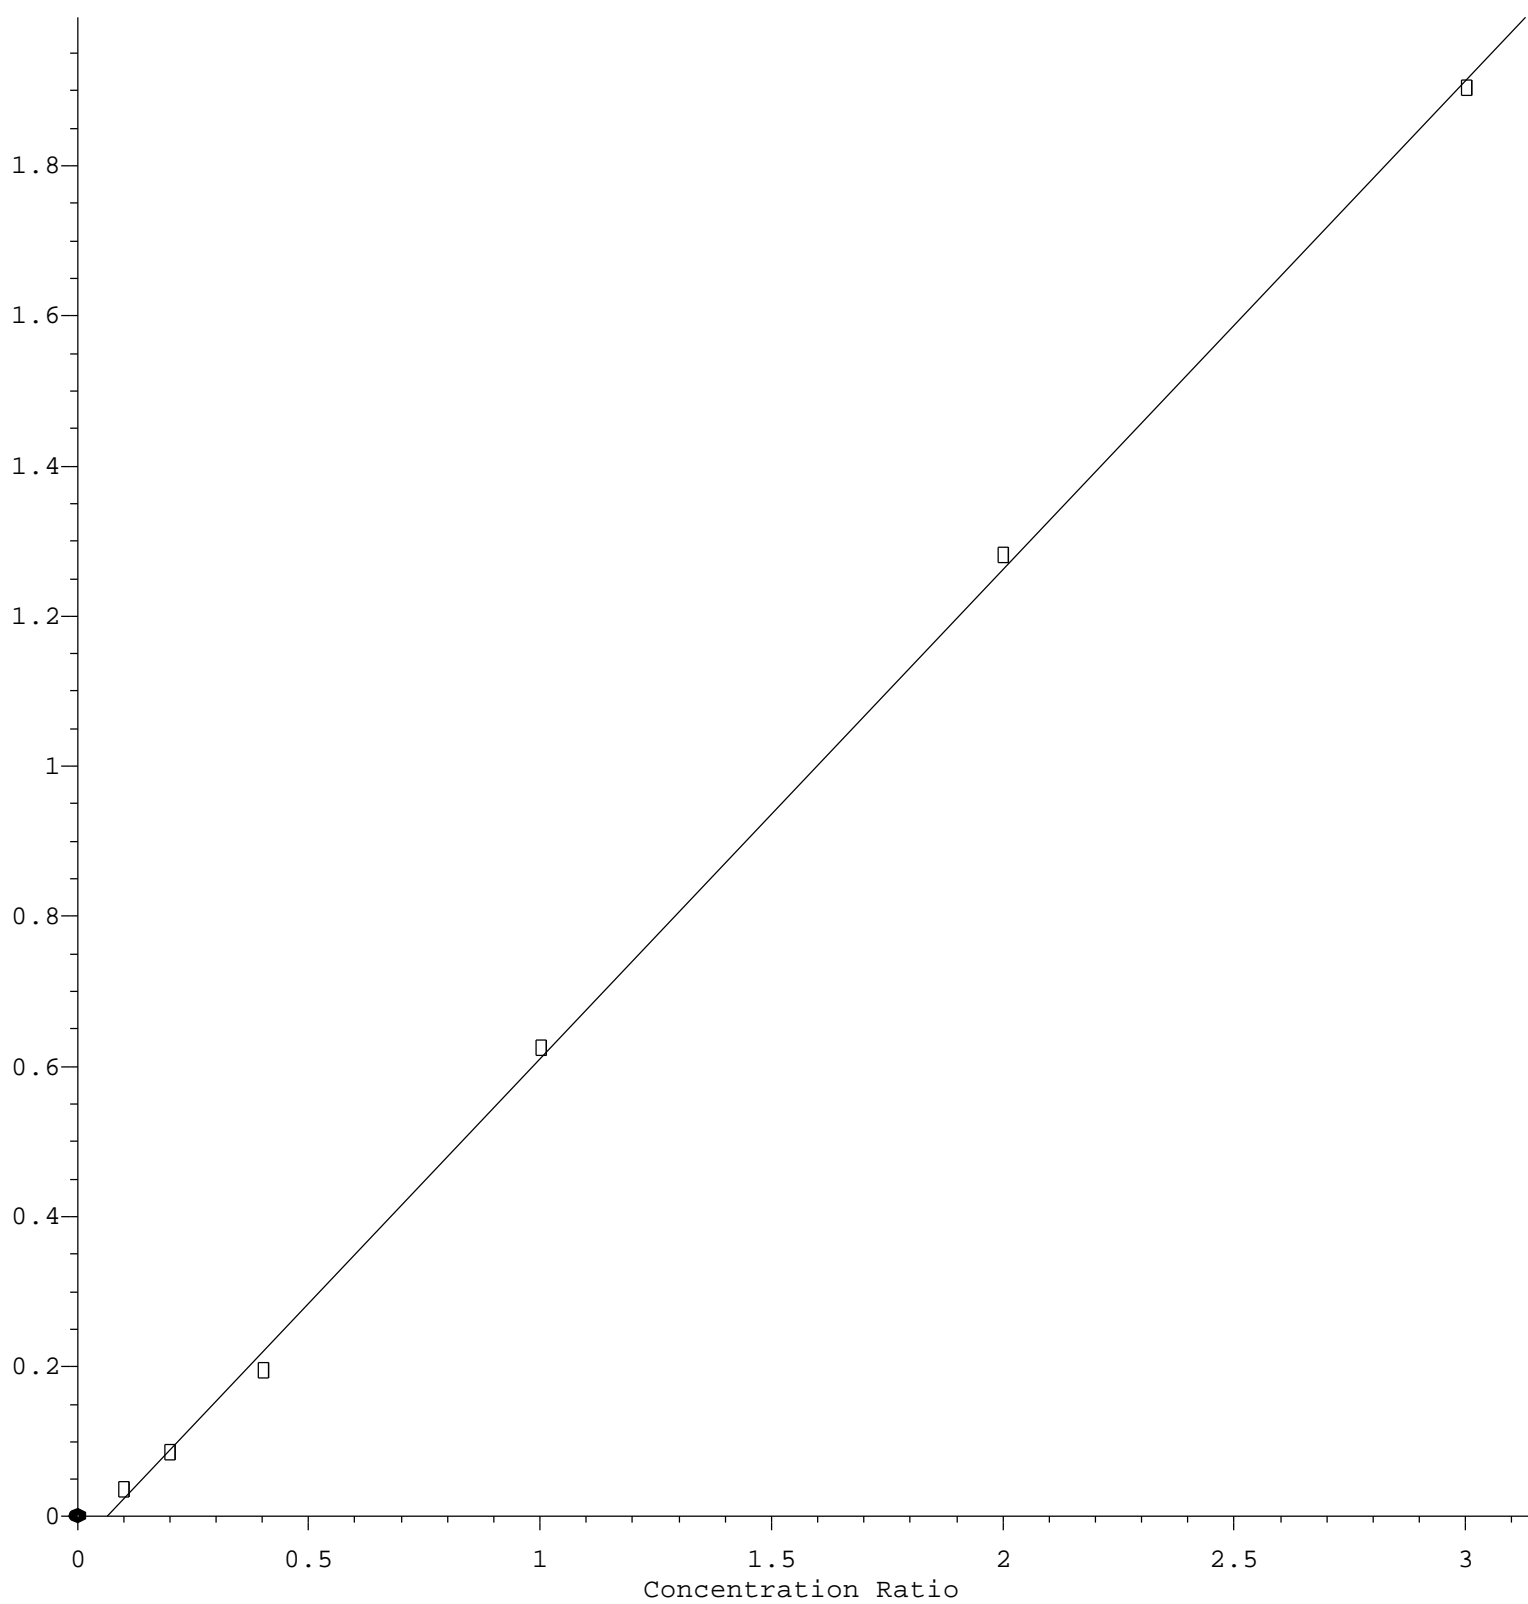


$$\text{Response} = 6.521\text{e-}001 * \text{Amt} - 4.122\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.999511 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D011921S.M

Calibration Table Last Updated: Tue Jan 19 13:19:08 2021


## Tert butyl alcohol

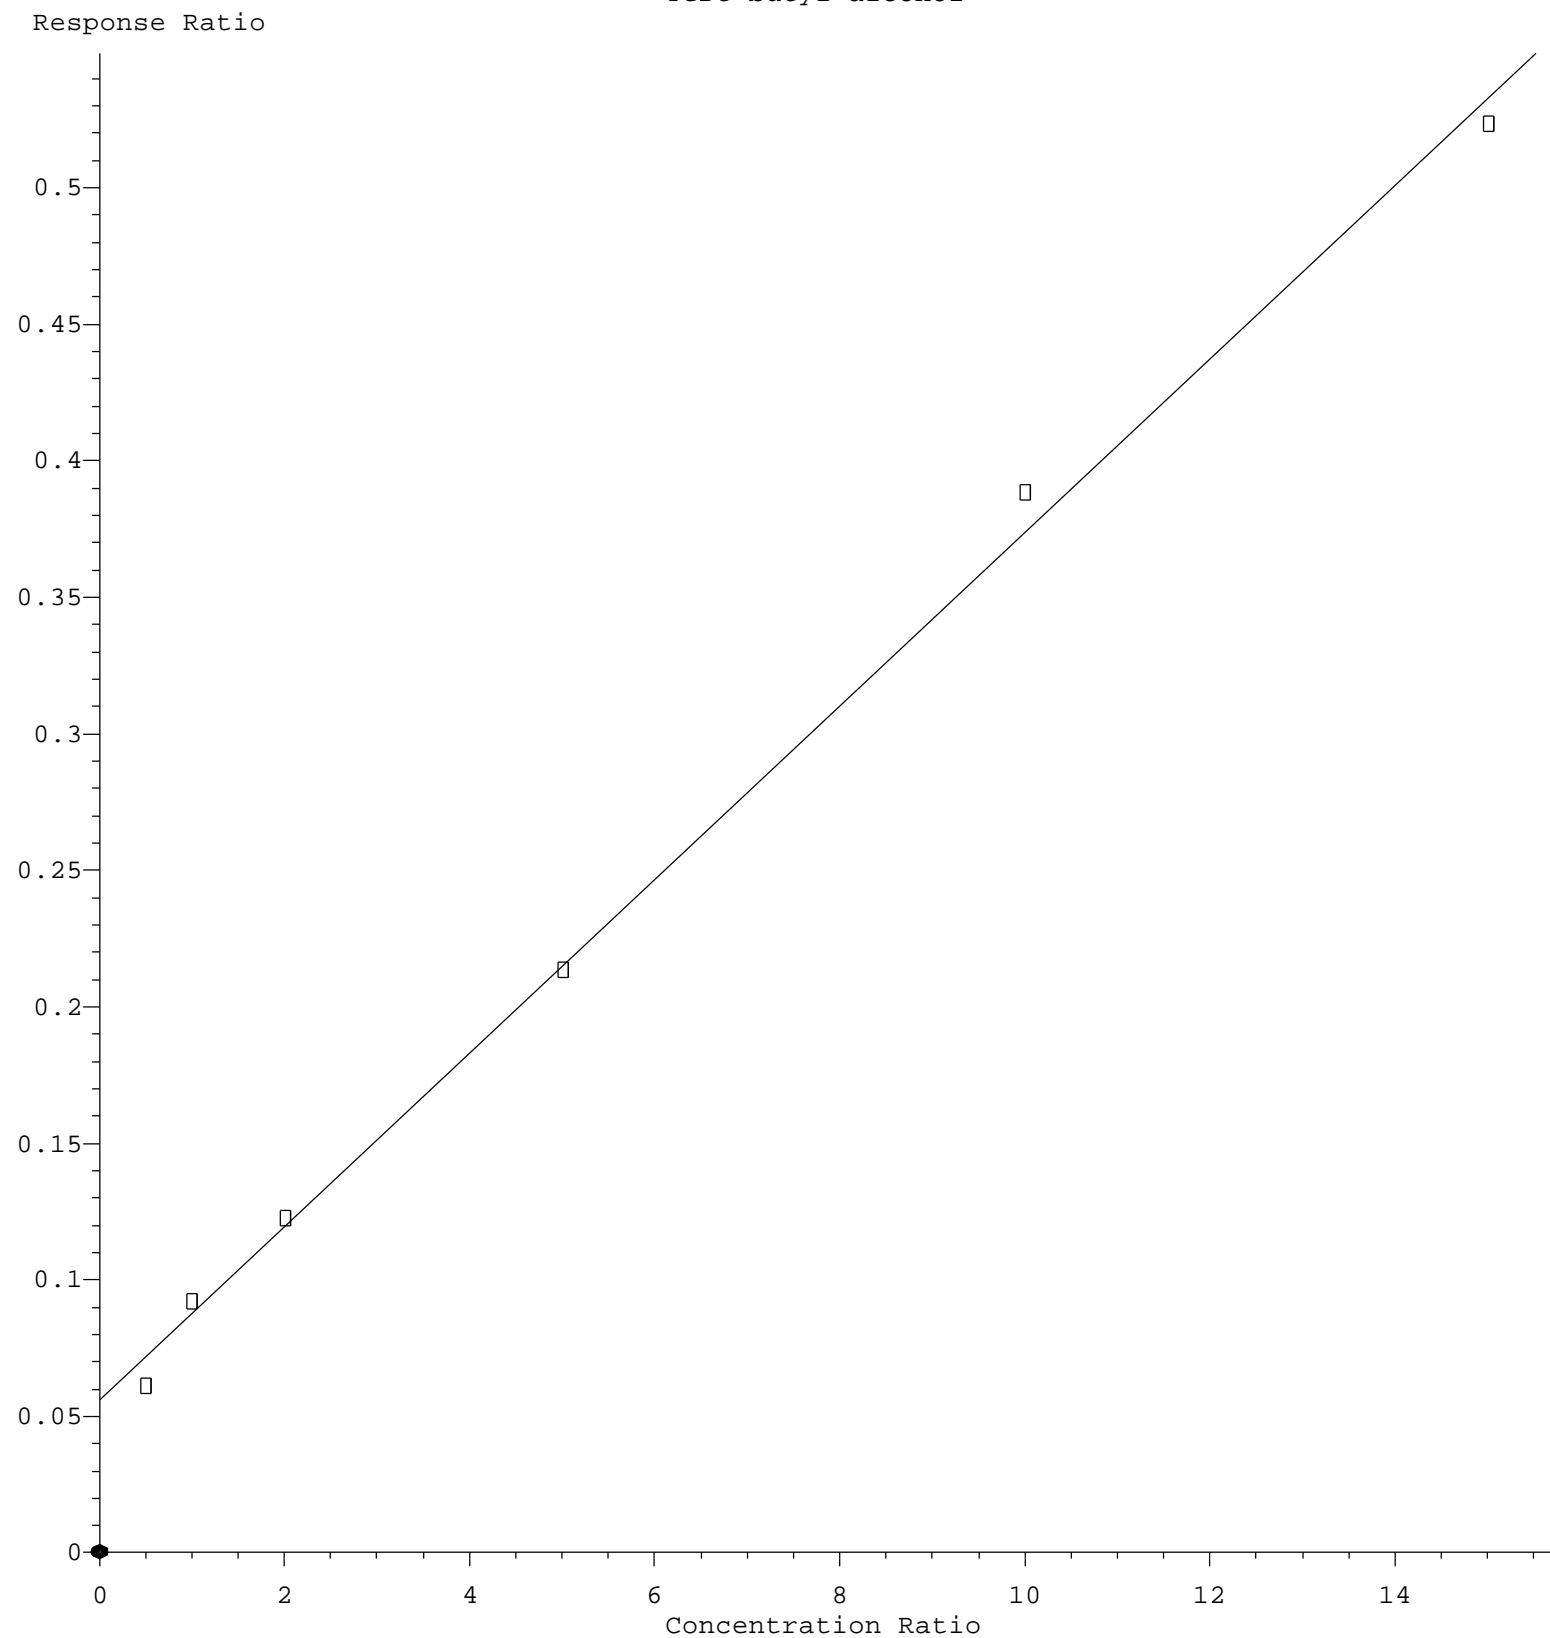

Response =  $3.179 \times 10^{-2} \times \text{Amt} + 5.581 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997332    Curve Fit: Linear  
Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D011921S.M  
Calibration Table Last Updated: Tue Jan 19 13:19:08 2021

## Methylene Chloride

Response Ratio

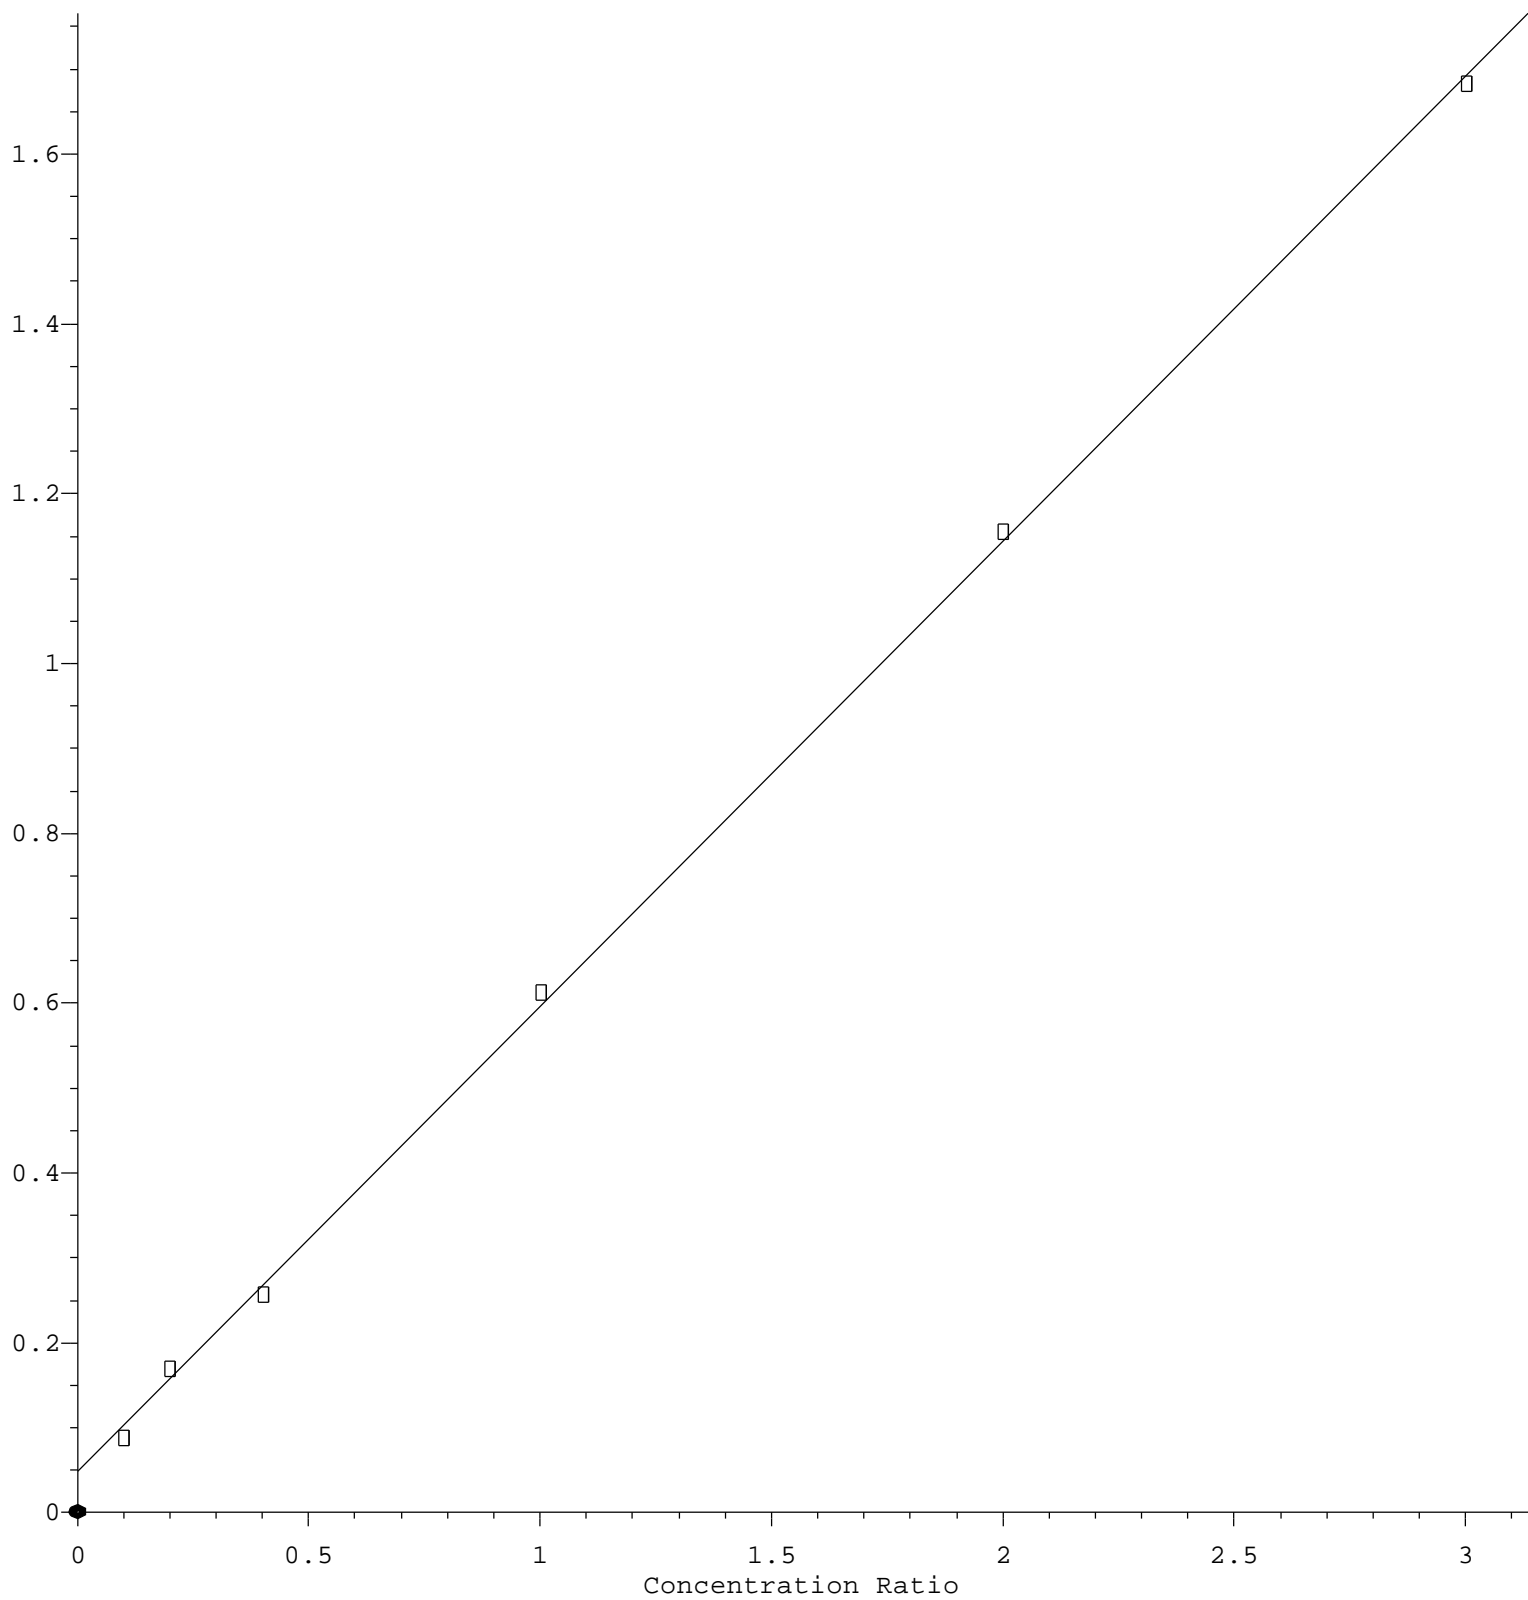

$$\text{Response} = 5.483\text{e-}001 * \text{Amt} + 4.779\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.999523 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D011921S.M

Calibration Table Last Updated: Tue Jan 19 13:19:08 2021