

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011921\
 Data File : VD068098.D
 Acq On : 19 Jan 2021 18:48
 Operator : VA/SY
 Sample : M1160-03
 Misc : 5.43G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BASIN-1

Quant Time: Jan 20 00:31:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 13:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.979	168	21711	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	38895	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.650	117	40701	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	21043	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.338	65	16019	77.13	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 154.26%			
35) Dibromofluoromethane	7.920	113	10188	47.38	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 94.76%			
50) Toluene-d8	10.344	98	51177	59.50	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 119.00%			
62) 4-Bromofluorobenzene	12.632	95	20866	67.36	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 134.72%			
Target Compounds						Qvalue
3) Chloromethane	2.215	50	1950	7.02	ug/l	93
5) Bromomethane	2.791	94	3168	14.95	ug/l #	77
10) Methyl Iodide	4.320	142	2561	12.20	ug/l #	68
11) Tert butyl alcohol	5.068	59	67	Below Cal	#	1
13) Acrolein	3.944	56	115	7.03	ug/l #	1
14) Allyl chloride	4.709	41	417	1.21	ug/l #	59
15) Acrylonitrile	5.403	53	846	17.89	ug/l #	21
16) Acetone	4.162	43	20017	539.77	ug/l	94
18) Methyl Acetate	4.715	43	706	7.34	ug/l #	58
20) Methylene Chloride	4.962	84	1375	1.42	ug/l #	78
25) 2-Butanone	7.214	43	10245	183.48	ug/l	99
29) Tetrahydrofuran	7.550	42	161	4.45	ug/l #	21
37) Ethyl Acetate	7.279	43	486	3.50	ug/l #	64
38) Carbon Tetrachloride	7.991	117	2426	6.61	ug/l #	12
41) Methacrylonitrile	7.544	41	222	2.65	ug/l #	59
43) Isopropyl Acetate	8.456	43	383	1.32	ug/l #	46
48) Methyl methacrylate	9.450	41	294	2.04	ug/l #	1
51) 4-Methyl-2-Pentanone	10.244	43	516	3.84	ug/l #	70
52) Toluene	10.414	92	874	1.22	ug/l #	67
55) 1,1,2-Trichloroethane	10.808	97	314	1.63	ug/l #	33
56) Ethyl methacrylate	10.661	69	652	2.54	ug/l #	75
59) 2-Hexanone	10.997	43	1241	13.32	ug/l #	49
67) Ethyl Benzene	11.755	91	1951	1.22	ug/l	97
74) N-amyl acetate	12.297	43	535	1.47	ug/l #	36
75) 1,1,2,2-Tetrachloroethane	12.773	83	729	2.62	ug/l #	26
76) 1,2,3-Trichloropropane	12.632	75	10735	52.76	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.632	75	10735	106.77	ug/l #	15
89) n-Butylbenzene	13.832	91	1618	1.07	ug/l #	47
92) 1,2-Dibromo-3-Chloropr...	14.485	75	57	1.25	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011921\
Data File : VD068098.D
Acq On : 19 Jan 2021 18:48
Operator : VA/SY
Sample : M1160-03
Misc : 5.43G/5.00ml/MSVOA_D/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BASIN-1

Quant Time: Jan 20 00:31:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 13:19:08 2021
Response via : Initial Calibration




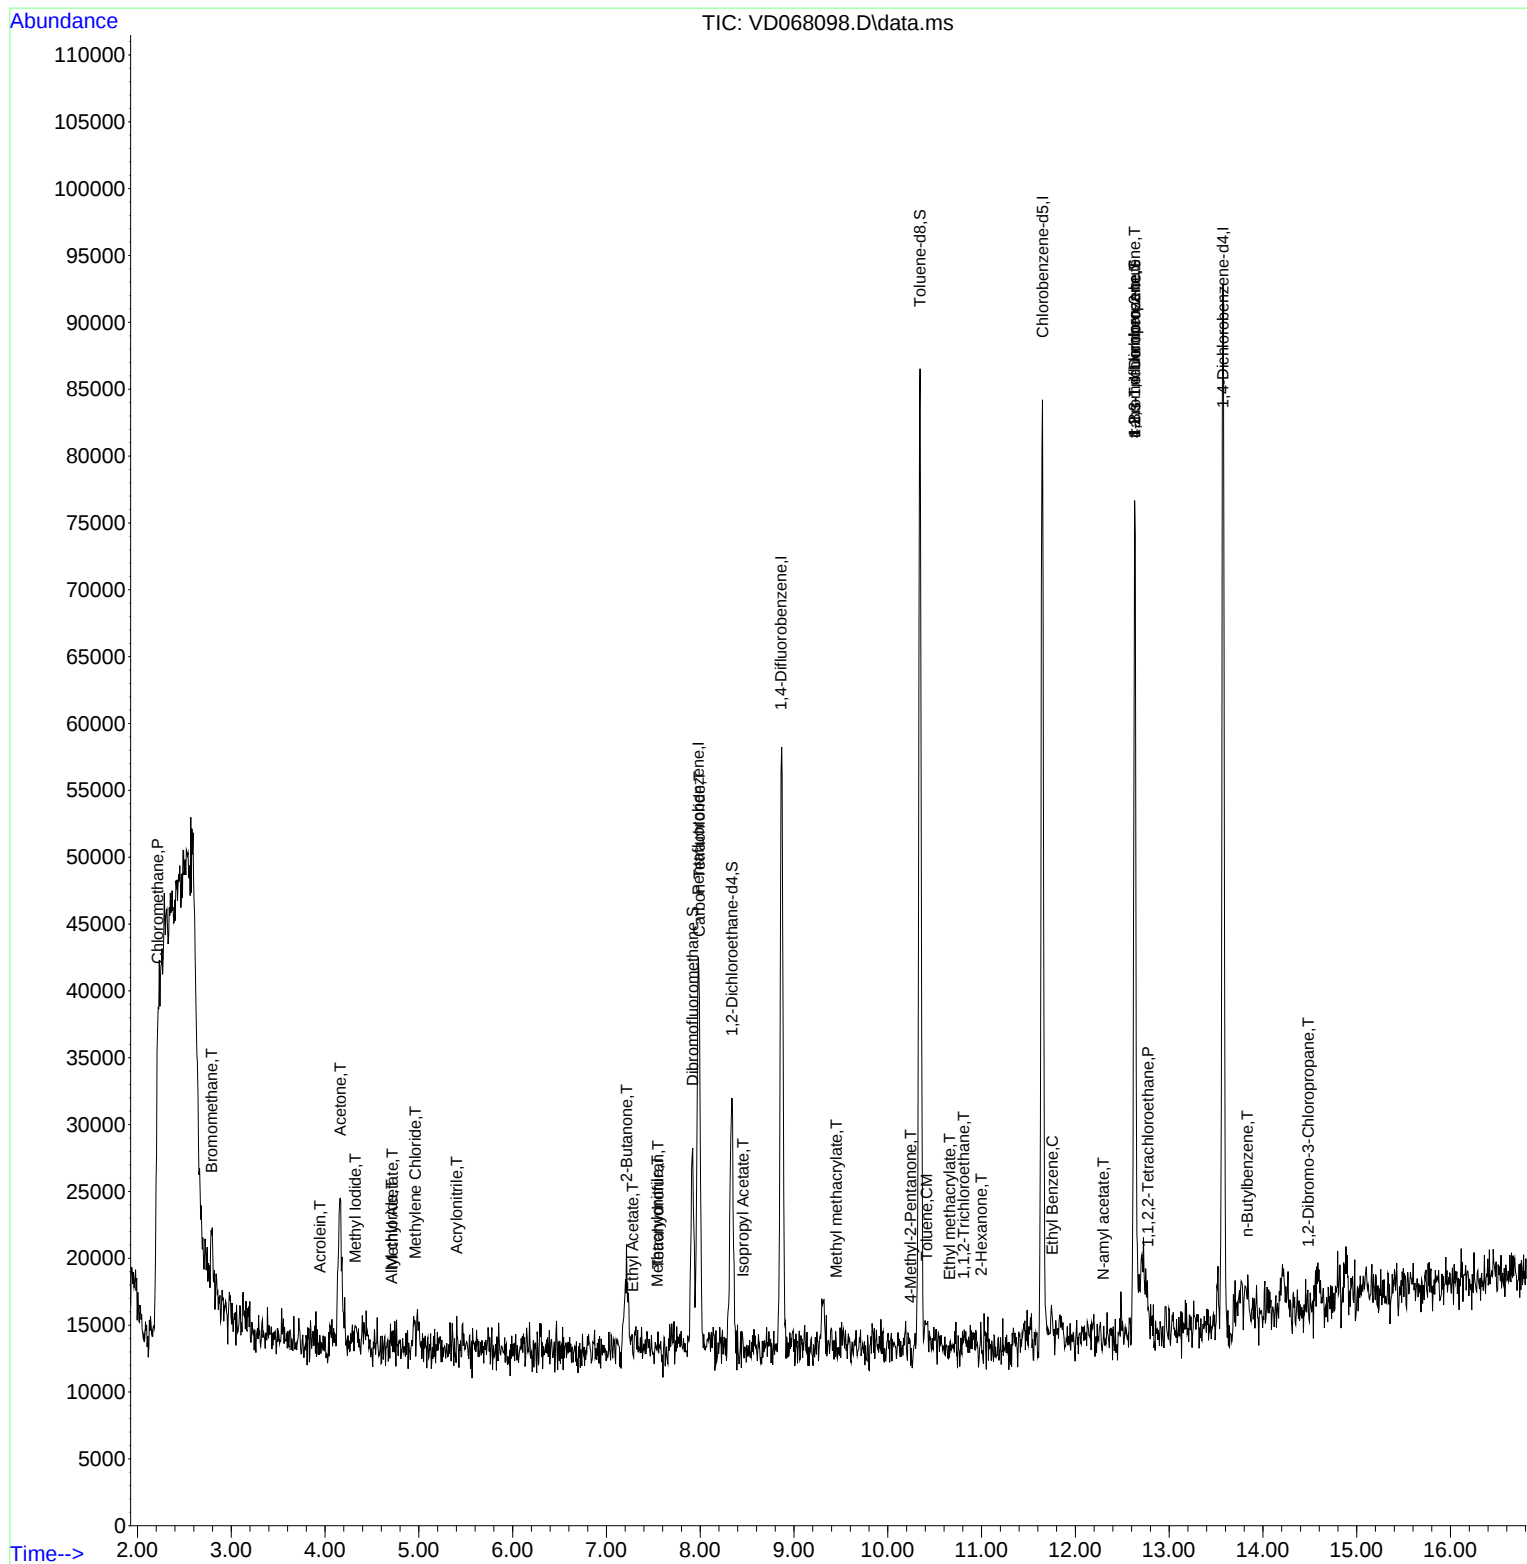




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion:168 Resp: 21711
Ion Ratio Lower Upper
168 100
99 55.0 43.5 65.3

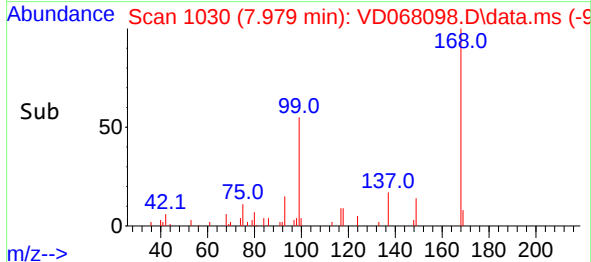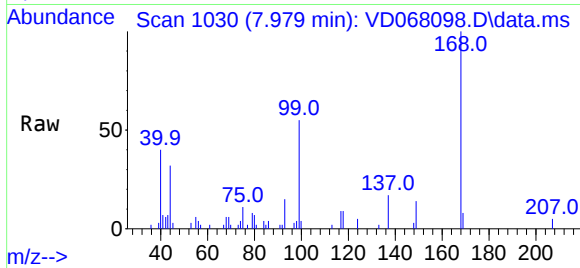

#3
Chloromethane
Concen: 7.02 ug/l
RT: 2.215 min Scan# 50
Delta R.T. 0.001 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 50 Resp: 1950
Ion Ratio Lower Upper
50 100
52 35.7 25.4 38.2


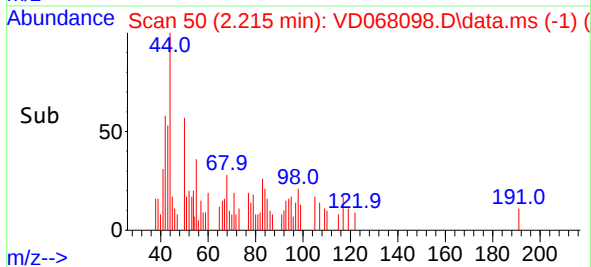

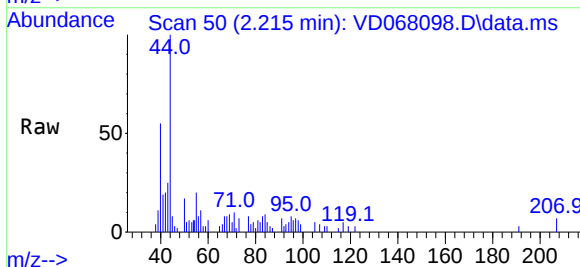




#5
Bromomethane
Concen: 14.95 ug/l
RT: 2.791 min Scan# 148
Delta R.T. 0.018 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 94 Resp: 3168
Ion Ratio Lower Upper
94 100
96 72.8 75.8 113.8#

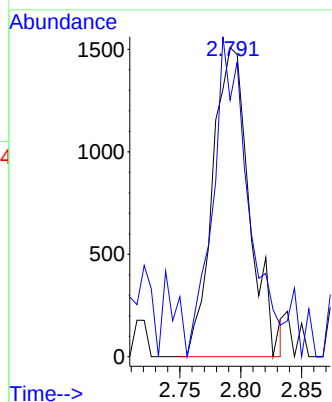

#10
Methyl Iodide
Concen: 12.20 ug/l
RT: 4.320 min Scan# 408
Delta R.T. 0.012 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 142 Resp: 2561
Ion Ratio Lower Upper
142 100
127 26.9 37.9 56.9#
141 0.0 11.5 17.3#


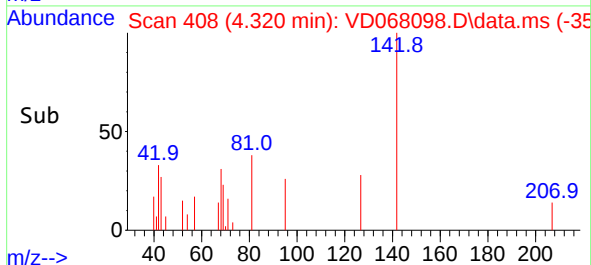

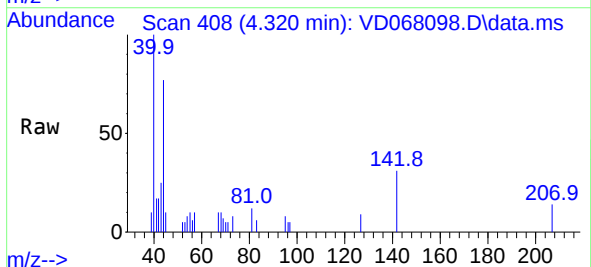




#11
Tert butyl alcohol
Concen: Below Cal
RT: 5.068 min Scan# 535
Delta R.T. -0.152 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampleId :
BASIN-1


Tgt Ion: 59 Resp: 67
Ion Ratio Lower Upper
59 100
57 1009.0 7.4 11.2#



#13
Acrolein
Concen: 7.03 ug/l
RT: 3.944 min Scan# 344
Delta R.T. 0.018 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 56 Resp: 115
Ion Ratio Lower Upper
56 100
55 443.5 56.5 84.7#









#14
 Allyl chloride
 Concen: 1.21 ug/l
 RT: 4.709 min Scan# 474
 Delta R.T. -0.011 min
 Lab File: VD068098.D
 Acq: 19 Jan 2021 18:48




Instrument :
 MSVOA_D
 ClientSampleID :
 BASIN-1


Tgt Ion: 41 Resp: 417
 Ion Ratio Lower Upper
 41 100
 39 54.4 56.3 84.5#
 76 0.0 38.9 58.3#



#15
 Acrylonitrile
 Concen: 17.89 ug/l
 RT: 5.403 min Scan# 592
 Delta R.T. -0.023 min
 Lab File: VD068098.D
 Acq: 19 Jan 2021 18:48

Tgt Ion: 53 Resp: 846
 Ion Ratio Lower Upper
 53 100
 52 0.0 66.2 99.2#
 51 7.0 29.0 43.4#


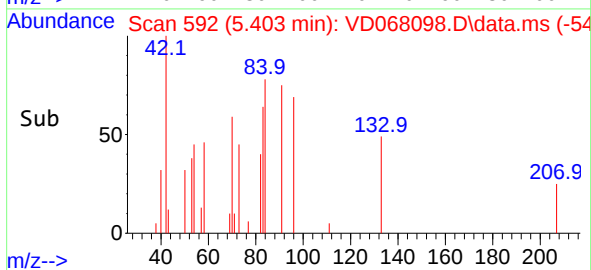






#16
Acetone
Concen: 539.77 ug/l
RT: 4.162 min Scan# 381
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 43 Resp: 20017
Ion Ratio Lower Upper
43 100
58 27.1 24.2 36.4

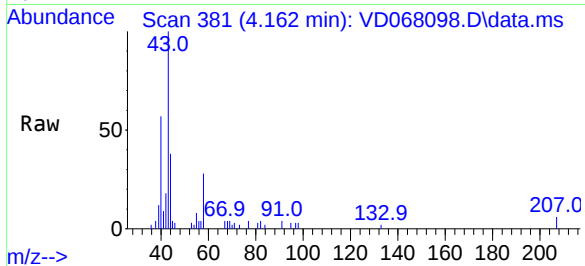

#18
Methyl Acetate
Concen: 7.34 ug/l
RT: 4.715 min Scan# 475
Delta R.T. -0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 43 Resp: 706
Ion Ratio Lower Upper
43 100
74 8.6 25.4 38.0#

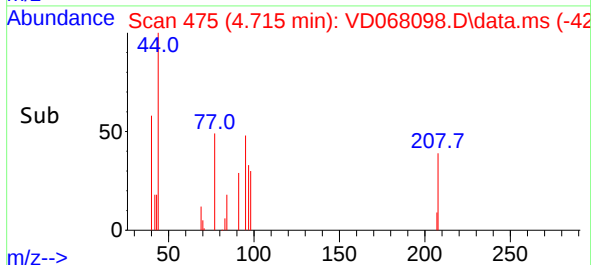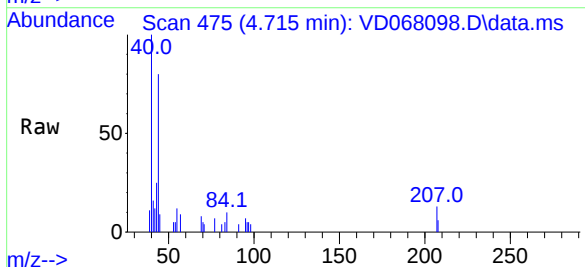







#20
Methylene Chloride
Concen: 1.42 ug/l
RT: 4.962 min Scan# 517
Delta R.T. -0.011 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Instrument :
MSVOA_D
ClientSampled :
BASIN-1

Tgt Ion: 84 Resp: 1375




Ion	Ratio	Lower	Upper
84	100		
49	81.3	77.4	116.2
51	48.6	26.1	39.1#
86	43.0	51.8	77.8#




#25
2-Butanone
Concen: 183.48 ug/l
RT: 7.214 min Scan# 900
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 43 Resp: 10245

Ion	Ratio	Lower	Upper
43	100		
72	31.7	25.1	37.7



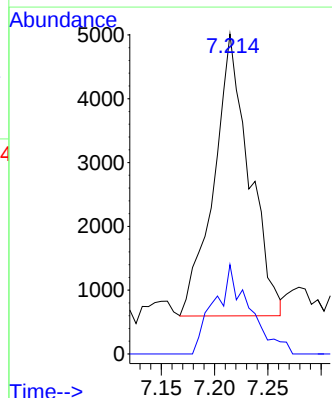





#29
Tetrahydrofuran
Concen: 4.45 ug/l
RT: 7.550 min Scan# 957
Delta R.T. -0.017 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampleId :
BASIN-1


Tgt Ion: 42 Resp: 161
Ion Ratio Lower Upper
42 100
72 92.5 43.4 65.0#
71 125.5 40.8 61.2#

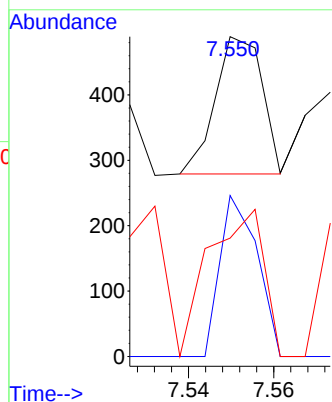

#33
1,2-Dichloroethane-d4
Concen: 77.13 ug/l
RT: 8.338 min Scan# 1091
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 65 Resp: 16019
Ion Ratio Lower Upper
65 100
67 60.1 0.0 105.0

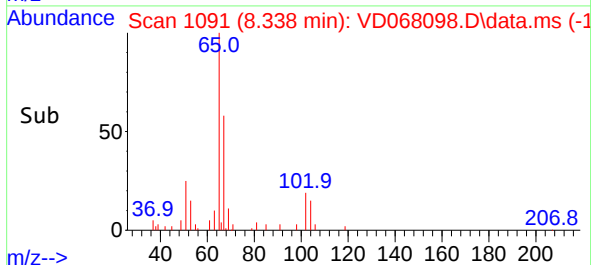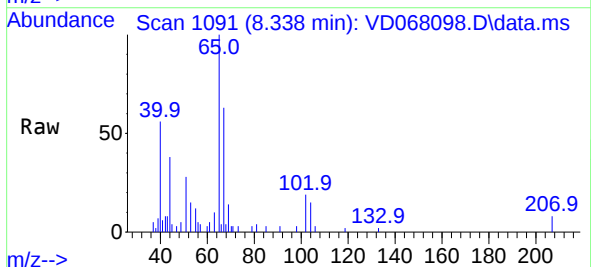




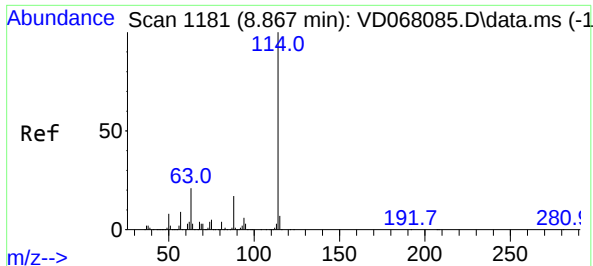


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. -0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Instrument :
MSVOA_D
ClientSampled :
BASIN-1




Tgt Ion:	114	Resp:	38895
Ion	Ratio	Lower	Upper
114	100		
63	19.2	0.0	34.8
88	15.1	0.0	31.6

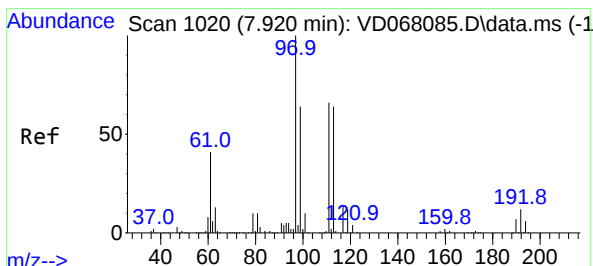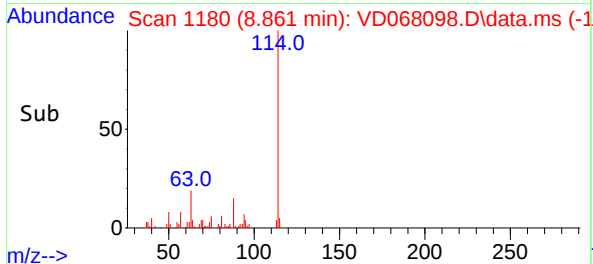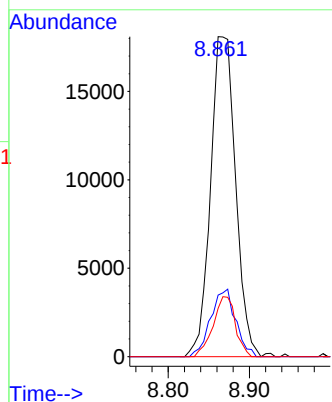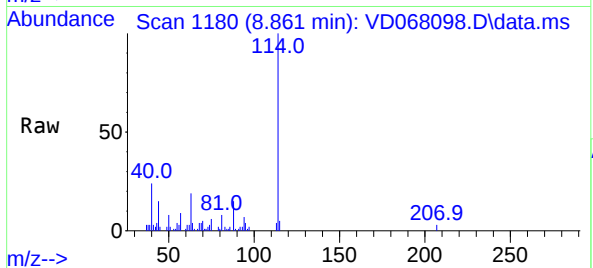


#35

Dibromofluoromethane
Concen: 47.38 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion:	113	Resp:	10188
Ion	Ratio	Lower	Upper
113	100		
111	101.3	81.4	122.0
192	19.6	16.1	24.1


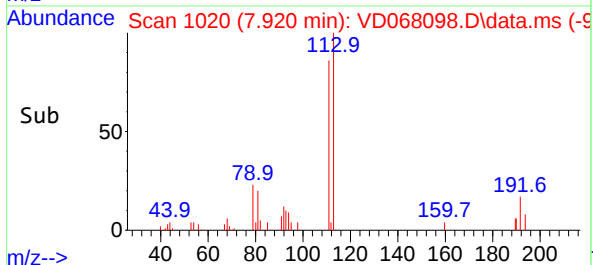

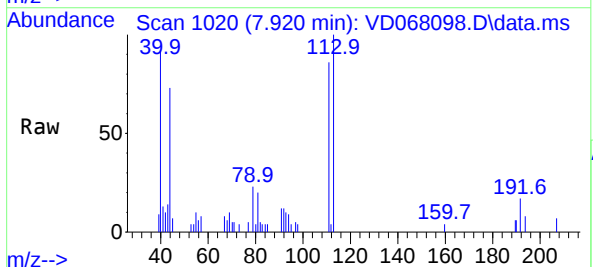




#37
Ethyl Acetate
Concen: 3.50 ug/l
RT: 7.279 min Scan# 911
Delta R.T. -0.017 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampleId :
BASIN-1


Tgt Ion: 43 Resp: 486
Ion Ratio Lower Upper
43 100
61 0.0 12.9 19.3#
70 0.0 11.0 16.6#

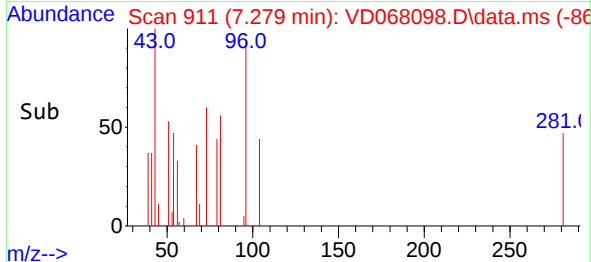

#38
Carbon Tetrachloride
Concen: 6.61 ug/l
RT: 7.991 min Scan# 1032
Delta R.T. -0.111 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 117 Resp: 2426
Ion Ratio Lower Upper
117 100
119 0.0 77.3 115.9#
121 0.0 24.7 37.1#

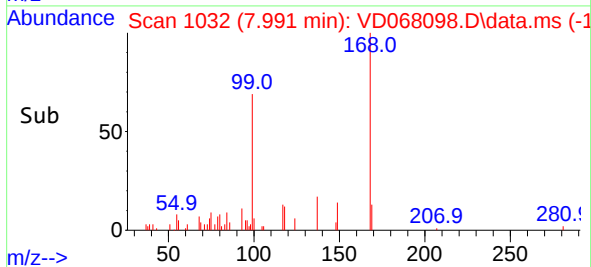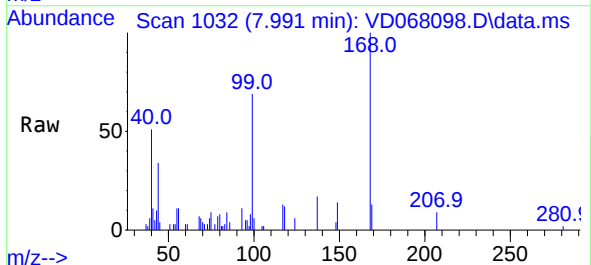







#41
Methacrylonitrile
Concen: 2.65 ug/l
RT: 7.544 min Scan# 956
Delta R.T. 0.012 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Instrument :
MSVOA_D
ClientSampled :
BASIN-1

Tgt Ion: 41 Resp: 222




Ion	Ratio	Lower	Upper
41	100		
39	86.5	45.2	67.8#
67	53.6	67.4	101.2#
52	0.0	27.5	41.3#




#43
Isopropyl Acetate
Concen: 1.32 ug/l
RT: 8.456 min Scan# 1111
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 43 Resp: 383

Ion	Ratio	Lower	Upper
43	100		
61	0.0	28.7	43.1#
87	0.0	13.9	20.9#

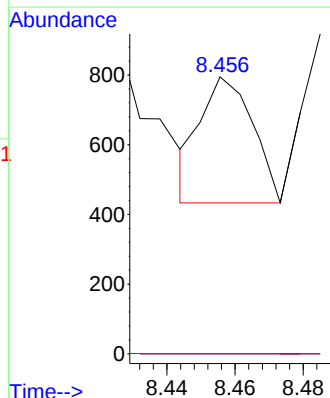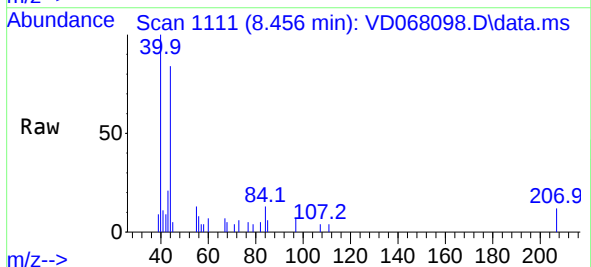

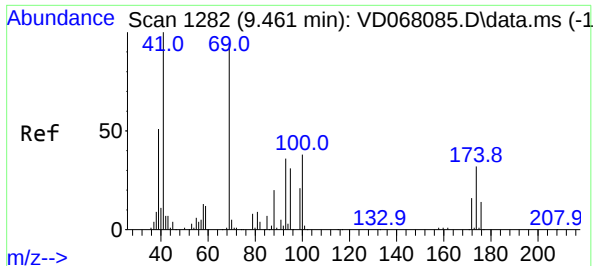

#48

Methyl methacrylate

Concen: 2.04 ug/l

RT: 9.450 min Scan# 1280

Delta R.T. -0.011 min

Lab File: VD068098.D

Acq: 19 Jan 2021 18:48

Instrument :





MSVOA_D

ClientSampled :

BASIN-1

Tgt Ion: 41 Resp: 294

Ion	Ratio	Lower	Upper
41	100		
69	259.2	77.1	115.7#
39	85.7	41.5	62.3#

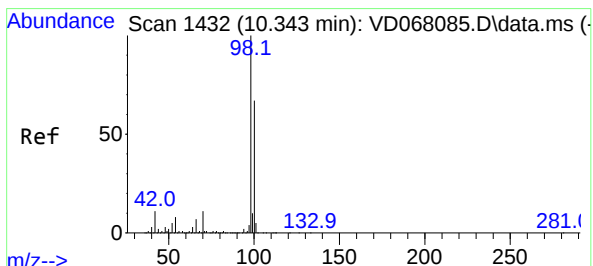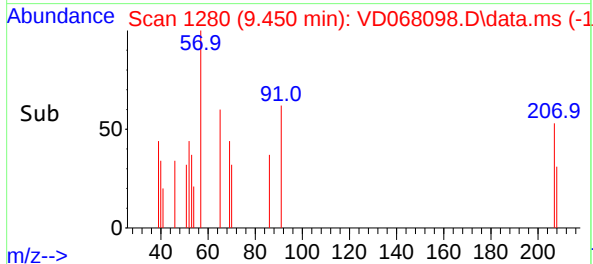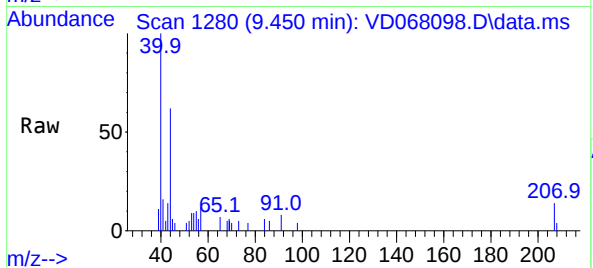

#50

Toluene-d8

Concen: 59.50 ug/l

RT: 10.344 min Scan# 1432




Delta R.T. 0.000 min


Lab File: VD068098.D

Acq: 19 Jan 2021 18:48

Tgt Ion: 98 Resp: 51177

Ion	Ratio	Lower	Upper
98	100		
100	65.6	53.0	79.4


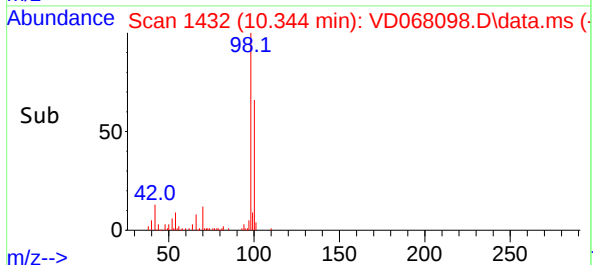
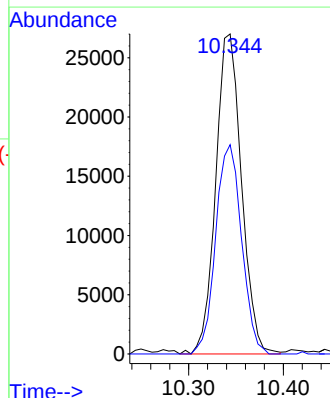
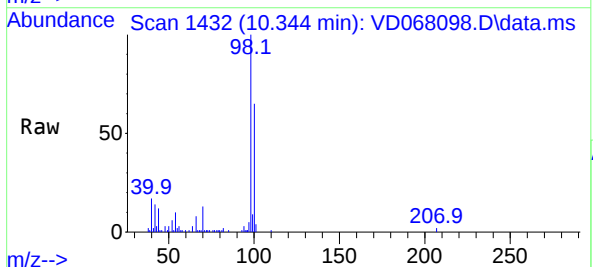




#51
4-Methyl-2-Pentanone
Concen: 3.84 ug/l
RT: 10.244 min Scan# 1415
Delta R.T. 0.012 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 43 Resp: 516
Ion Ratio Lower Upper
43 100
58 25.4 36.1 54.1#

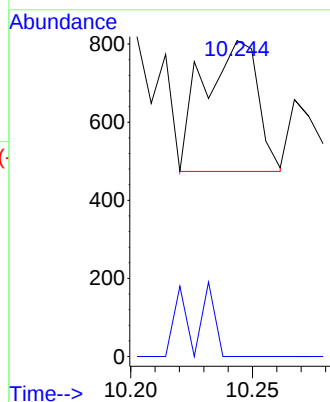

#52
Toluene
Concen: 1.22 ug/l
RT: 10.414 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 92 Resp: 874
Ion Ratio Lower Upper
92 100
91 212.9 134.1 201.1#


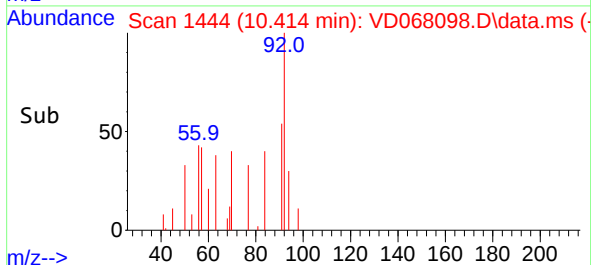

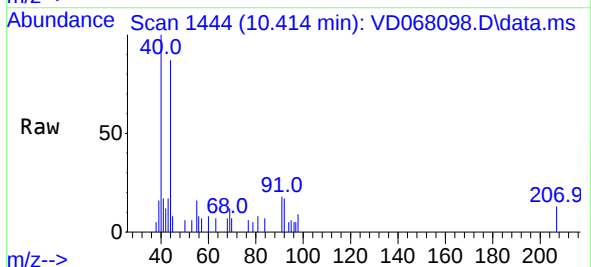




#55
1,1,2-Trichloroethane
Concen: 1.63 ug/l
RT: 10.808 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion:	97	Resp:	314
Ion	Ratio	Lower	Upper
97	100		
83	32.2	61.8	92.6#
85	0.0	42.2	63.2#
99	0.0	48.3	72.5#



#56
Ethyl methacrylate
Concen: 2.54 ug/l
RT: 10.661 min Scan# 1486
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion:	69	Resp:	652
Ion	Ratio	Lower	Upper
69	100		
41	64.7	44.9	67.3
39	0.0	21.9	32.9#



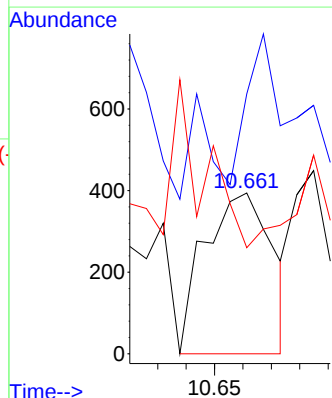





#59
2-Hexanone
Concen: 13.32 ug/l
RT: 10.997 min Scan# 1543
Delta R.T. 0.012 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 43 Resp: 1241
Ion Ratio Lower Upper
43 100
58 22.8 31.0 93.0#

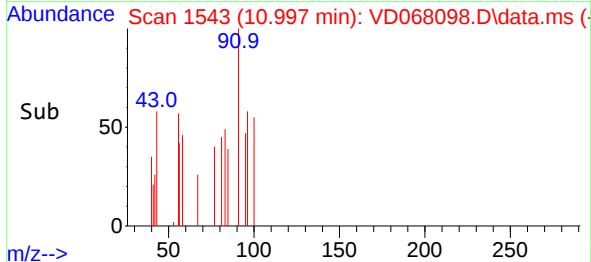

#62
4-Bromofluorobenzene
Concen: 67.36 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 95 Resp: 20866
Ion Ratio Lower Upper
95 100
174 73.4 0.0 172.4
176 74.7 0.0 168.4


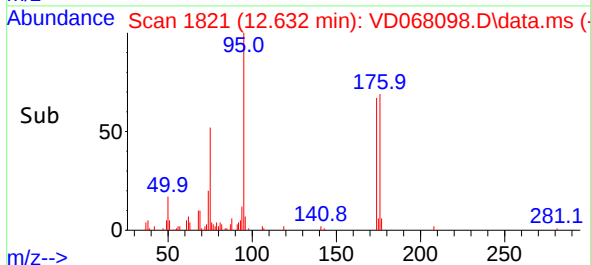
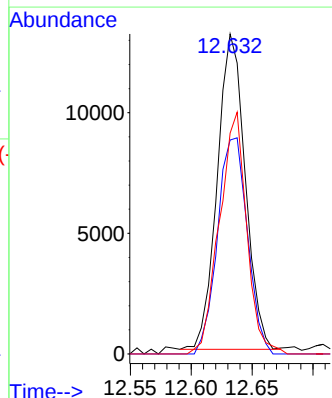
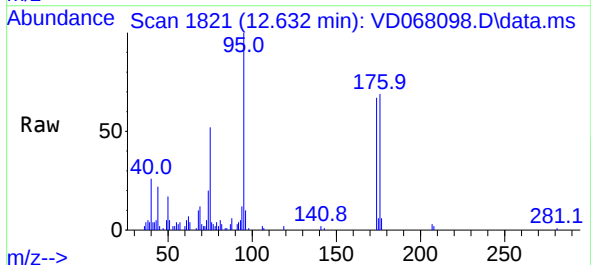




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.650 min Scan# 1654
Delta R.T. 0.001 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion:	117	Resp:	40701
Ion	Ratio	Lower	Upper
117	100		
82	57.0	41.4	62.0
119	31.9	26.1	39.1

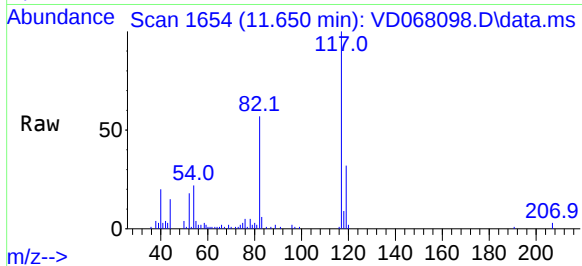

#67
Ethyl Benzene
Concen: 1.22 ug/l
RT: 11.755 min Scan# 1672
Delta R.T. 0.012 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion:	91	Resp:	1951
Ion	Ratio	Lower	Upper
91	100		
106	33.9	25.9	38.9


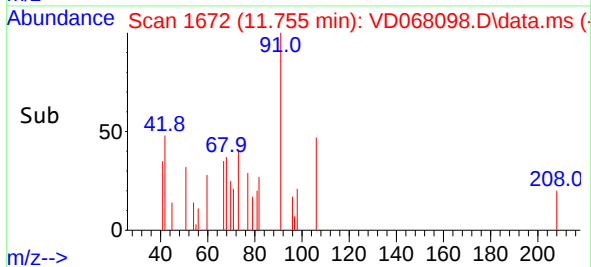

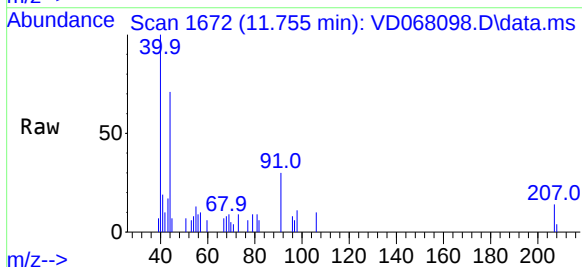




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.000 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion:152 Resp: 21043
Ion Ratio Lower Upper
152 100
115 63.9 28.9 86.8
150 161.0 0.0 344.4

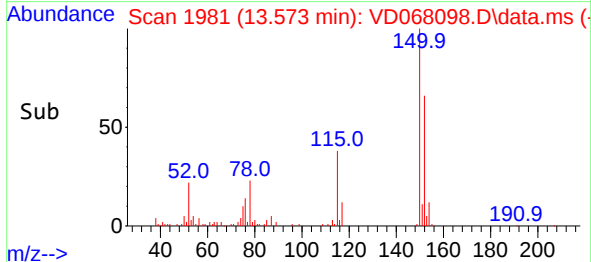

#74
N-ethyl acetate
Concen: 1.47 ug/l
RT: 12.297 min Scan# 1764
Delta R.T. 0.006 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 43 Resp: 535
Ion Ratio Lower Upper
43 100
70 0.0 41.8 62.8#
55 0.0 24.2 36.4#
61 0.0 21.7 32.5#


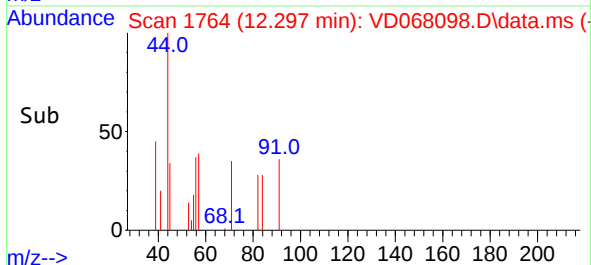
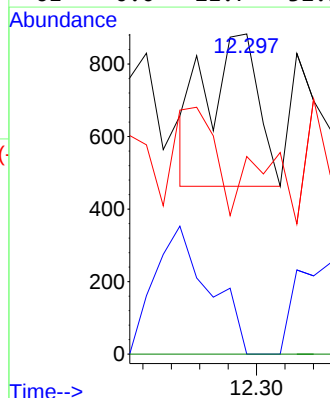
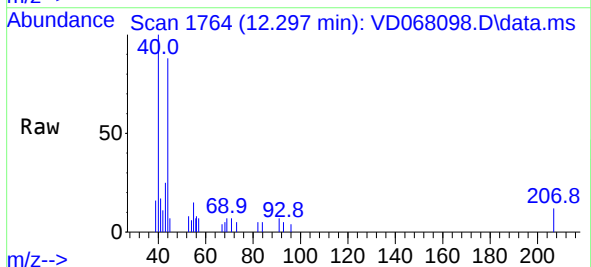




#75
1,1,2,2-Tetrachloroethane
Concen: 2.62 ug/l
RT: 12.773 min Scan# 1845
Delta R.T. 0.042 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 83 Resp: 729
Ion Ratio Lower Upper
83 100
131 0.0 5.8 17.4#
85 0.0 32.4 97.2#

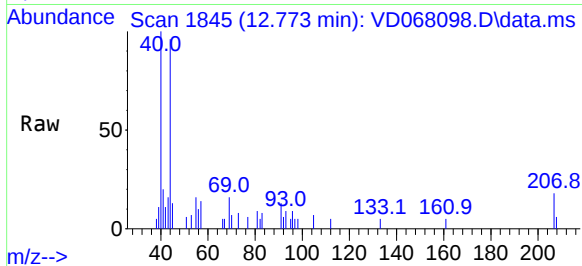

#76
1,2,3-Trichloropropane
Concen: 52.76 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.153 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 75 Resp: 10735
Ion Ratio Lower Upper
75 100
77 5.0 0.0 0.0#



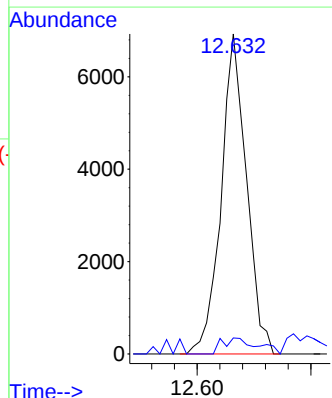
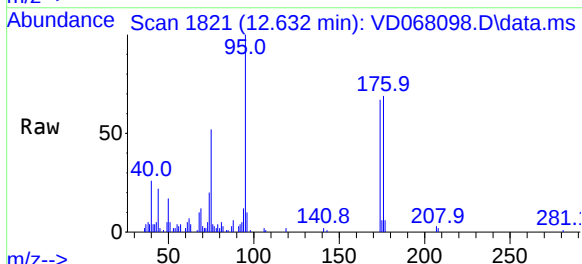


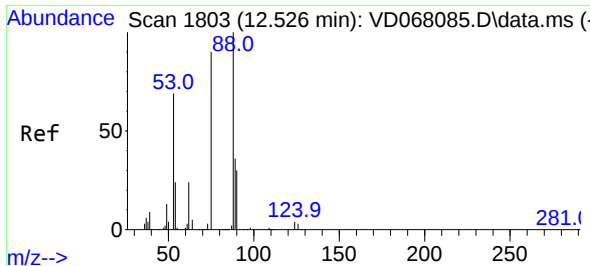

#81
trans-1,4-Dichloro-2-butene
Concen: 106.77 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48




Instrument :
MSVOA_D
ClientSampled :
BASIN-1


Tgt Ion: 75 Resp: 10735
Ion Ratio Lower Upper
75 100
53 2.7 70.2 105.2#
89 0.0 40.3 60.5#

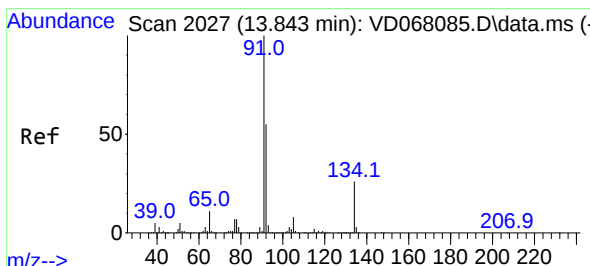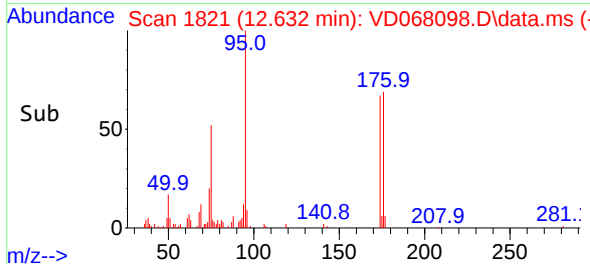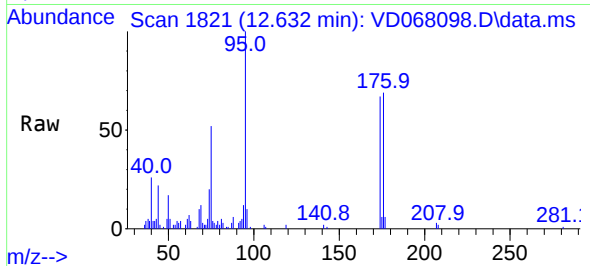

#89
n-Butylbenzene
Concen: 1.07 ug/l
RT: 13.832 min Scan# 2025
Delta R.T. -0.011 min
Lab File: VD068098.D
Acq: 19 Jan 2021 18:48

Tgt Ion: 91 Resp: 1618
Ion Ratio Lower Upper
91 100
92 13.7 27.2 81.6#
134 3.5 13.9 41.7#

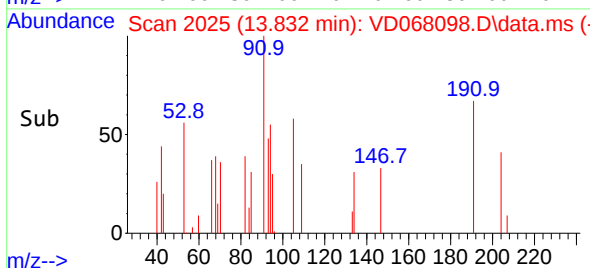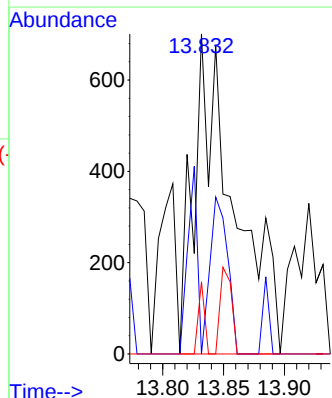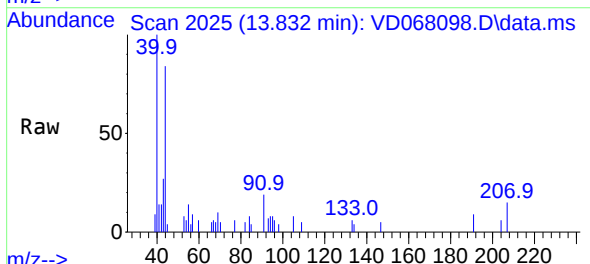



#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.25 ug/l
 RT: 14.485 min Scan# 2136
 Delta R.T. -0.023 min
 Lab File: VD068098.D
 Acq: 19 Jan 2021 18:48

Instrument :
 MSVOA_D
 ClientSampleId :
 BASIN-1

Tgt Ion:	75	Resp:	57
Ion	Ratio	Lower	Upper
75	100		
155	0.0	48.0	144.2#
157	0.0	65.0	194.8#

