
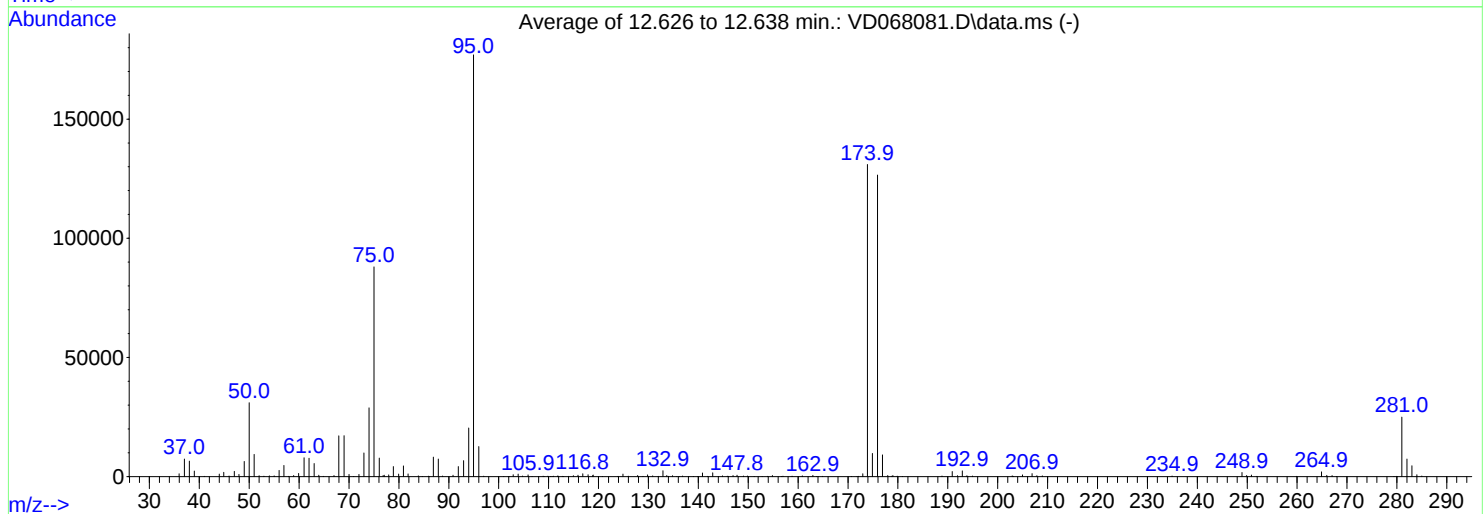


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011921\
Data File : VD068081.D
Acq On : 19 Jan 2021 09:43
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Title : SW846 8260
Last Update : Tue Jan 19 13:19:08 2021

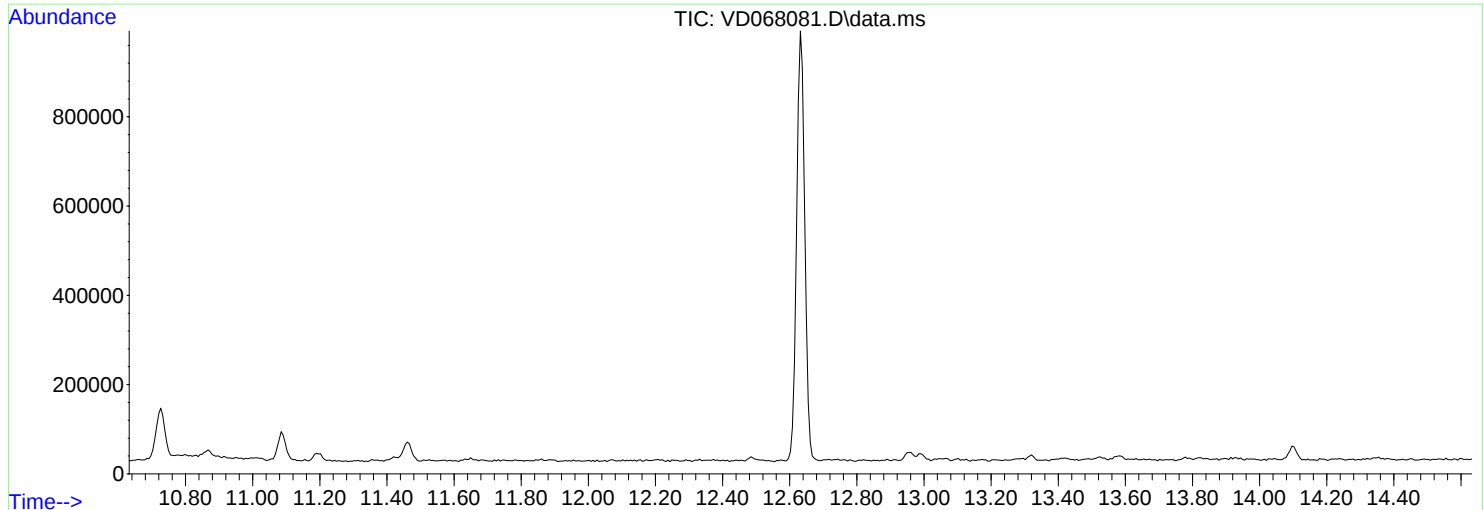

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1811

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	31043	PASS
75	95	30	60	49.7	88011	PASS
95	95	100	100	100.0	176968	PASS
96	95	5	9	7.1	12621	PASS
173	174	0.00	2	0.9	1200	PASS
174	95	50	100	74.0	130955	PASS
175	174	5	9	7.4	9736	PASS
176	174	95	101	96.6	126531	PASS
177	176	5	9	7.2	9109	PASS