


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011922\
Data File : VD071735.D
Acq On : 19 Jan 2022 08:52
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D010722S.M
Title : SW846 8260
Last Update : Fri Jan 07 15:39:14 2022

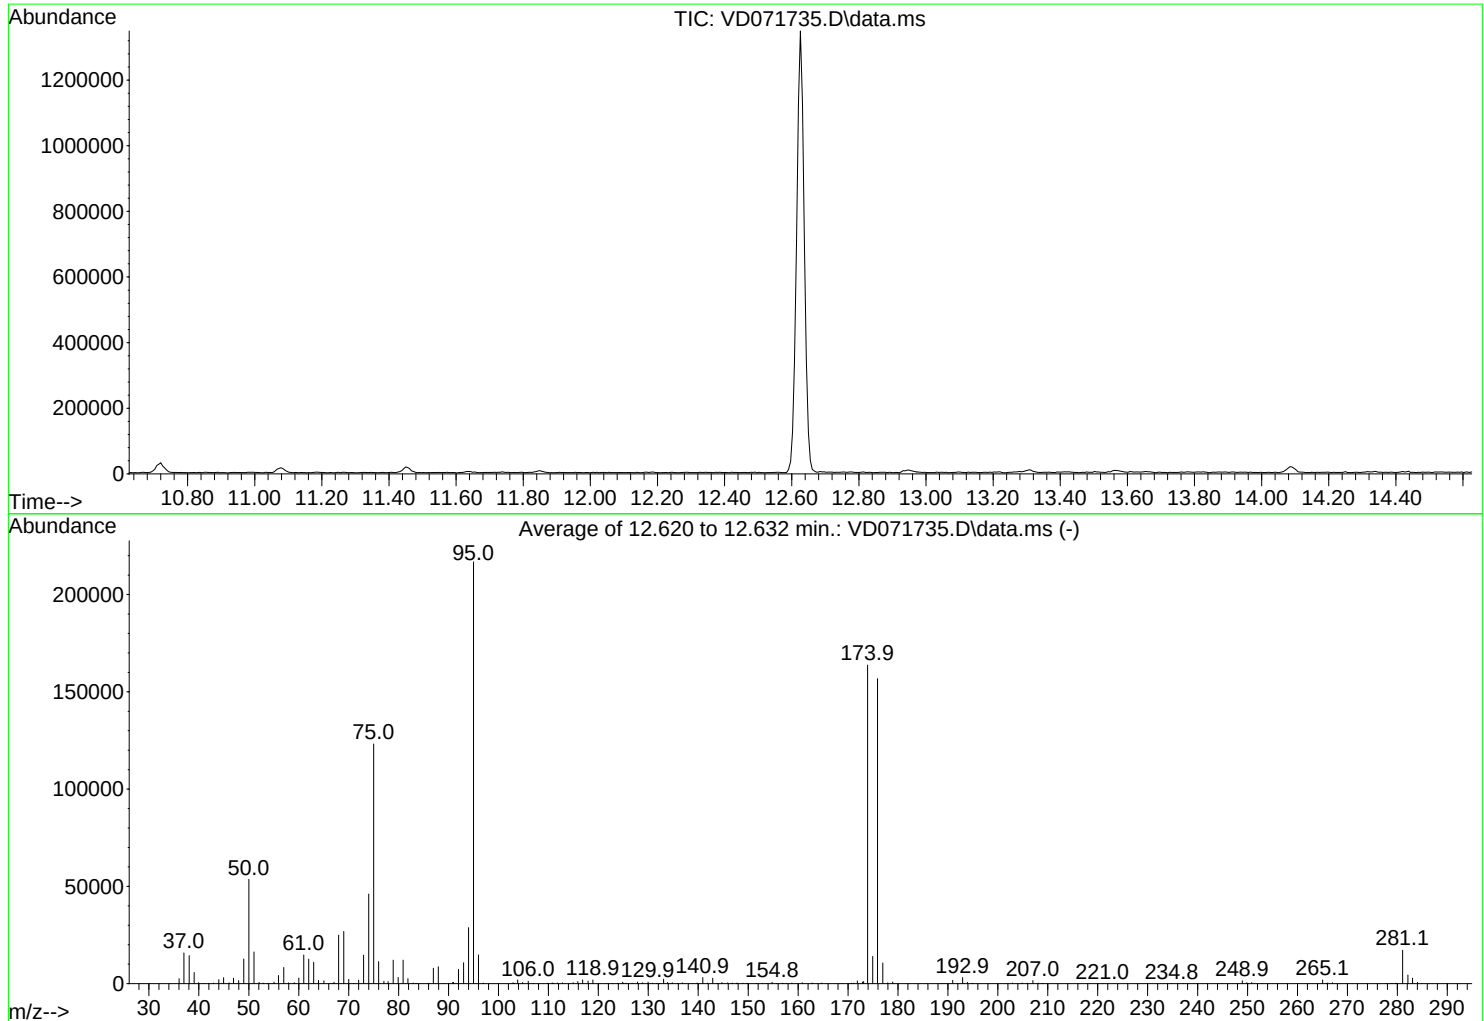

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	53619	PASS
75	95	30	60	56.8	123213	PASS
95	95	100	100	100.0	216811	PASS
96	95	5	9	6.8	14797	PASS
173	174	0.00	2	0.7	1086	PASS
174	95	50	100	75.5	163733	PASS
175	174	5	9	8.5	13995	PASS
176	174	95	101	95.7	156736	PASS
177	176	5	9	6.8	10623	PASS