
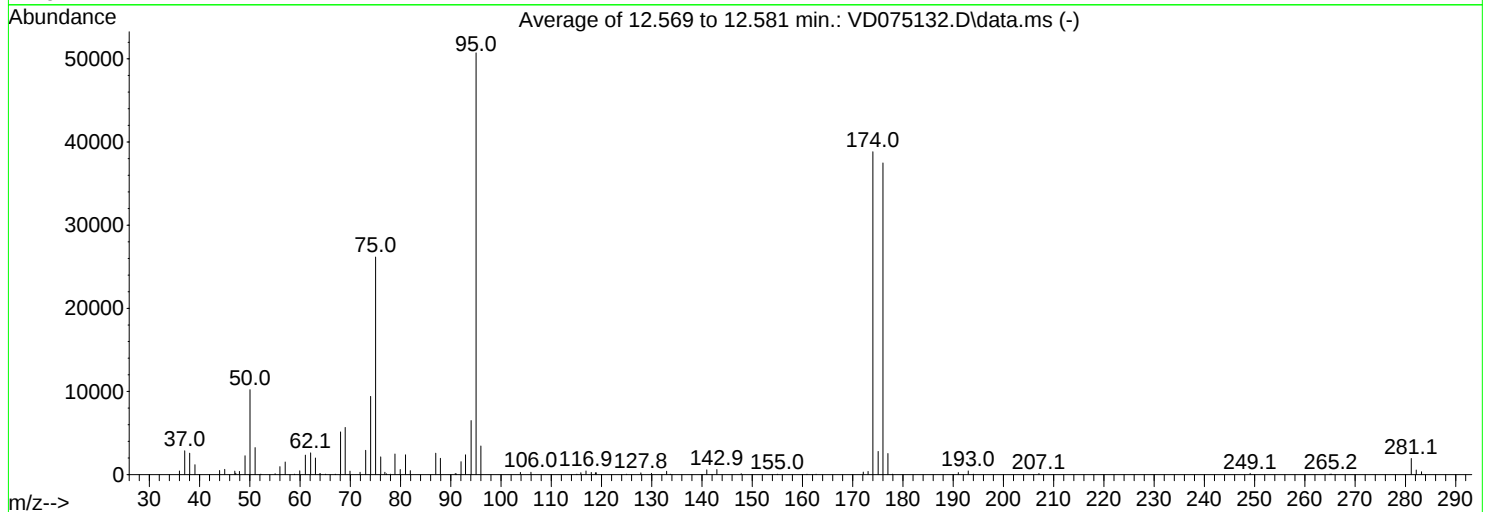


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011923\
Data File : VD075132.D
Acq On : 19 Jan 2023 10:19
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011823S.M
Title : SW846 8260
Last Update : Thu Jan 19 01:32:27 2023

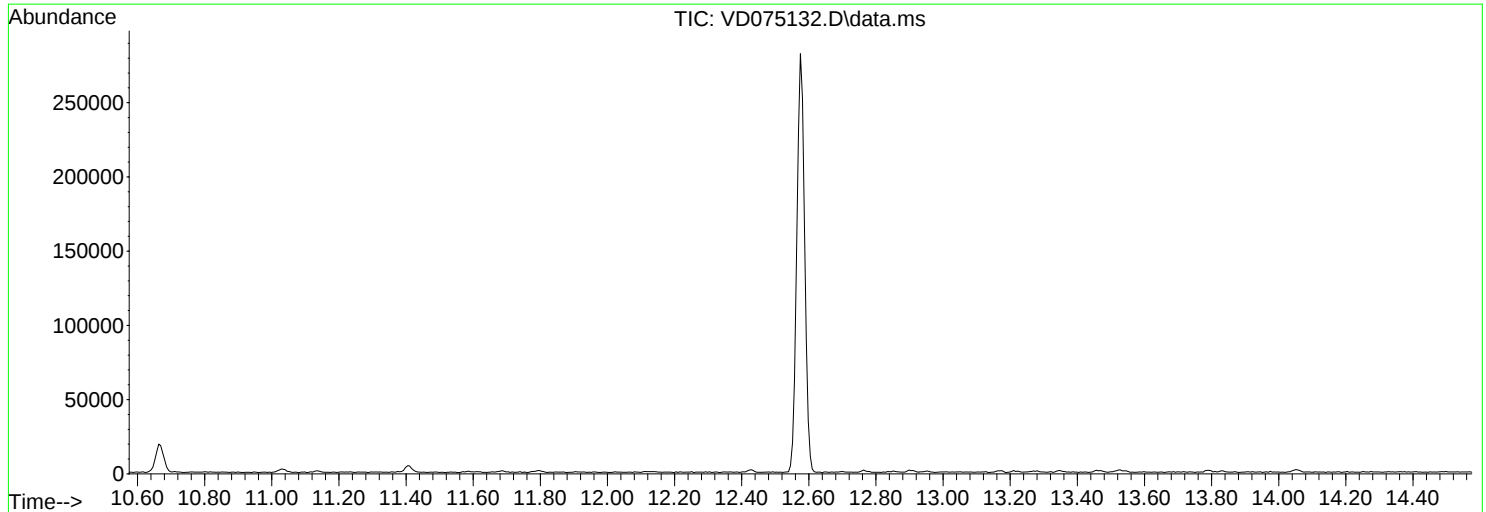

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	10210	PASS
75	95	30	60	51.6	26165	PASS
95	95	100	100	100.0	50725	PASS
96	95	5	9	6.8	3437	PASS
173	174	0.00	2	1.0	380	PASS
174	95	50	100	76.6	38832	PASS
175	174	5	9	7.2	2793	PASS
176	174	95	101	96.5	37477	PASS
177	176	5	9	6.8	2538	PASS