


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD012120\
Data File : VD064900.D
Acq On : 21 Jan 2020 08:40
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Title : SW846 8260
Last Update : Tue Dec 24 13:19:06 2019

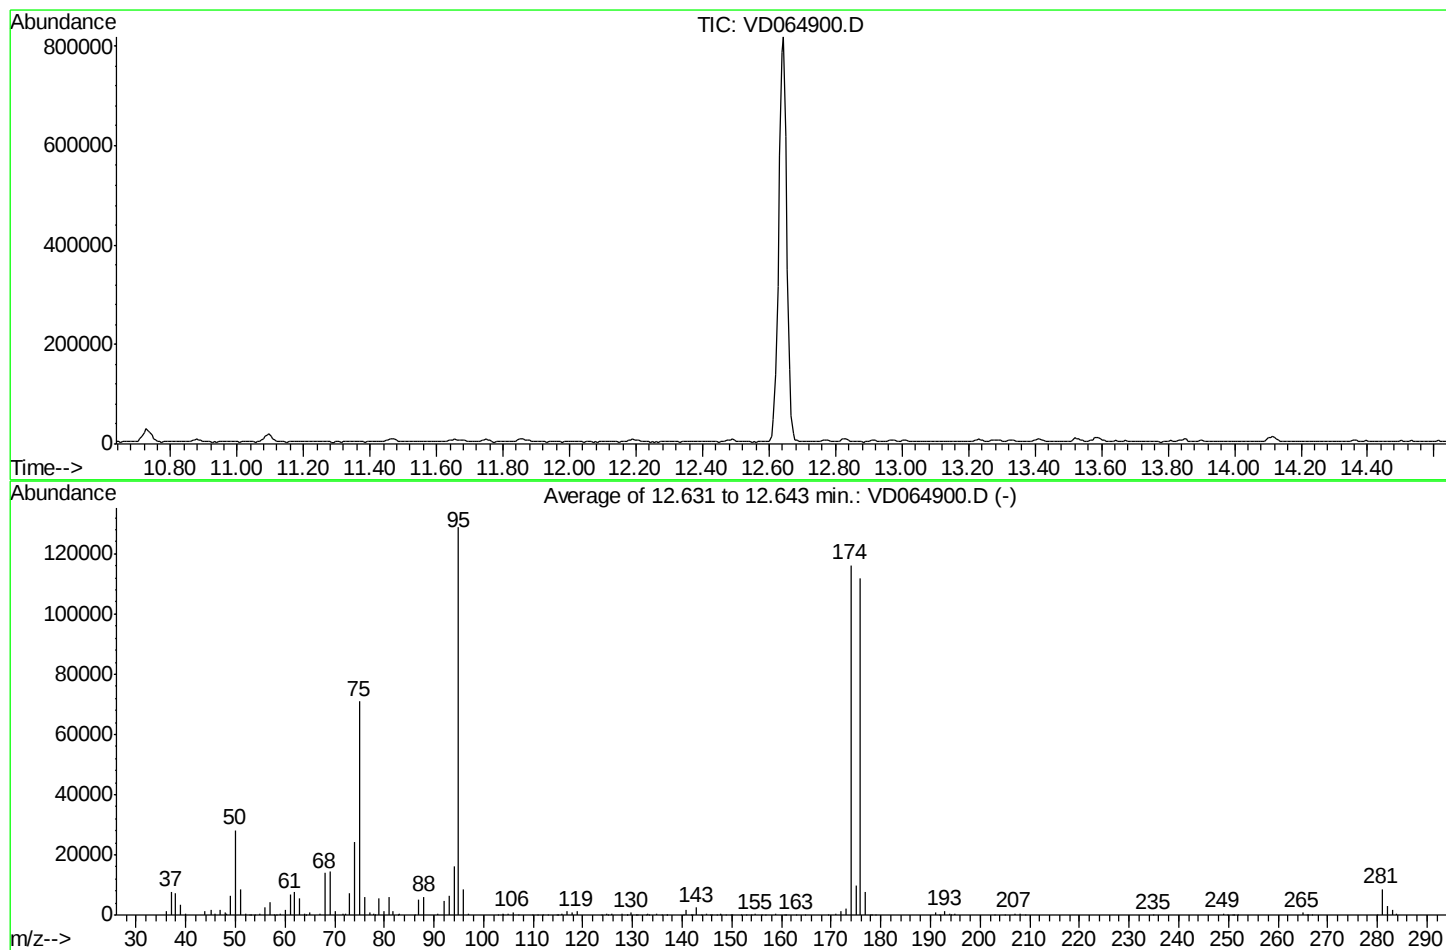

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	28226	PASS
75	95	30	60	55.1	70917	PASS
95	95	100	100	100.0	128797	PASS
96	95	5	9	6.7	8691	PASS
173	174	0.00	2	1.8	2071	PASS
174	95	50	100	90.2	116221	PASS
175	174	5	9	8.3	9665	PASS
176	174	95	101	96.4	112000	PASS
177	176	5	9	7.0	7865	PASS