
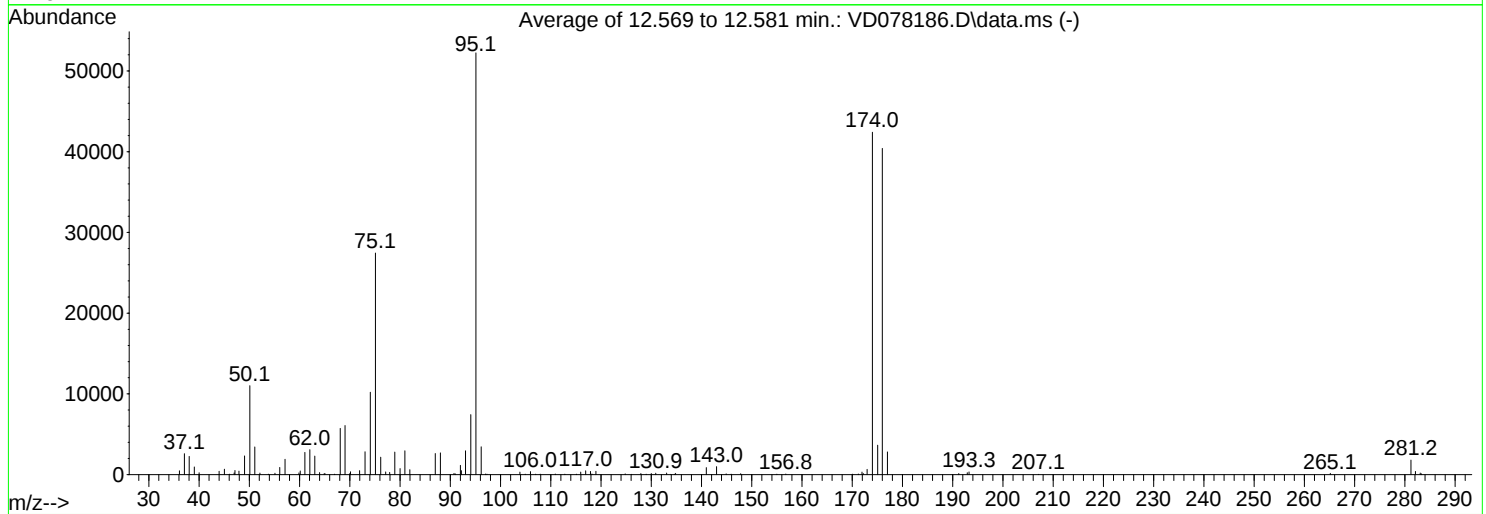


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012224\
Data File : VD078186.D
Acq On : 22 Jan 2024 09:29
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D012224S.M
Title : SW846 8260
Last Update : Tue Jan 23 05:43:07 2024

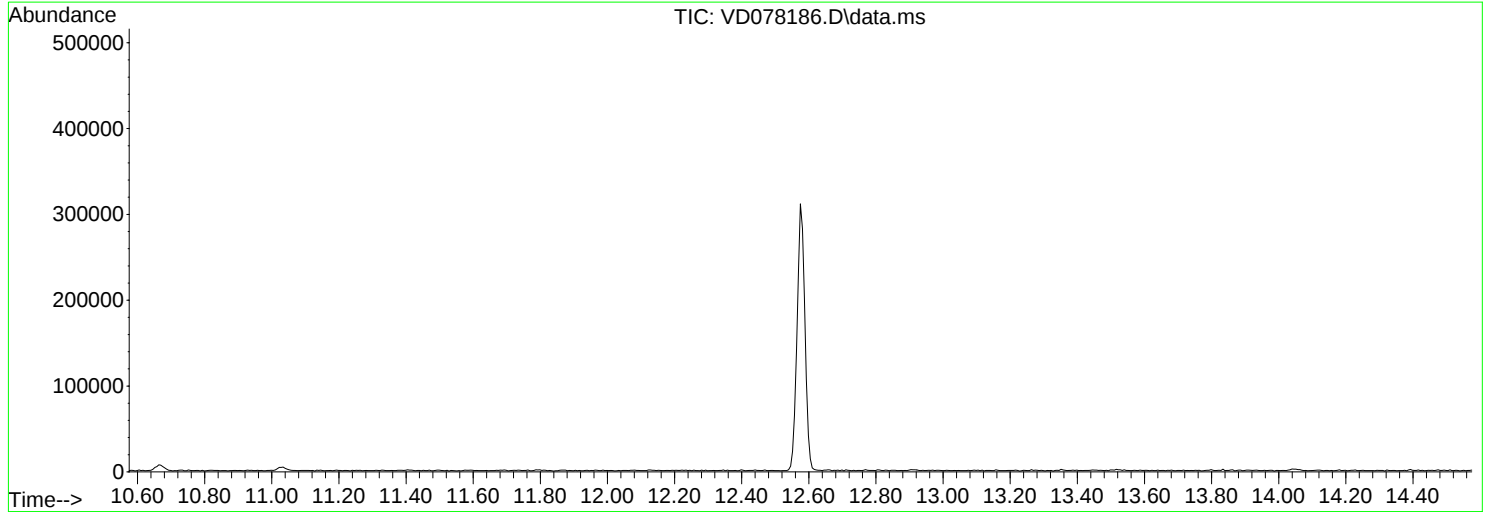

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	11013	PASS
75	95	30	60	52.5	27443	PASS
95	95	100	100	100.0	52243	PASS
96	95	5	9	6.6	3448	PASS
173	174	0.00	2	1.5	653	PASS
174	95	50	100	81.2	42403	PASS
175	174	5	9	8.6	3640	PASS
176	174	95	101	95.3	40416	PASS
177	176	5	9	7.0	2822	PASS